

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122619\
 Data File : BN009172.D
 Acq On : 26 Dec 2019 11:01
 Operator : JU
 Sample : PB125717BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK17

Quant Time: Dec 26 11:55:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 01:06:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	214472	20.00	ng/ul	0.00
18) Naphthalene-d8	10.28	136	1016716	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.15	164	693318	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	1539215	20.00	ng/ul	0.00
77) Chrysene-d12	21.11	240	1615249	20.00	ng/ul	0.00
85) Perylene-d12	23.25	264	1819215	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	31785	6.77	ng/uL	0.00
5) Phenol-d5	6.71	99	640618	31.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	447380	34.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	488321	33.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	535501	32.53	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	261422	34.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	294640	34.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	509167	31.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	651280	33.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.57	166	1861769	35.75	ng/ul	0.00
46) Acenaphthylene-d8	13.84	160	2180464	35.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.37	143	340815	32.92	ng/ul	0.00
57) Fluorene-d10	15.15	176	1632568	36.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.28	200	266810	27.78	ng/ul	0.00
70) Anthracene-d10	17.00	188	2616658	36.55	ng/ul	0.00
78) Pyrene-d10	19.30	212	3018294	35.82	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.12	264	3428186	37.40	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.23	70	15471	1.106 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122619\
Data File : BN009172.D
Acq On : 26 Dec 2019 11:01
Operator : JU
Sample : PB125717BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK17

Quant Time: Dec 26 11:55:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 01:06:45 2019
Response via : Initial Calibration

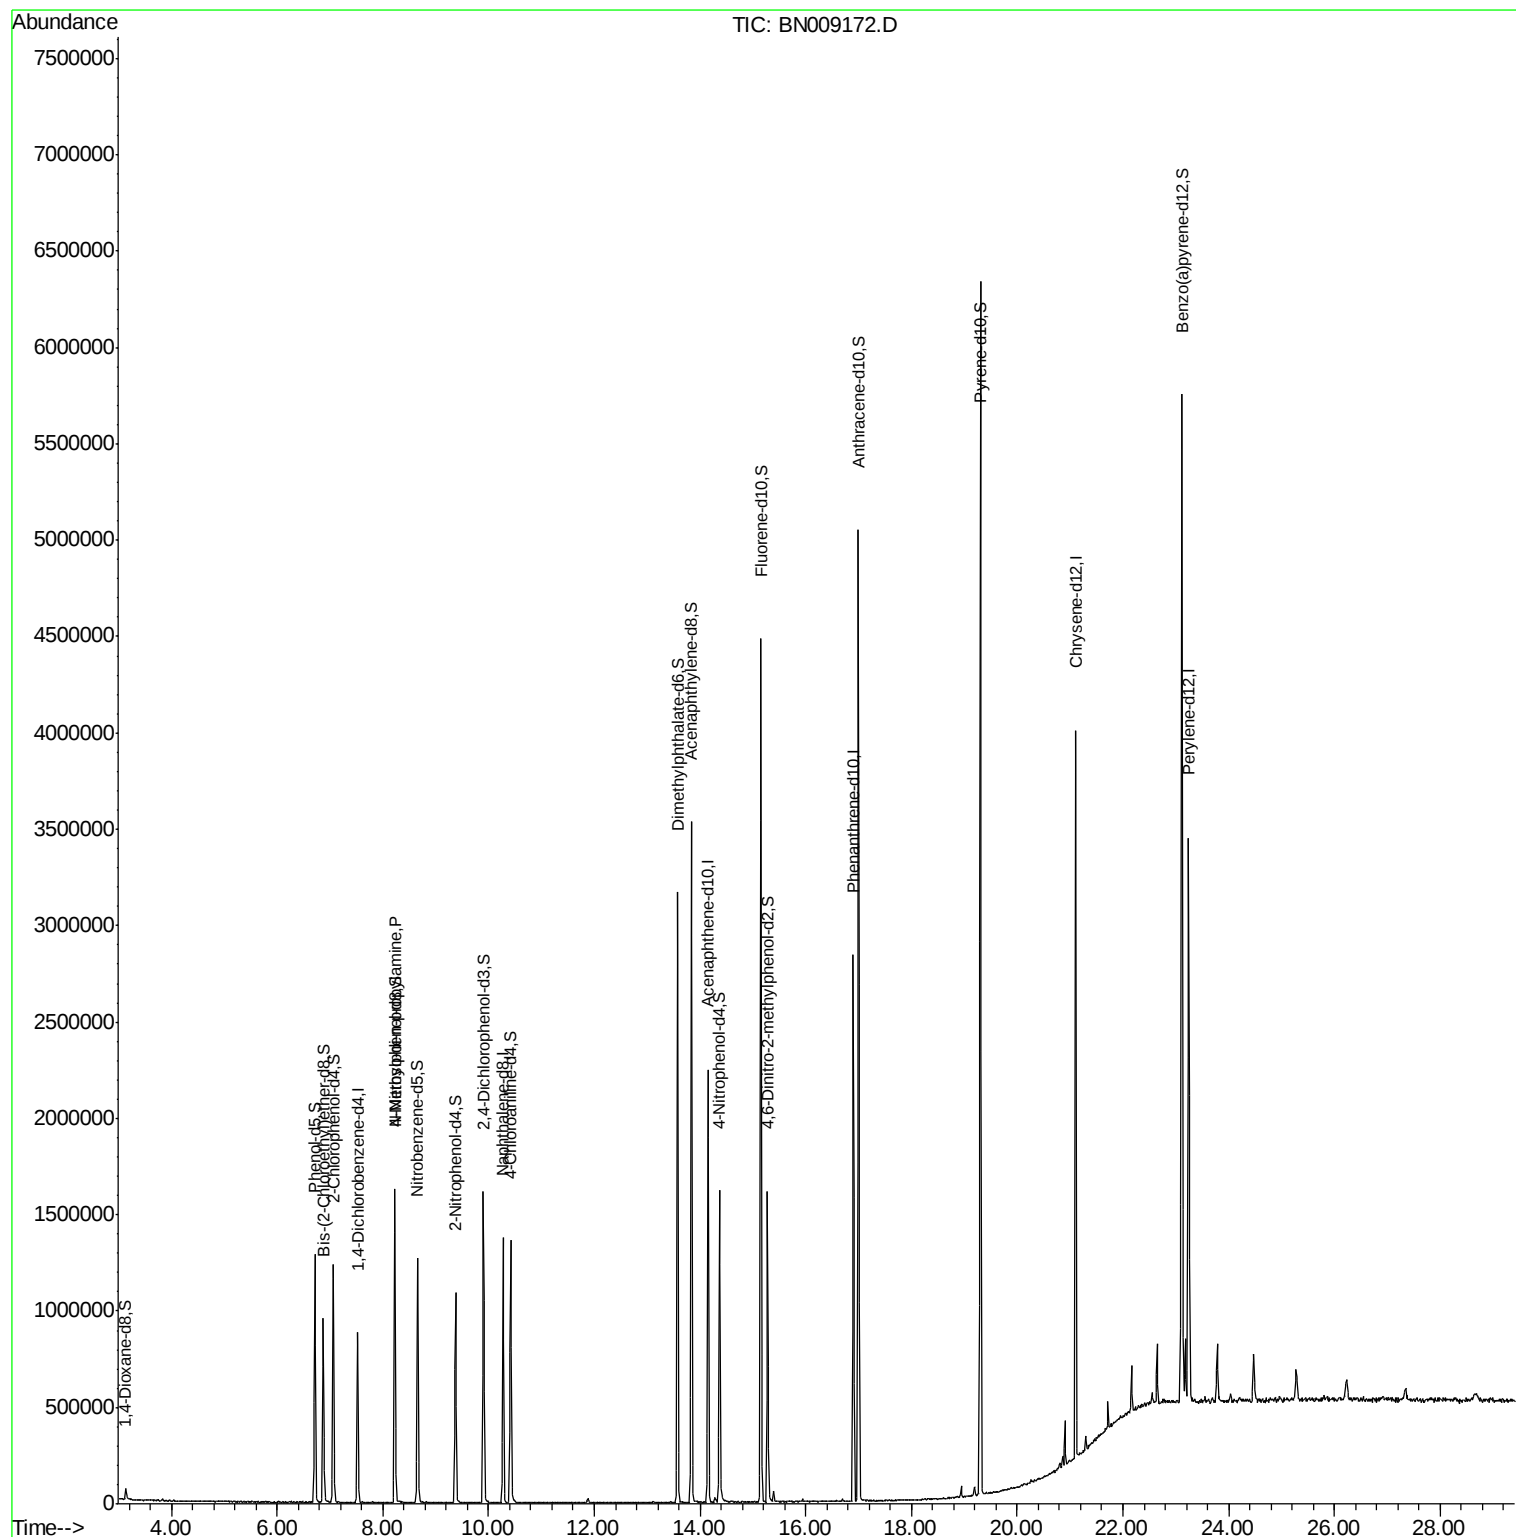

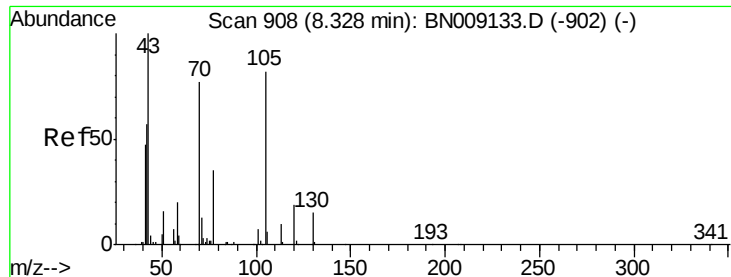

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.106 ng/ul
 RT: 8.23 min Scan# 891
 Delta R.T. -0.10 min
 Lab File: BN009172.D
 Acq: 26 Dec 2019 11:01

Instrument :
 BNA_N
 ClientSampleId :
 SBLK17

Tot Ion: 70 Resp: 15471
 Ion Ratio Lower Upper
 70 100
 42 432.6 60.4 90.6#
 101 0.0 7.4 11.0#
 130 0.0 15.8 23.8#

