

Data File : BN009179.D
Acq On : 26 Dec 2019 19:04
Operator : JU
Sample : K6381-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB5R3

Quant Time: Dec 27 01:33:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 27 01:30:55 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	303763	20.00	ng/ul	0.00
18) Naphthalene-d8	10.27	136	1391126	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.15	164	891658	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	1861758	20.00	ng/ul	0.00
77) Chrysene-d12	21.11	240	1537217	20.00	ng/ul	0.00
85) Perylene-d12	23.24	264	1374318	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	33814	5.09	ng/uL	0.00
5) Phenol-d5	6.72	99	805653	27.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	539056	29.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	616877	29.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	672126	28.83	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	324220	30.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.37	143	371449	31.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	647082	29.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	899478	33.81	ng/ul	0.00
43) Dimethylphthalate-d6	13.57	166	1932652	28.86	ng/ul	0.00
46) Acenaphthylene-d8	13.84	160	2453289	31.25	ng/ul	0.00
51) 4-Nitrophenol-d4	14.37	143	358954	26.96	ng/ul	0.00
57) Fluorene-d10	15.15	176	1756745	30.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.29	200	227752	19.61	ng/ul	0.00
70) Anthracene-d10	17.00	188	2630628	30.38	ng/ul	0.00
78) Pyrene-d10	19.30	212	2851900	35.56	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.12	264	2167649	31.30	ng/ul	0.00

Target Compounds


					Qvalue
69) Phenanthrene	16.94	178	446464	4.349 ng/ul	99
76) Fluoranthene	18.97	202	768607	6.483 ng/ul	98
79) Pyrene	19.33	202	669007	6.275 ng/ul	100
82) Benzo(a)anthracene	21.09	228	330922	3.186 ng/ul	95
84) Chrysene	21.14	228	323028	3.236 ng/ul	99
87) Benzo(b)fluoranthene	22.62	252	350236	4.170 ng/ul	96
88) Benzo(k)fluoranthene	22.62	252	350236	4.270 ng/ul	96
90) Benzo(a)pyrene	23.16	252	200810	2.604 ng/ul#	95
91) Indeno(1,2,3-cd)pyrene	25.34	276	111593	1.194 ng/ul#	92
93) Benzo(g,h,i)perylene	25.97	276	110675	1.416 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009179.D
Acq On : 26 Dec 2019 19:04
Operator : JU
Sample : K6381-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB5R3

Quant Time: Dec 27 01:33:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 27 01:30:55 2019
Response via : Initial Calibration

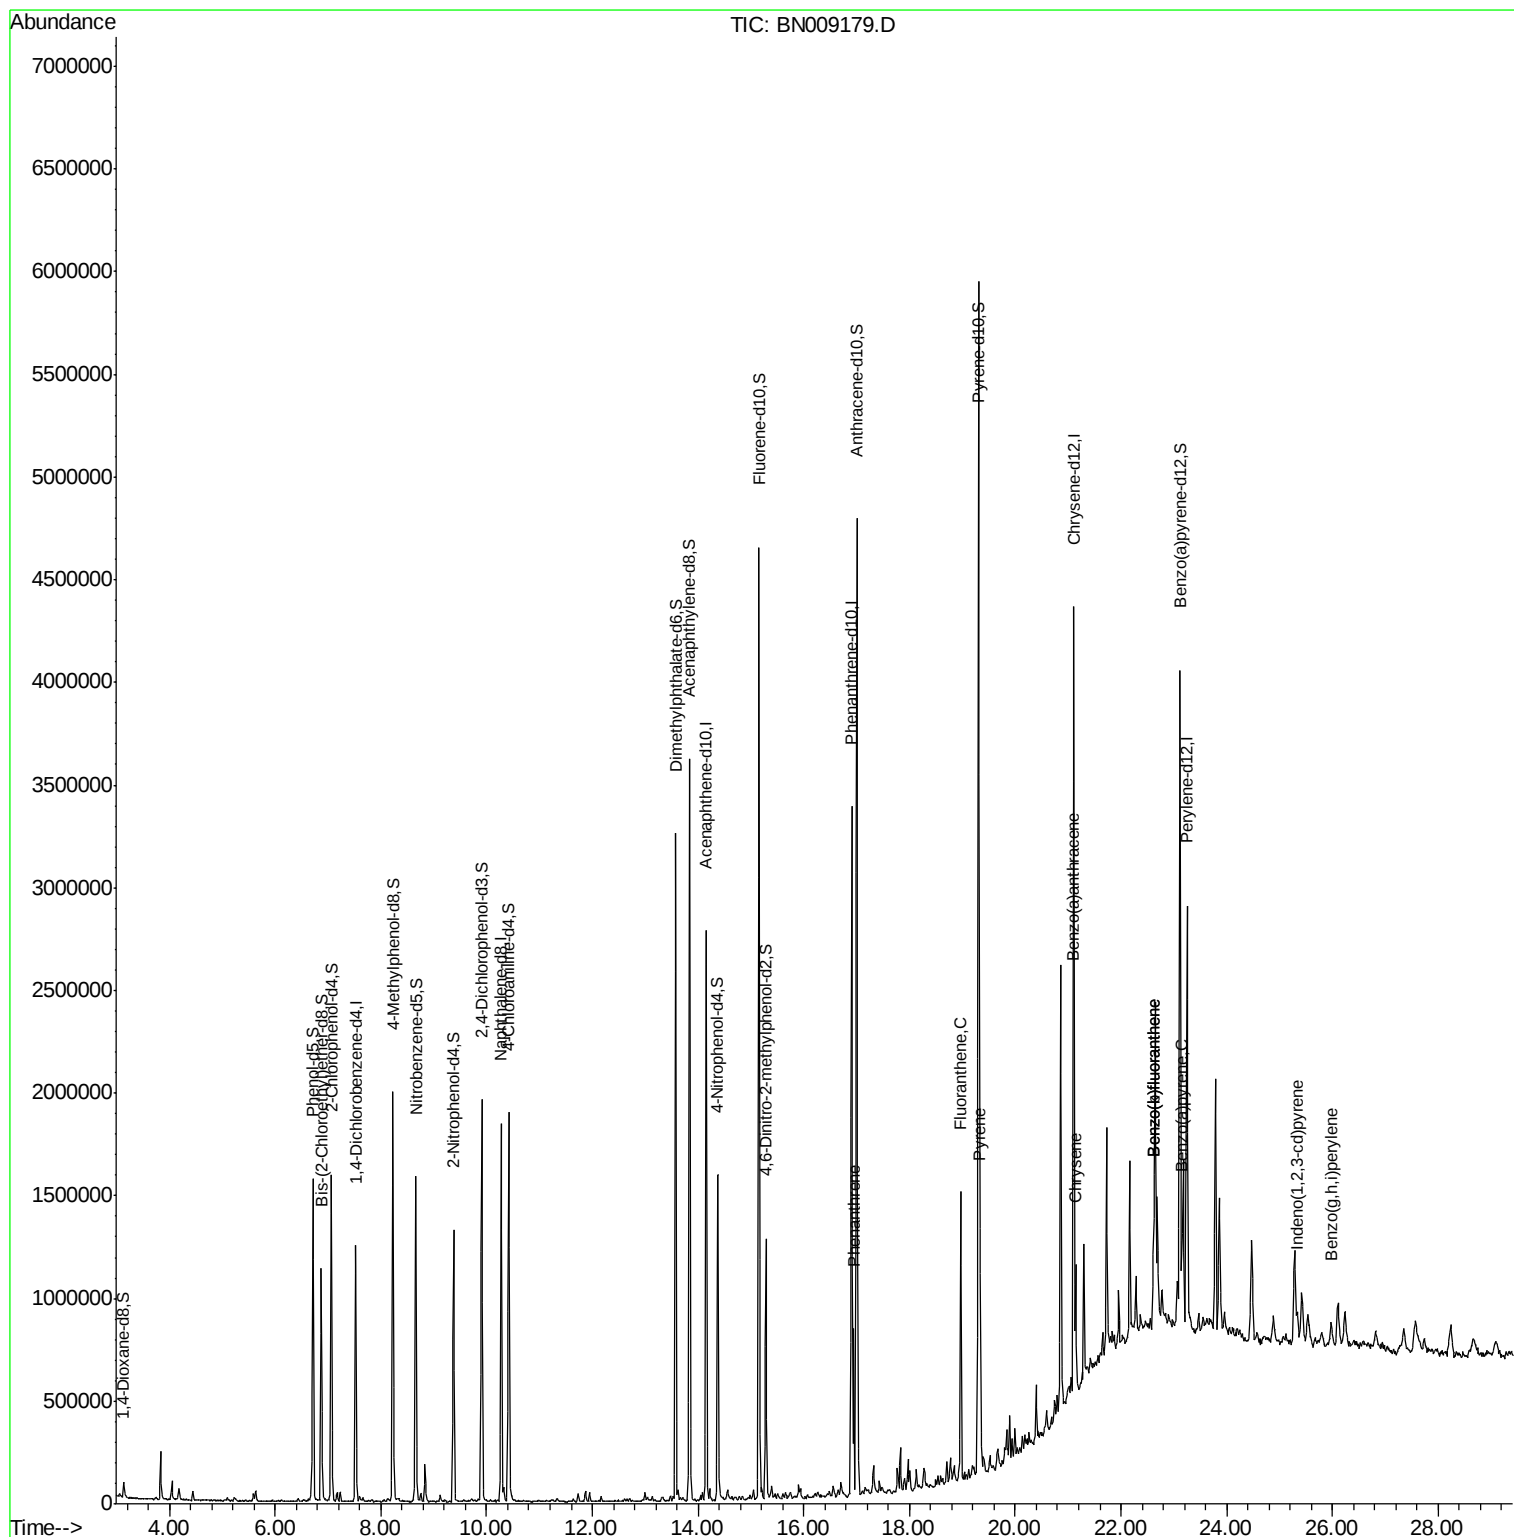

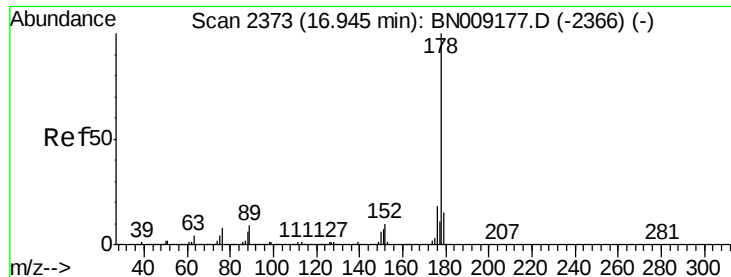

#69

Phenanthrene

Concen: 4.349 ng/ul

RT: 16.94 min Scan# 2373

Delta R.T. -0.00 min

Lab File: BN009179.D

Acq: 26 Dec 2019 19:04

Instrument :

BNA_N

ClientSampleId :

CB5R3


Tgt Ion:178 Resp: 446464

Ion Ratio Lower Upper

178 100

179 14.3 11.8 17.8




176 18.9 15.2 22.8

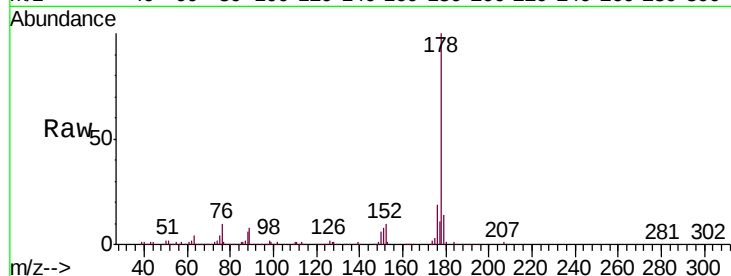

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

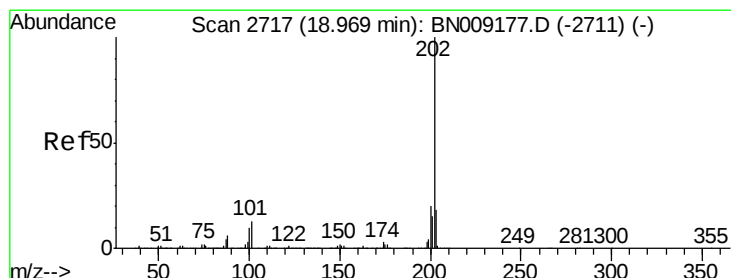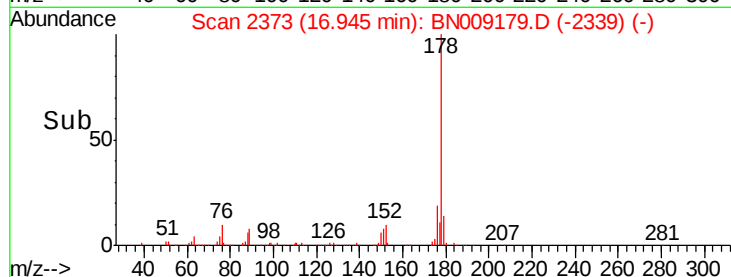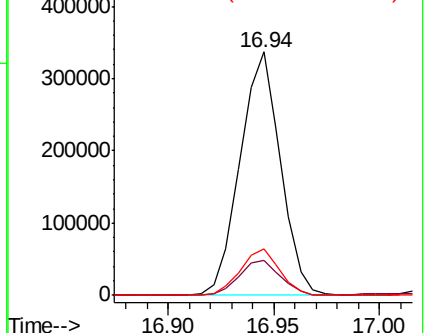

#76

Fluoranthene

Concen: 6.483 ng/ul

RT: 18.97 min Scan# 2717

Delta R.T. -0.00 min

Lab File: BN009179.D

Acq: 26 Dec 2019 19:04


Tgt Ion:202 Resp: 768607

Ion Ratio Lower Upper

202 100

101 12.5 9.3 13.9



100 9.8 7.6 11.4

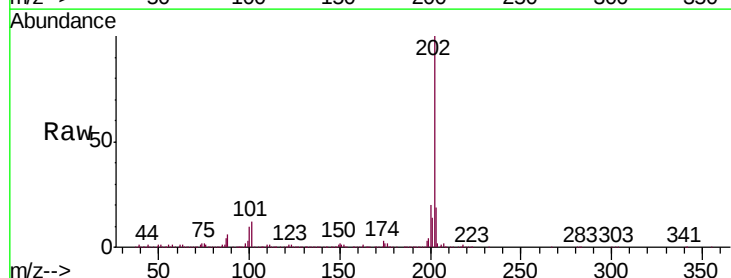


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



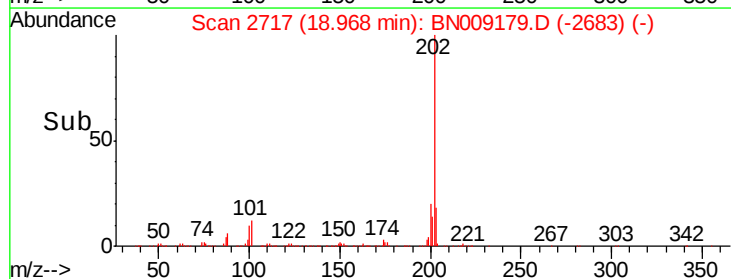
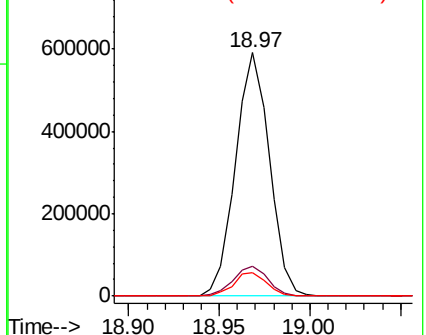


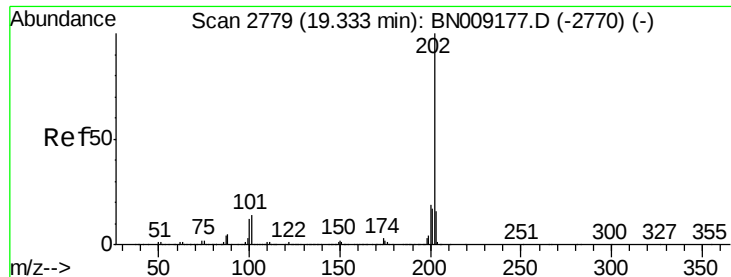

#79
 Pyrene
 Concen: 6.275 ng/ul
 RT: 19.33 min Scan# 2779
 Delta R.T. -0.00 min
 Lab File: BN009179.D
 Acq: 26 Dec 2019 19:04




Instrument :
 BNA_N
 ClientSampleId :
 CB5R3


Tgt Ion:	202	Resp:	669007
Ion	Ratio	Lower	Upper
202	100		
101	13.6	11.1	16.7
100	11.2	9.0	13.4

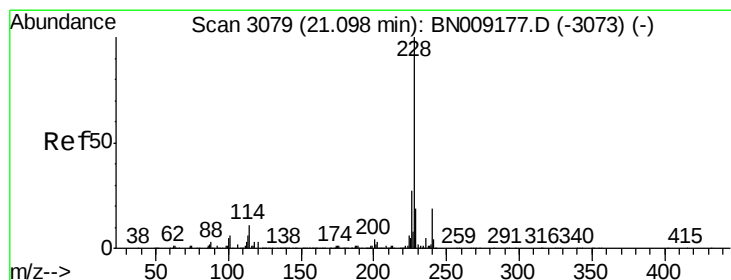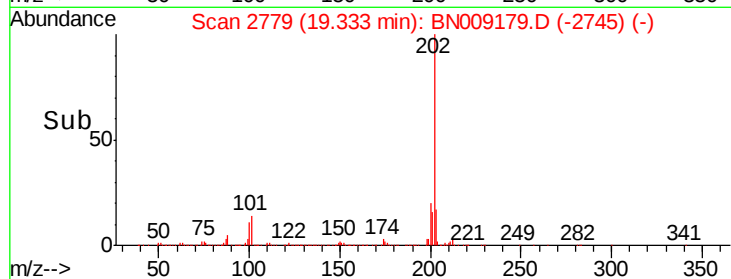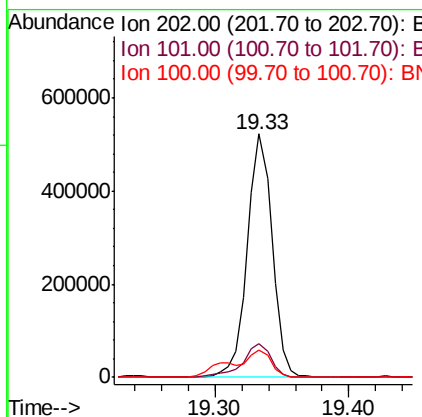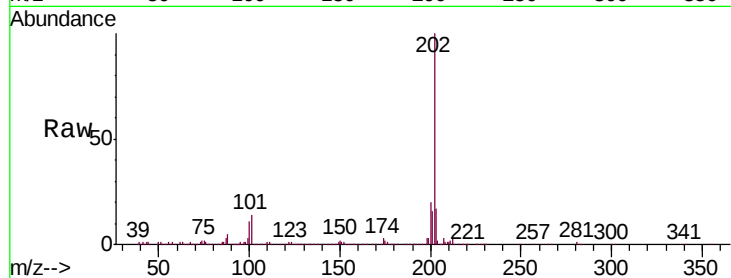

#82
 Benzo(a)anthracene
 Concen: 3.186 ng/ul
 RT: 21.09 min Scan# 3078
 Delta R.T. -0.01 min
 Lab File: BN009179.D
 Acq: 26 Dec 2019 19:04

Tgt Ion:	228	Resp:	330922
Ion	Ratio	Lower	Upper
228	100		
229	20.9	15.2	22.8
226	27.9	19.8	29.6

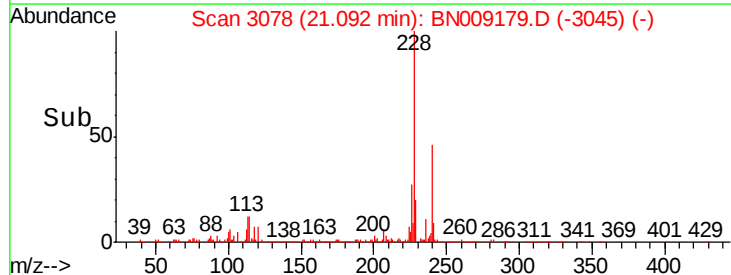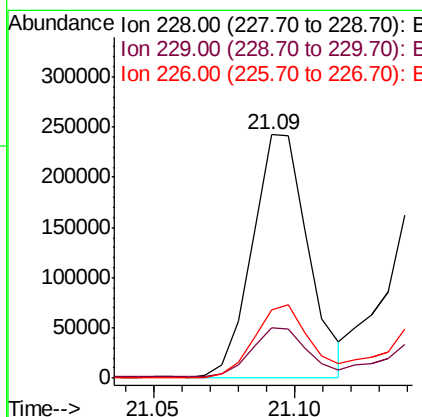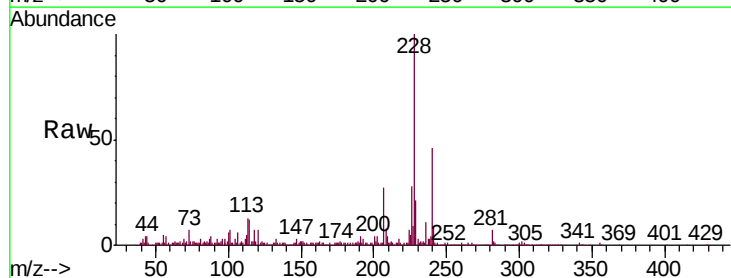

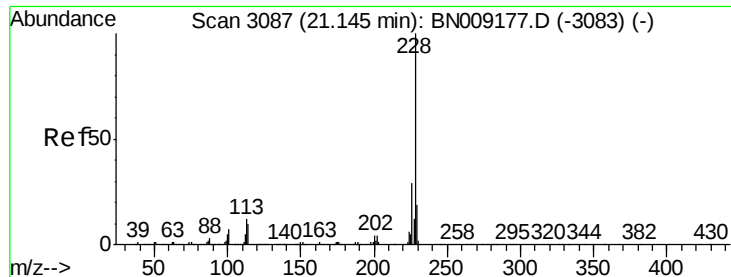

#84

Chrysene

Concen: 3.236 ng/u1

RT: 21.14 min Scan# 3087

Delta R.T. -0.00 min

Lab File: BN009179.D

Acq: 26 Dec 2019 19:04

Instrument :

BNA_N

ClientSampleId :

CB5R3


Tgt Ion:228 Resp: 323028

Ion Ratio Lower Upper

228 100

226 29.4 23.9 35.9




229 20.4 15.9 23.9

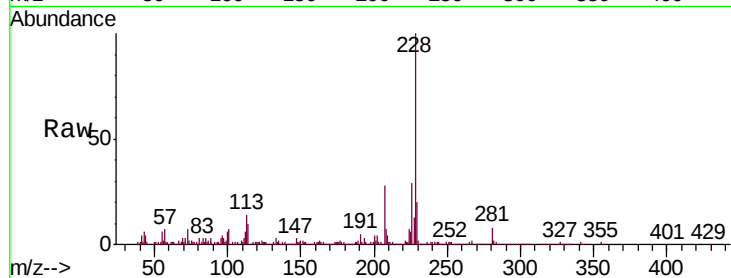

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

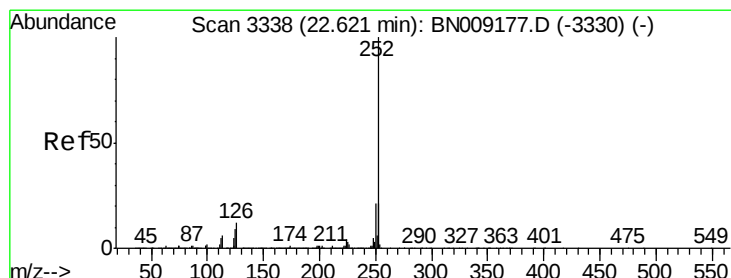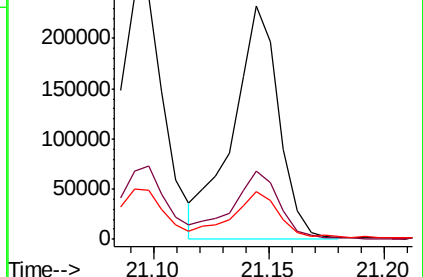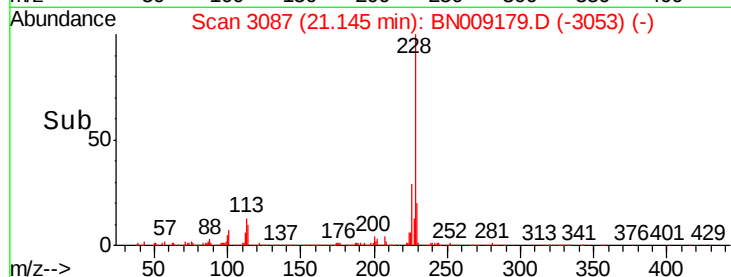

#87

Benzo(b)fluoranthene

Concen: 4.170 ng/u1

RT: 22.62 min Scan# 3338

Delta R.T. -0.00 min

Lab File: BN009179.D

Acq: 26 Dec 2019 19:04


Tgt Ion:252 Resp: 350236

Ion Ratio Lower Upper

252 100

253 23.5 17.2 25.8



125 12.2 8.5 12.7

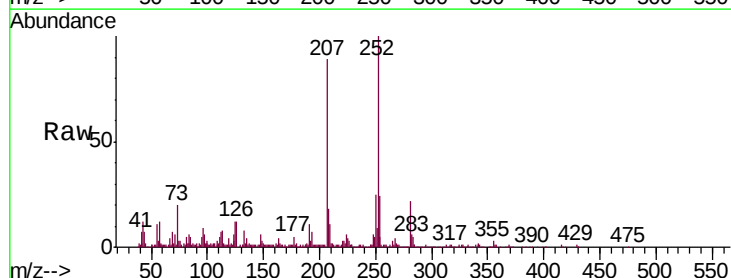


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

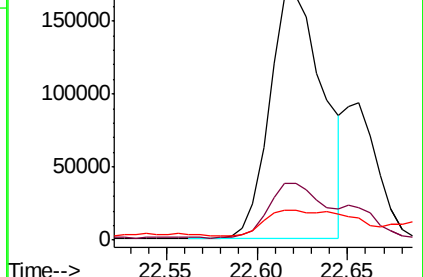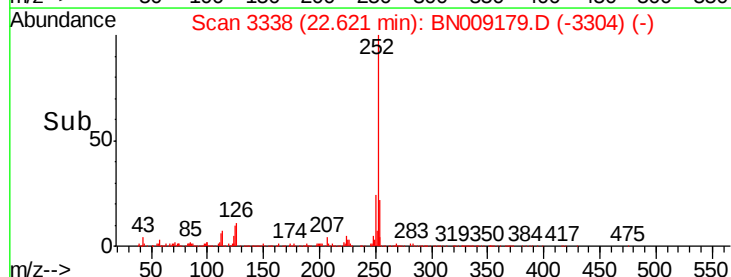

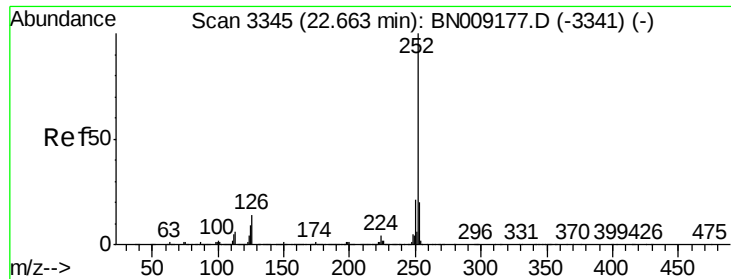

#88

Benzo(k)fluoranthene

Concen: 4.270 ng/ul

RT: 22.62 min Scan# 3338

Delta R.T. -0.04 min

Lab File: BN009179.D

Acq: 26 Dec 2019 19:04





Instrument :

BNA_N

ClientSampleId :

CB5R3

Tgt Ion:	252	Resp:	350236
Ion Ratio	Lower	Upper	
252	100		
253	23.5	17.4	26.0
125	12.2	8.8	13.2

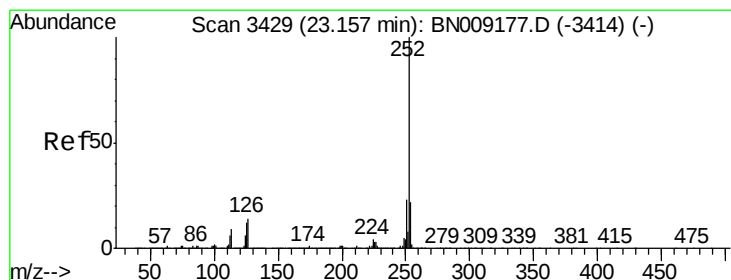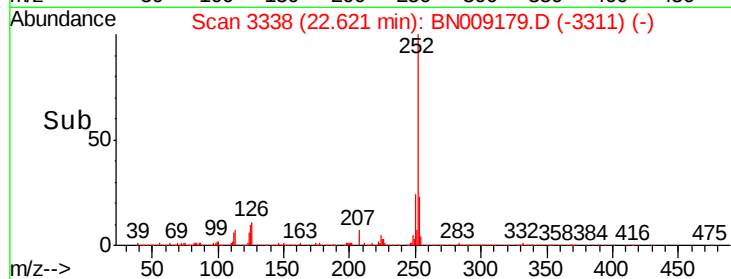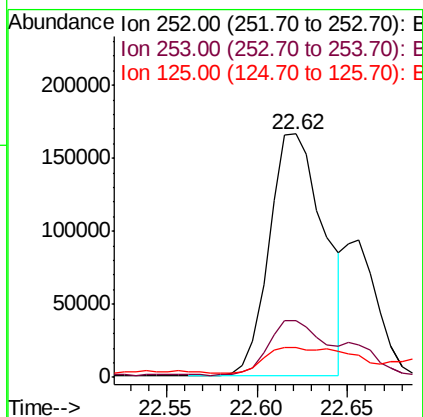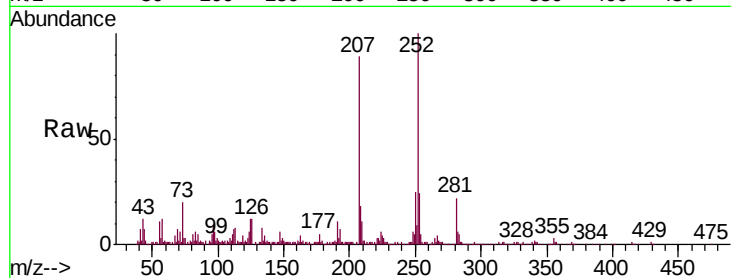

#90

Benzo(a)pyrene

Concen: 2.604 ng/ul




RT: 23.16 min Scan# 3429


Delta R.T. -0.00 min

Lab File: BN009179.D

Acq: 26 Dec 2019 19:04

Tgt Ion:	252	Resp:	200810
Ion Ratio	Lower	Upper	
252	100		
253	24.2	17.7	26.5
125	14.7	9.5	14.3#

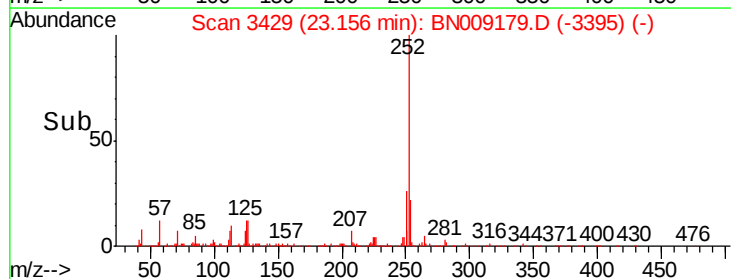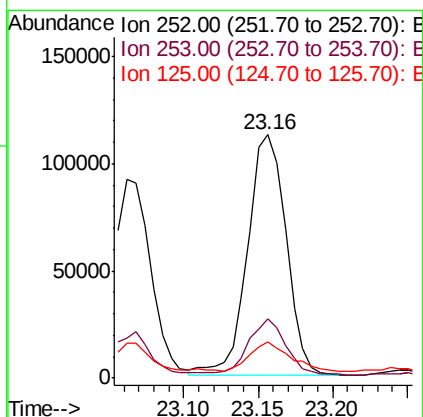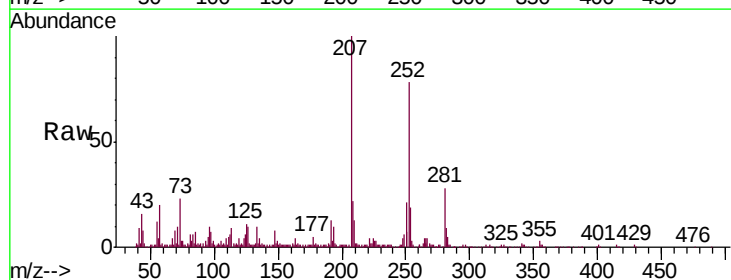

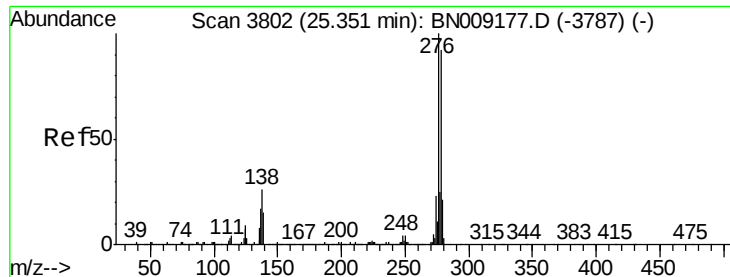

#91

Indeno(1,2,3-cd)pyrene

Concen: 1.194 ng/ul

RT: 25.34 min Scan# 3800

Delta R.T. -0.01 min

Lab File: BN009179.D

Acq: 26 Dec 2019 19:04

Instrument :

BNA_N

ClientSampleId :

CB5R3


Tgt Ion:276 Resp: 111593

Ion Ratio Lower Upper

276 100

138 19.3 20.5 30.7#




277 23.8 20.2 30.4

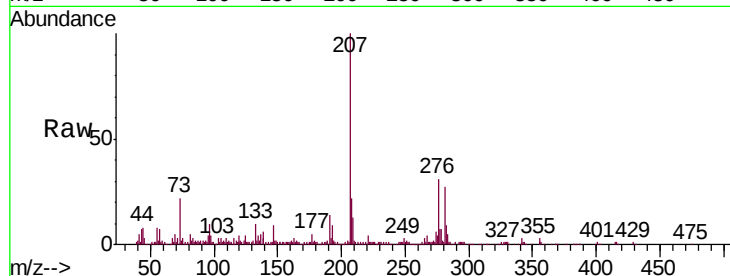

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

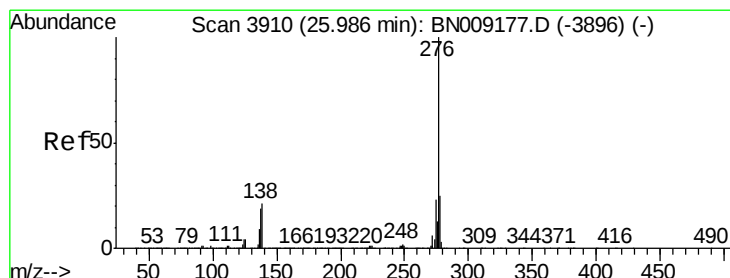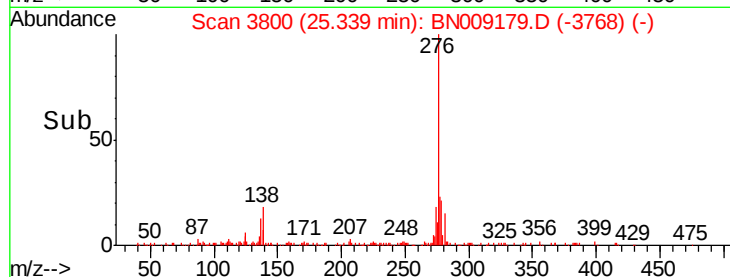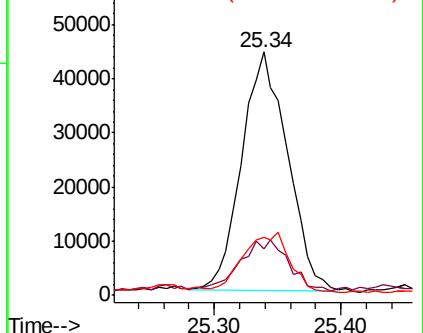

#93

Benzo(g,h,i)perylene

Concen: 1.416 ng/ul

RT: 25.97 min Scan# 3908

Delta R.T. -0.01 min

Lab File: BN009179.D

Acq: 26 Dec 2019 19:04


Tgt Ion:276 Resp: 110675

Ion Ratio Lower Upper

276 100

138 21.6 17.8 26.6

277 24.5 18.9 28.3

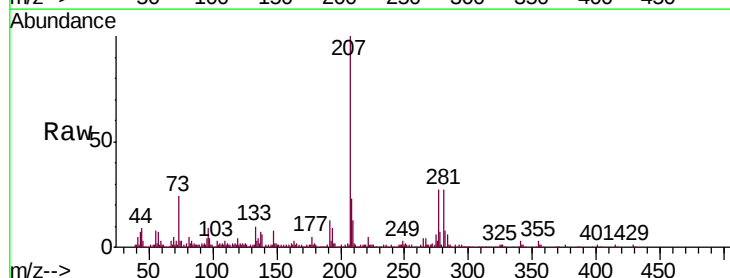

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

