
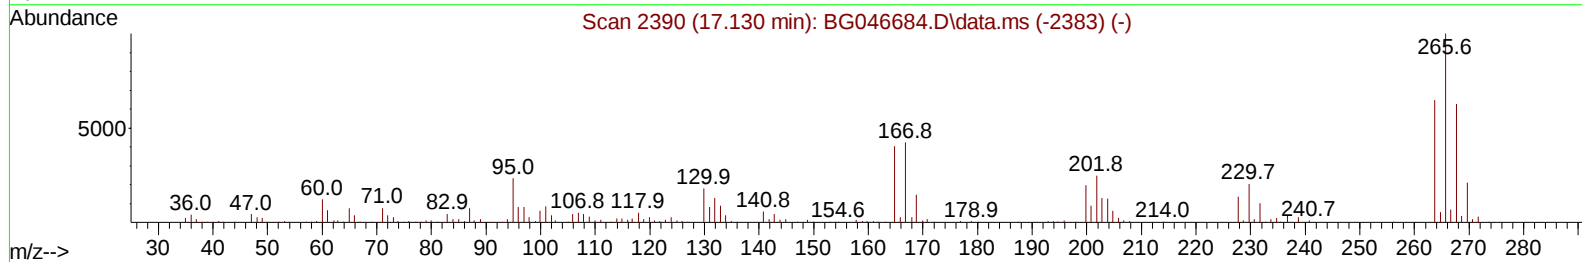
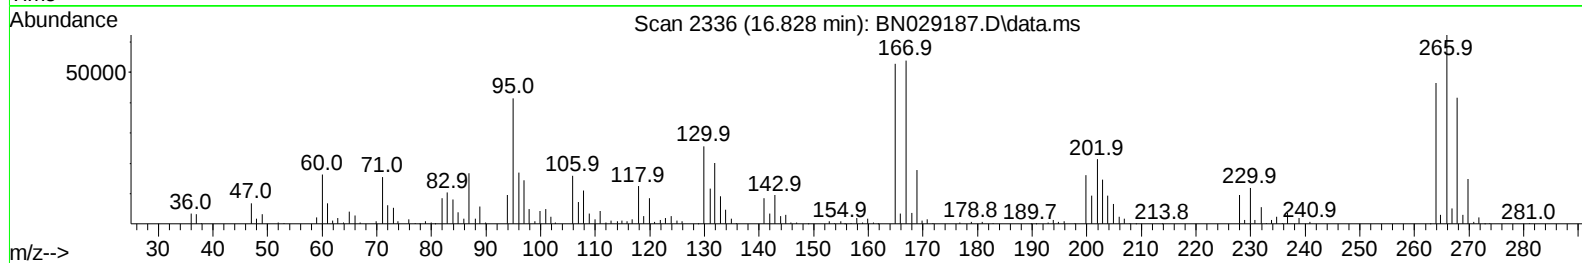


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122623\
Data File : BN029187.D
Acq On : 26 Dec 2023 10:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 01:51:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

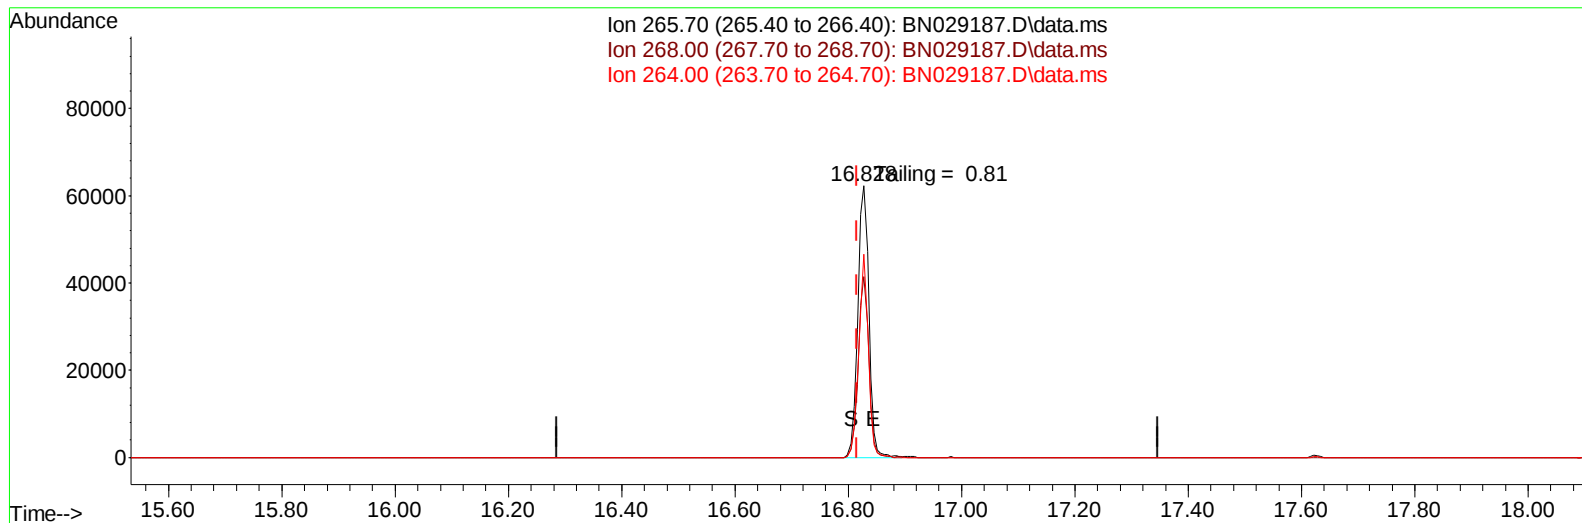

TIC: BN029187.D\data.ms

(70) Pentachlorophenol (C)




16.828min (+ 0.012) 16663.60 ng

response 84217

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.72
264.00	61.60	74.76#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122623\
Data File : BN029187.D
Acq On : 26 Dec 2023 10:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 01:51:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

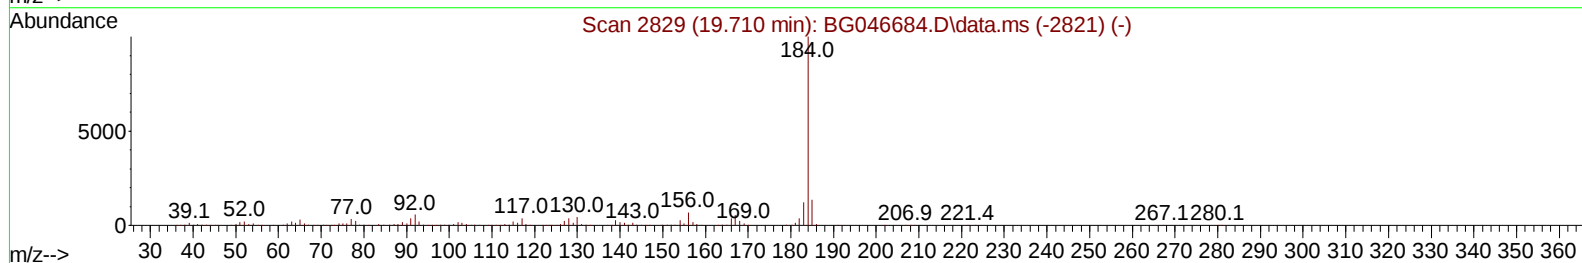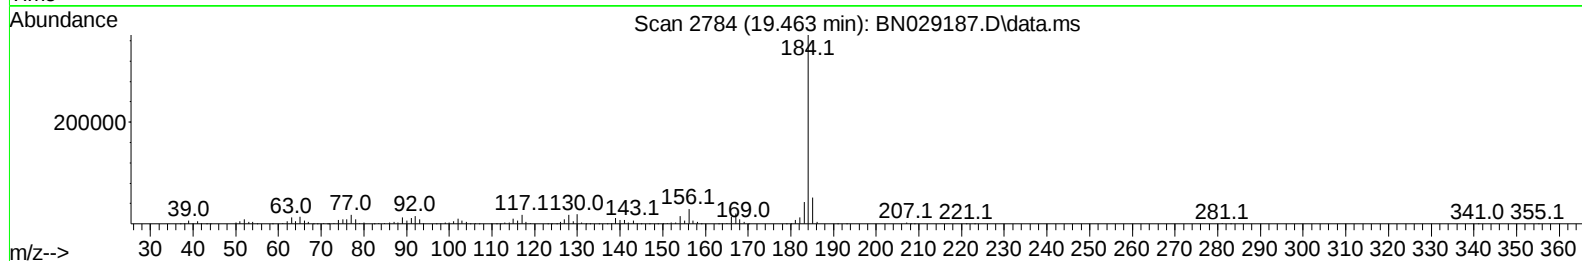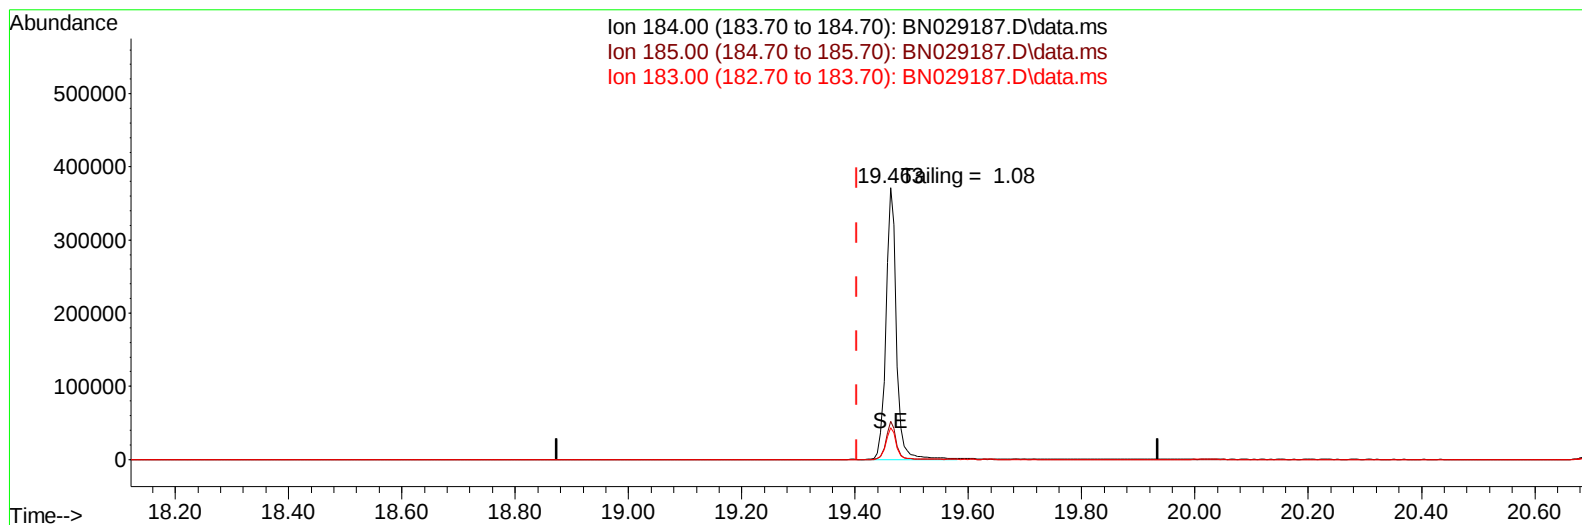

TIC: BN029187.D\data.ms

(77) Benzidine**19.463min (+ 0.059) 0.00 ng****response 478799**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	11.70
0.00	0.00	0.00