
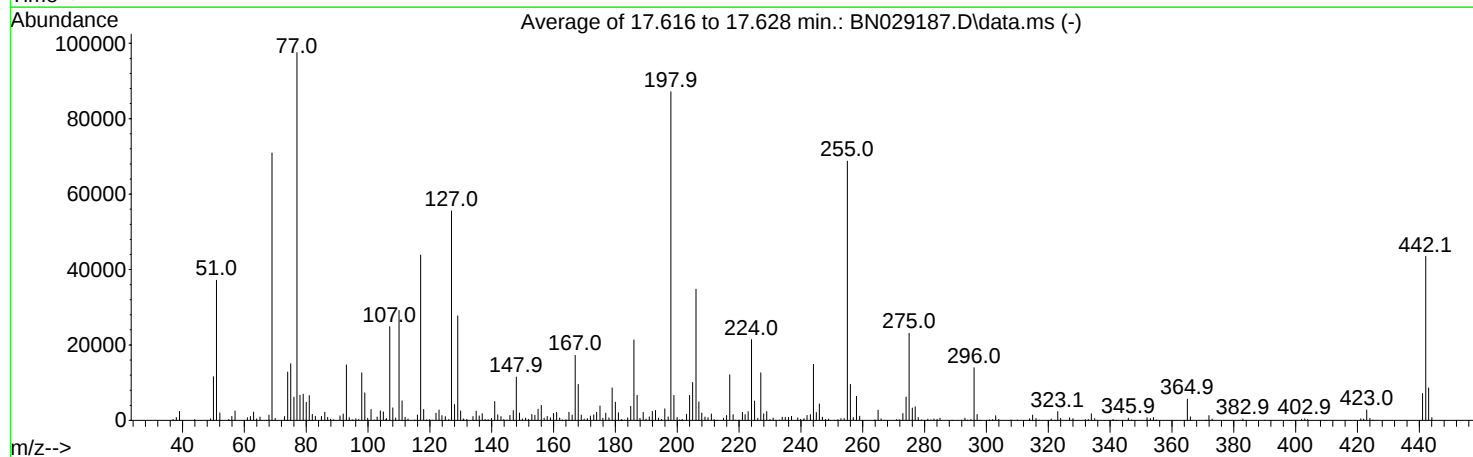


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122623\
Data File : BN029187.D
Acq On : 26 Dec 2023 10:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 27 01:26:11 2023

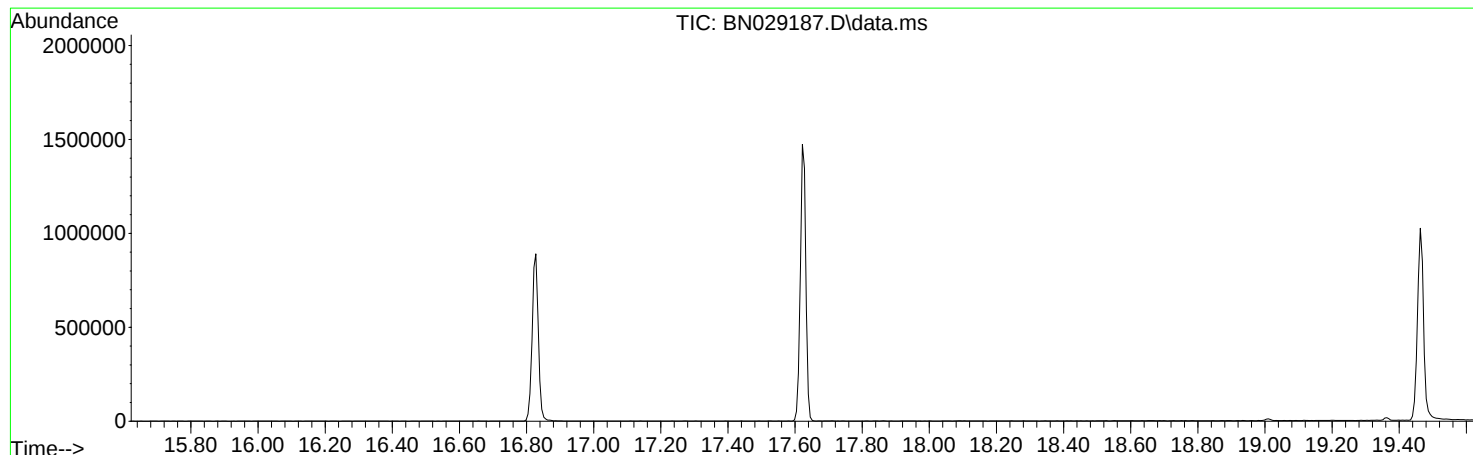




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	37187	PASS
68	69	0.00	2	2.0	1394	PASS
69	198	0.00	100	81.3	70891	PASS
70	69	0.00	2	0.7	520	PASS
127	198	10	80	63.7	55560	PASS
197	198	0.00	2	1.1	952	PASS
198	198	100	100	100.0	87176	PASS
199	198	5	9	7.6	6637	PASS
275	198	10	60	26.5	23101	PASS
365	198	1	100	6.5	5647	PASS
441	198	0.01	100	8.2	7117	PASS
442	442	50	100	100.0	43477	PASS
443	442	15	24	19.8	8600	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122623\
Data File : BN029187.D
Acq On : 26 Dec 2023 10:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 27 01:51:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

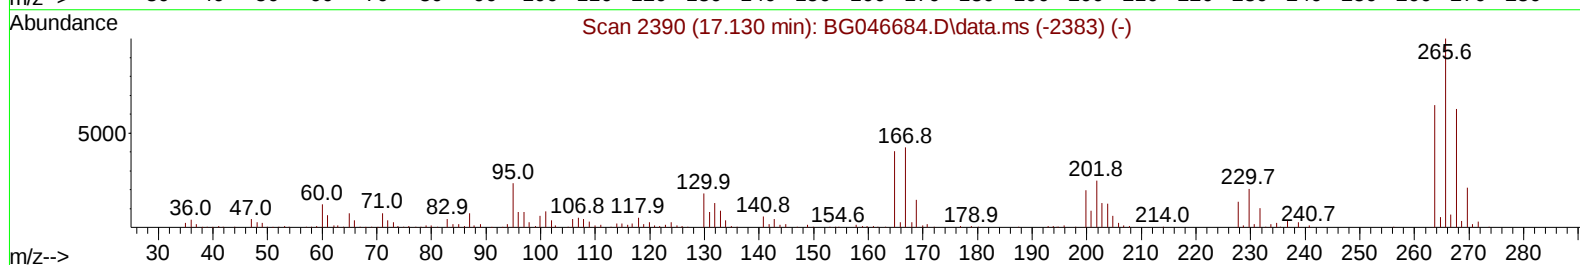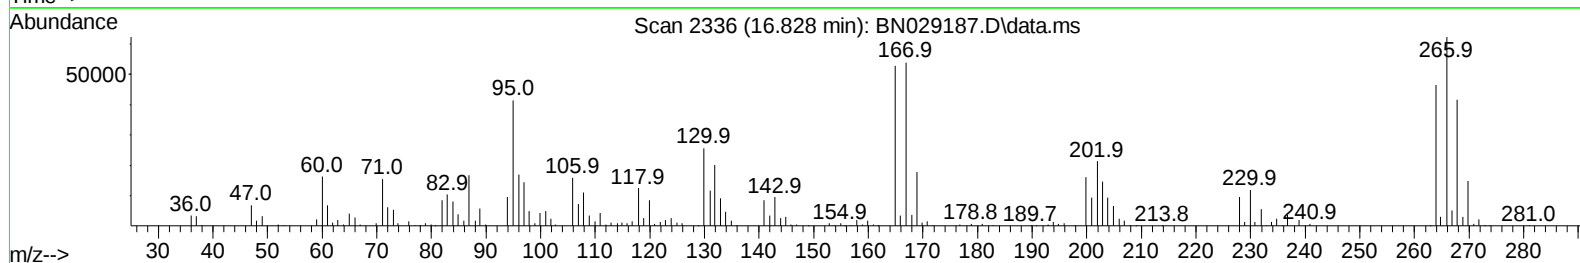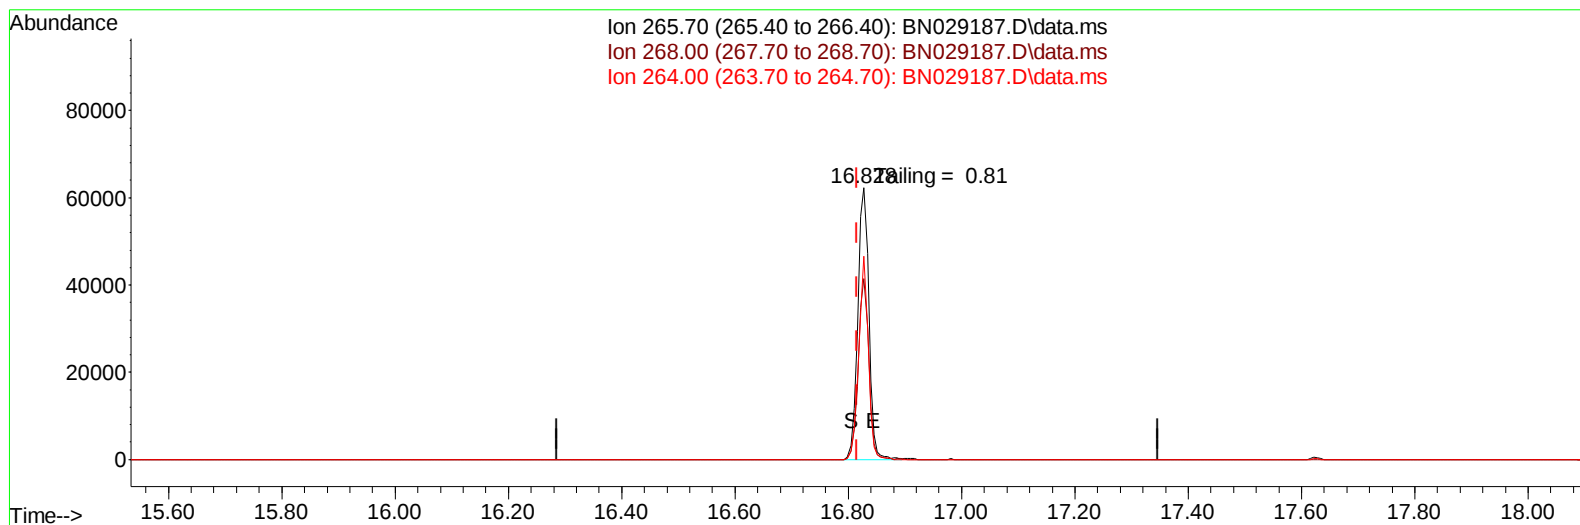

TIC: BN029187.D\data.ms

(70) Pentachlorophenol (C)

16.828min (+ 0.012) 16663.60 ng




response 84217

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.72
264.00	61.60	74.76#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122623\
Data File : BN029187.D
Acq On : 26 Dec 2023 10:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 27 01:51:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

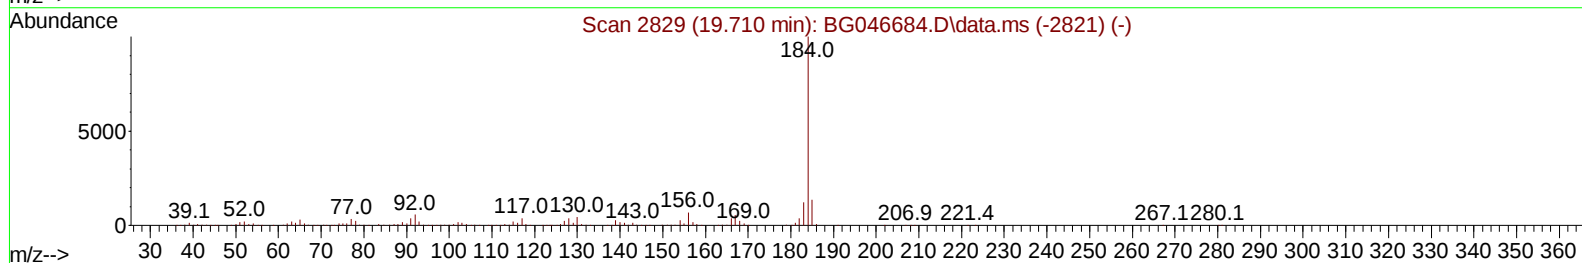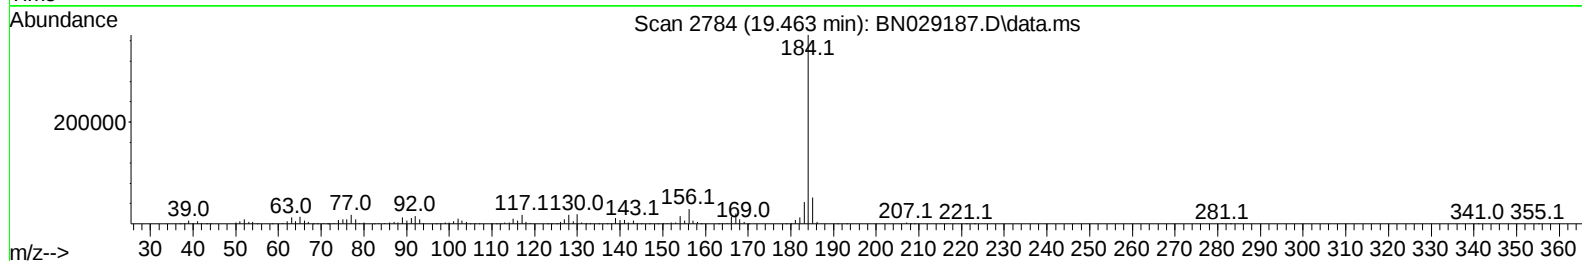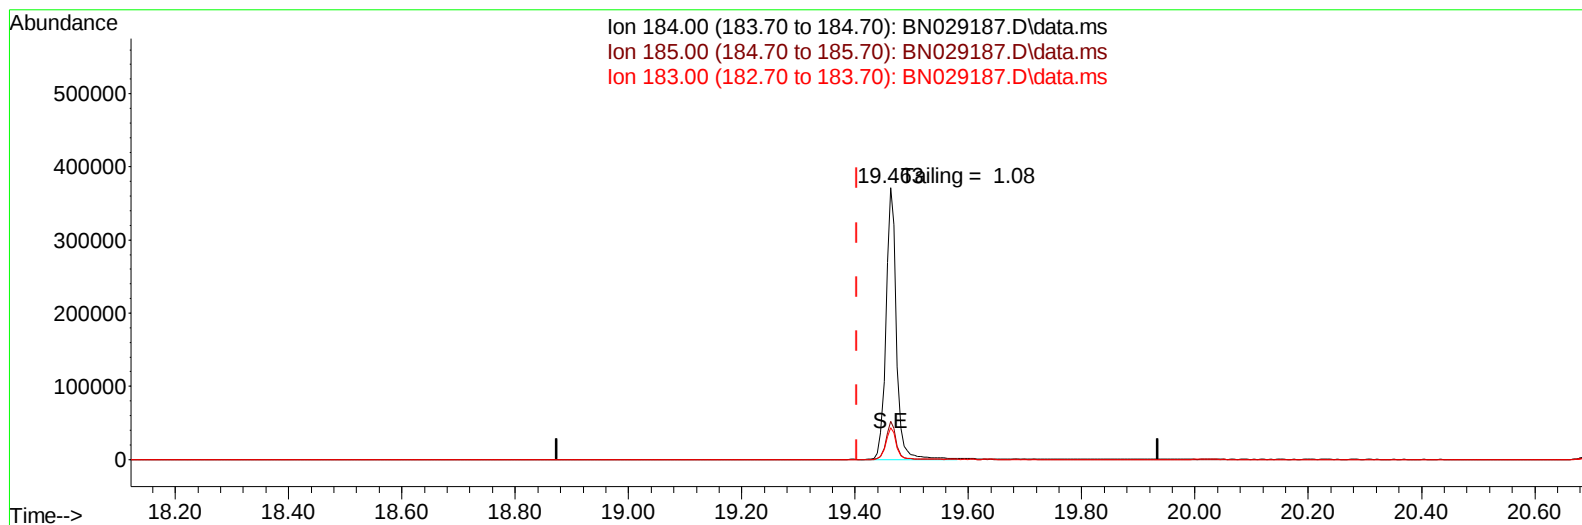

TIC: BN029187.D\data.ms

(77) Benzidine

19.463min (+ 0.059) 0.00 ng

response 478799

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/26/2023	BNA_N	<u>BN029187.D</u>
Compound Name	Response	Retention Time
DDT	258752	20.686
DDD	8902	20.245
DDE	377	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9279	268031	3.46

Instrument :
BNA_N
ClientSampleId :
DFTPP