
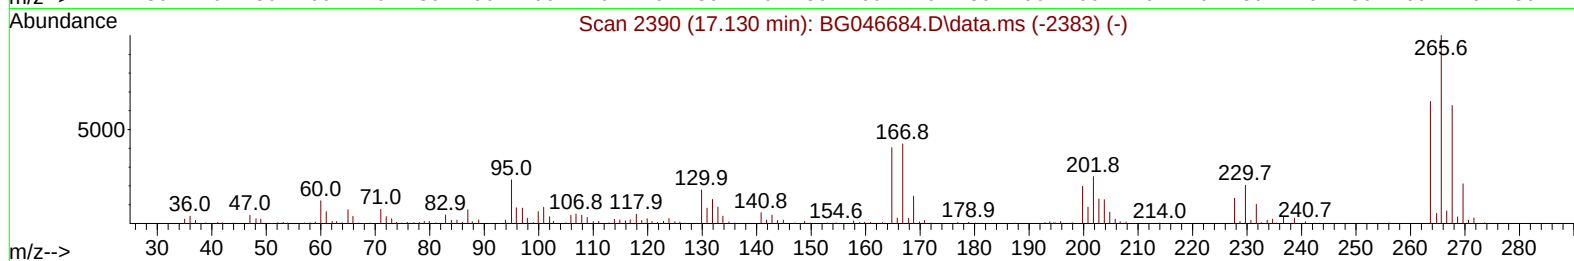
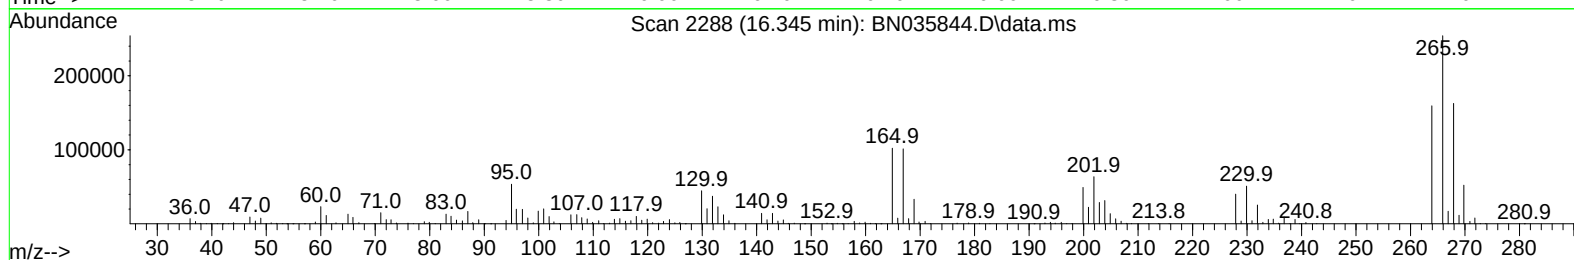


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122624\
Data File : BN035844.D
Acq On : 26 Dec 2024 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 18:22:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

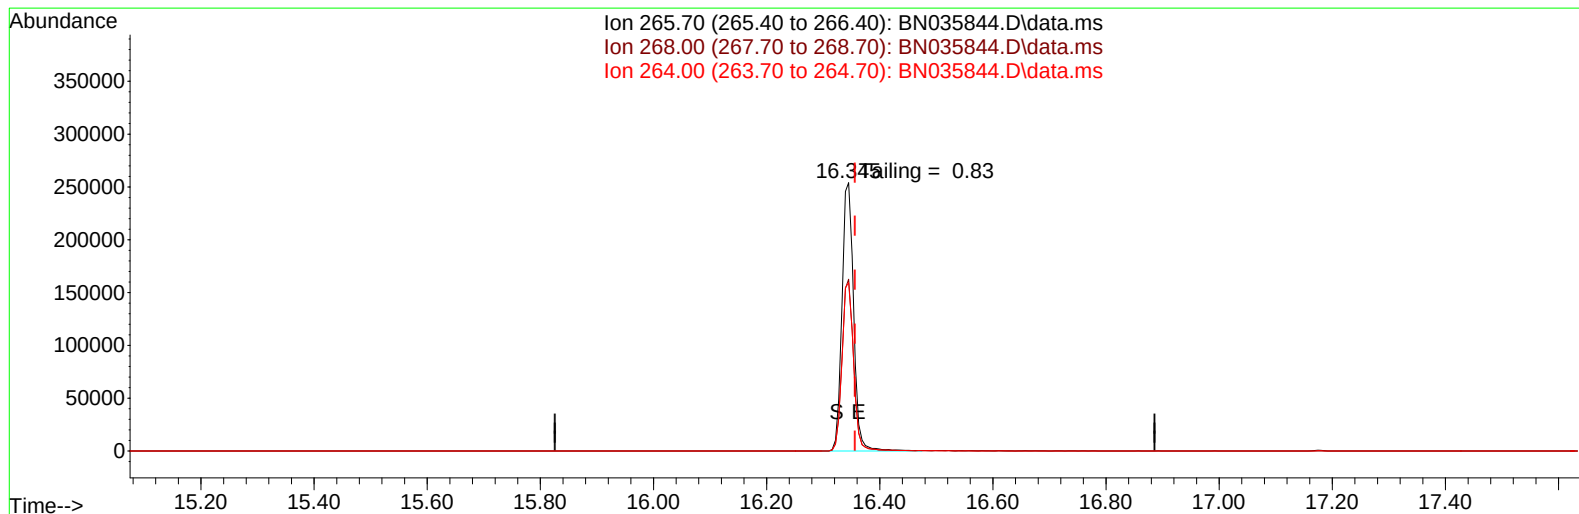

TIC: BN035844.D\data.ms

(70) Pentachlorophenol (C)




16.345min (-0.011) 24950.02 ng

response 363016

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.03
264.00	61.60	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122624\
Data File : BN035844.D
Acq On : 26 Dec 2024 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 18:24:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

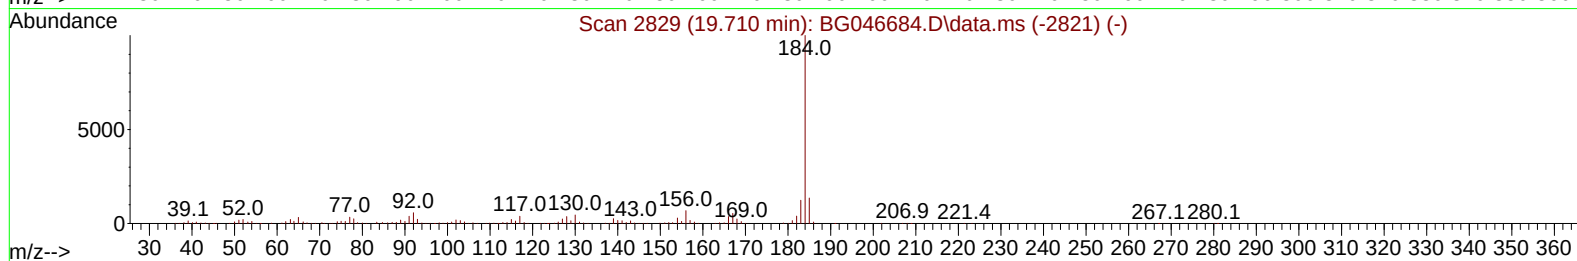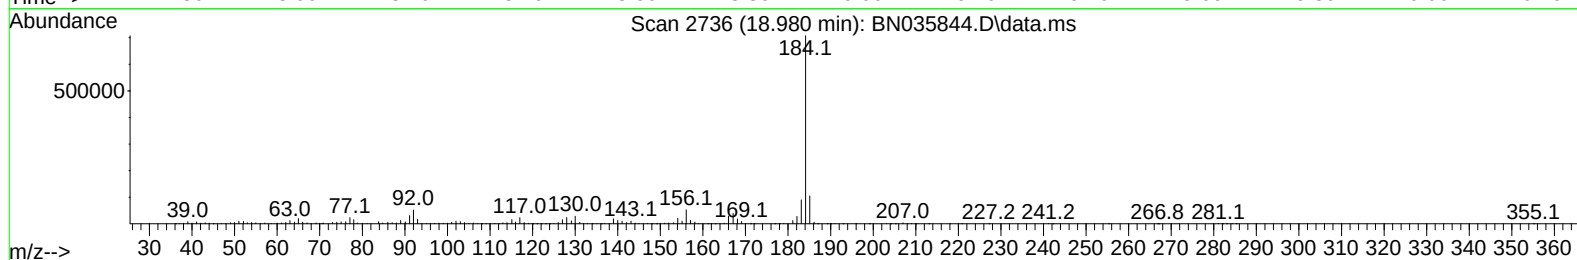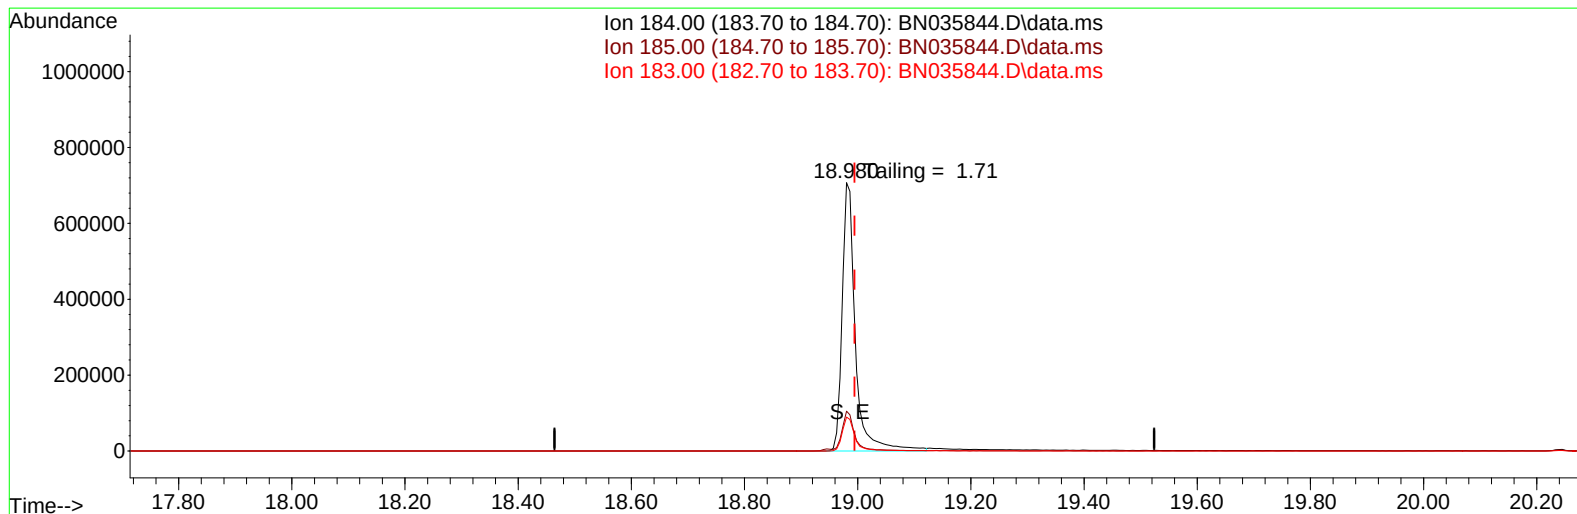

TIC: BN035844.D\data.ms

(77) Benzidine

18.980min (-0.014) 0.00 ng

response 1183784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.84
183.00	13.20	12.69
0.00	0.00	0.00