
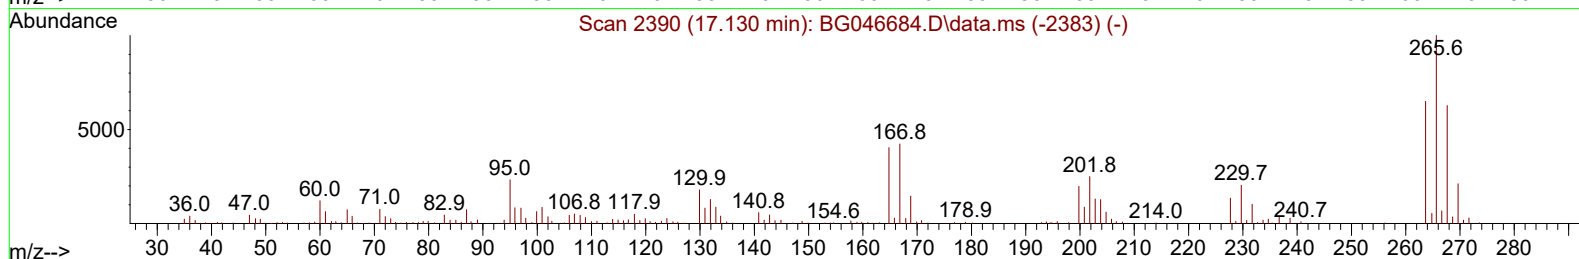
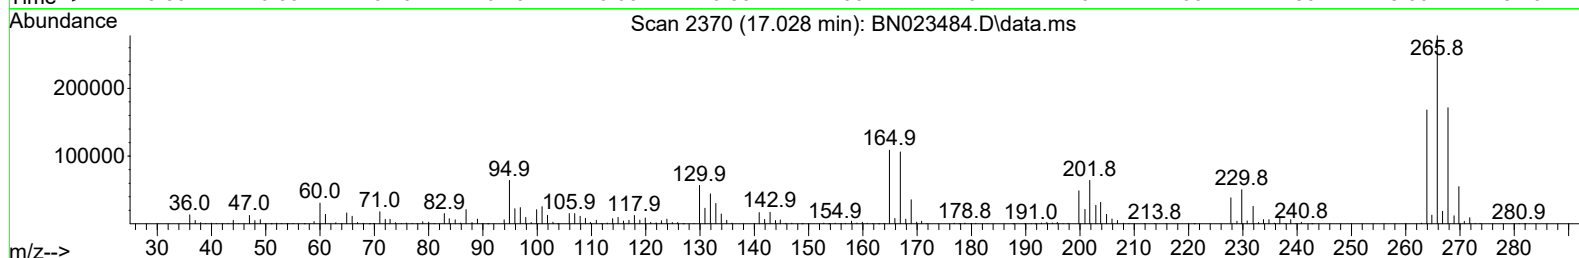


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122722\
Data File : BN023484.D
Acq On : 27 Dec 2022 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 07:03:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 07:03:10 2022
Response via : Initial Calibration

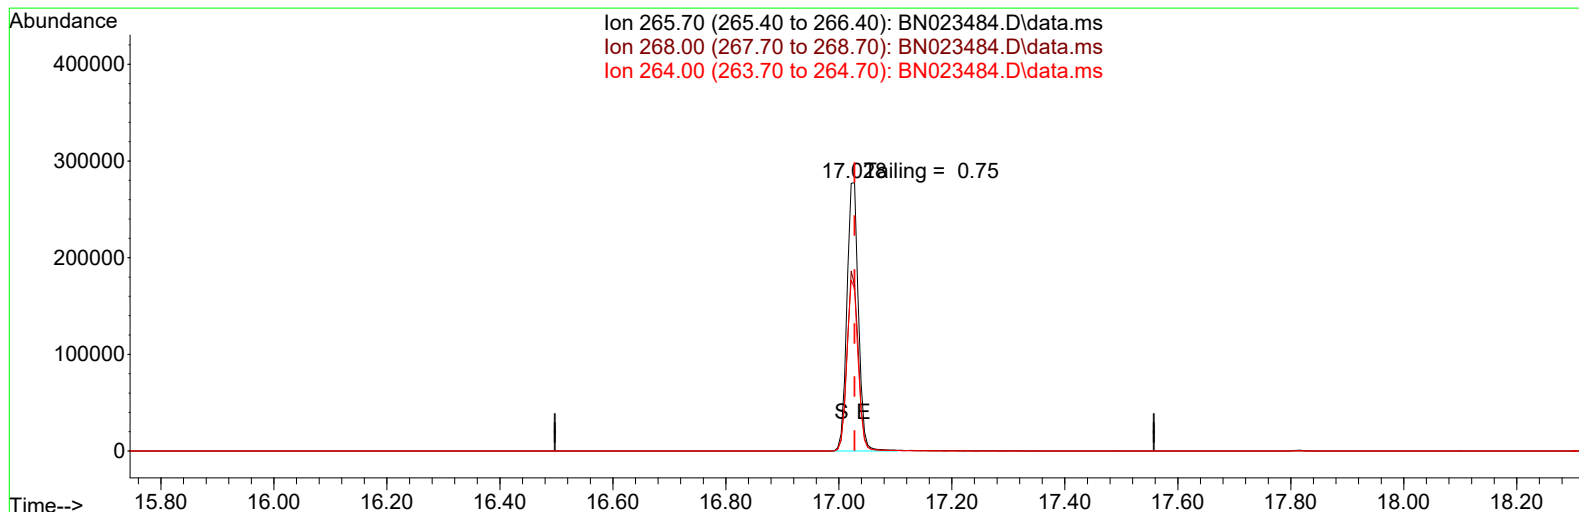

TIC: BN023484.D\data.ms

(70) Pentachlorophenol (C)




17.028min (0.000) 21448.91 ng

response 392872

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.73
264.00	61.60	60.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122722\
Data File : BN023484.D
Acq On : 27 Dec 2022 12:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 07:03:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 07:03:10 2022
Response via : Initial Calibration

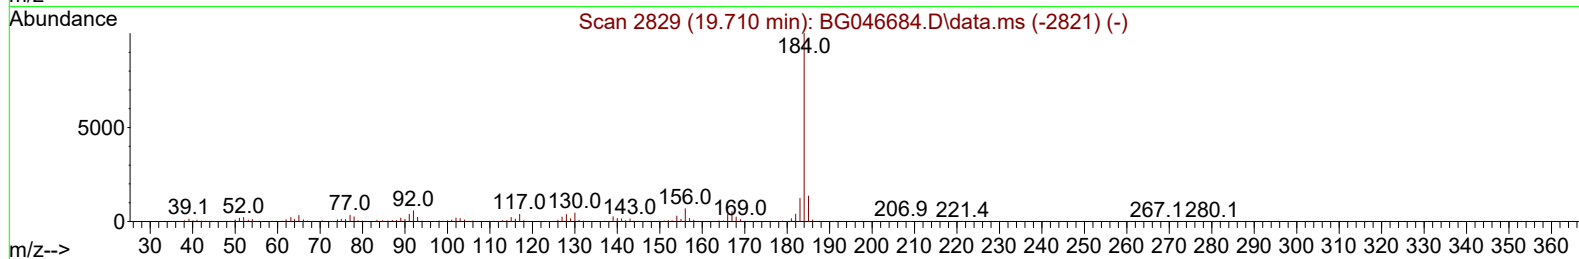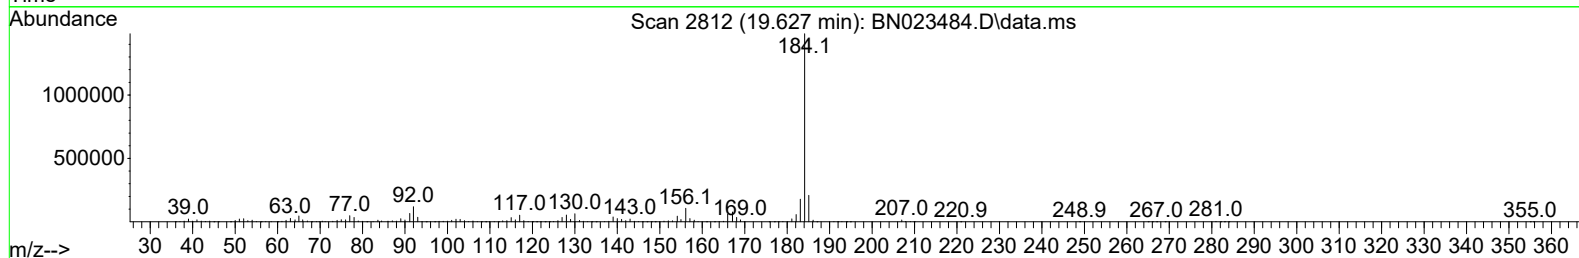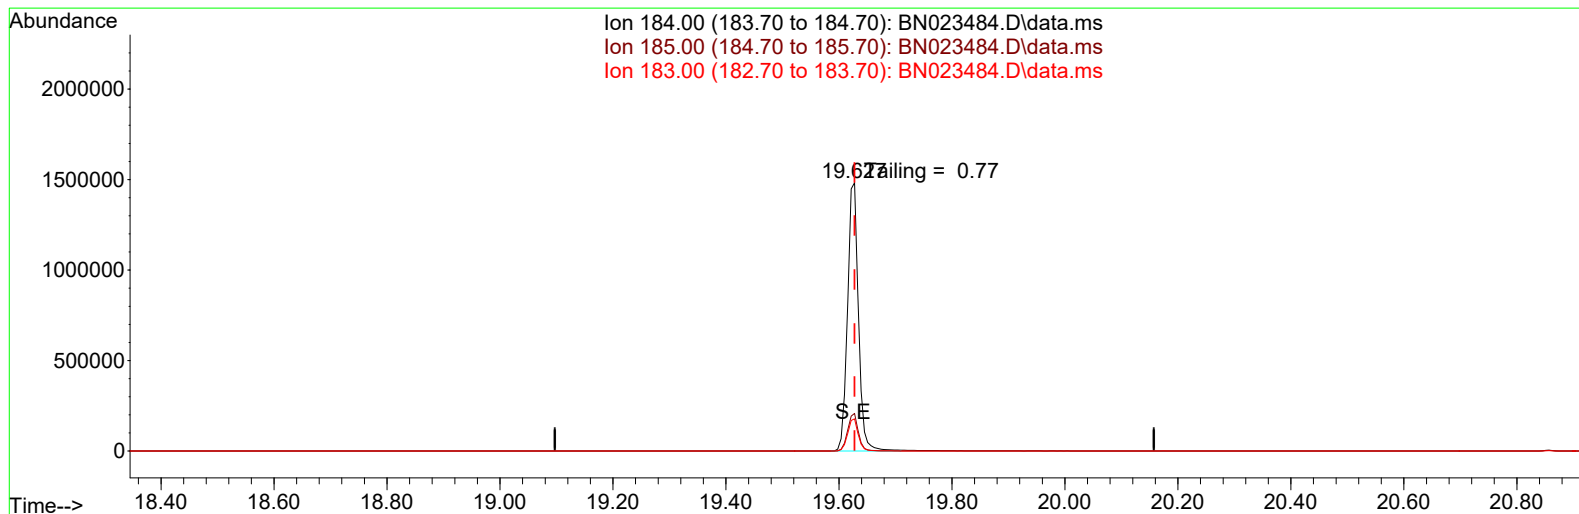

TIC: BN023484.D\data.ms

(77) Benzidine

19.627min (0.000) 0.00 ng

response 1998419

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	11.98
0.00	0.00	0.00