
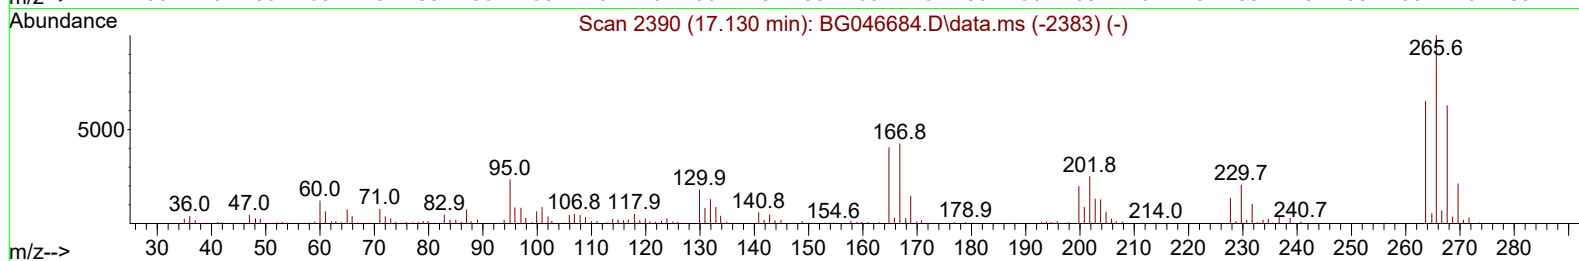
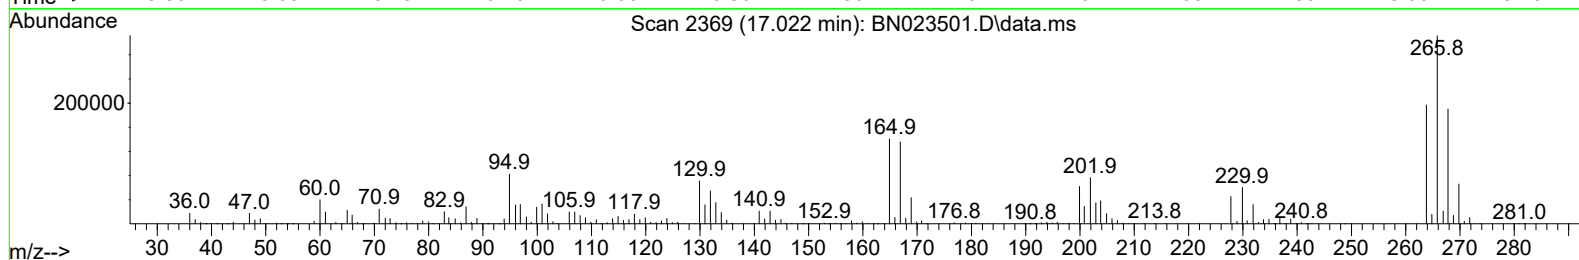


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122722\
Data File : BN023501.D
Acq On : 28 Dec 2022 00:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 07:04:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 07:03:10 2022
Response via : Initial Calibration

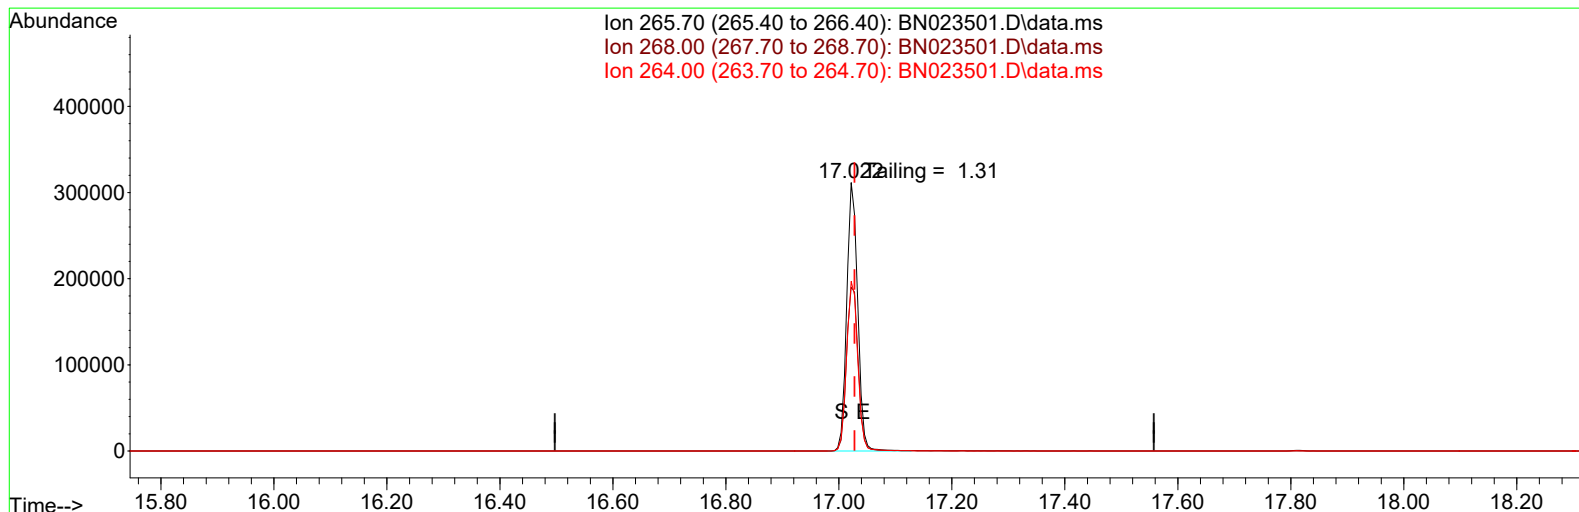

TIC: BN023501.D\data.ms

(70) Pentachlorophenol (C)




17.022min (-0.006) 22654.06 ng

response 420991

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.08
264.00	61.60	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122722\
Data File : BN023501.D
Acq On : 28 Dec 2022 00:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 07:04:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 07:03:10 2022
Response via : Initial Calibration

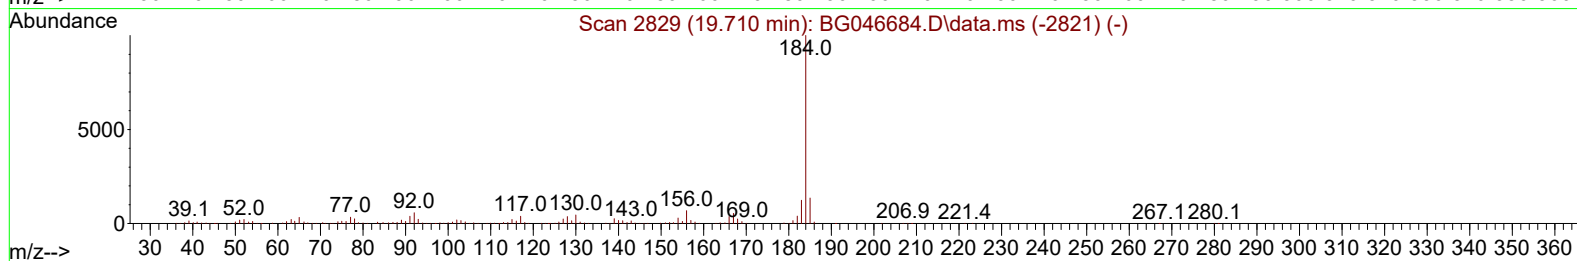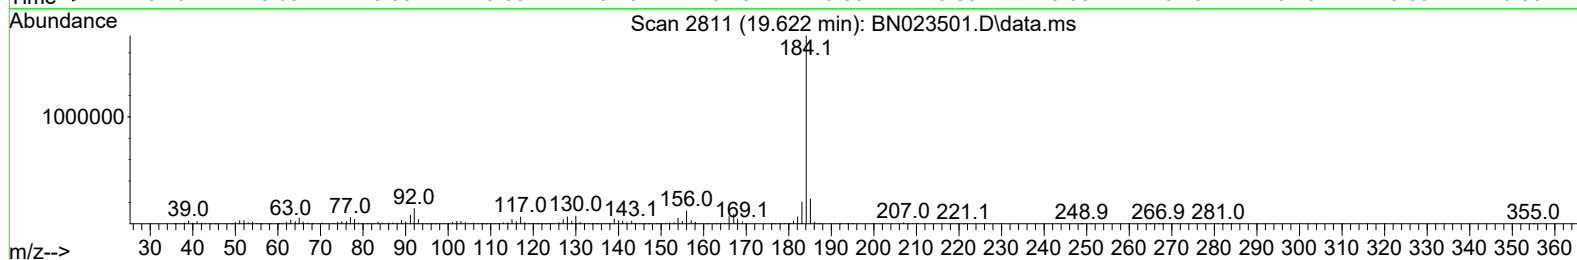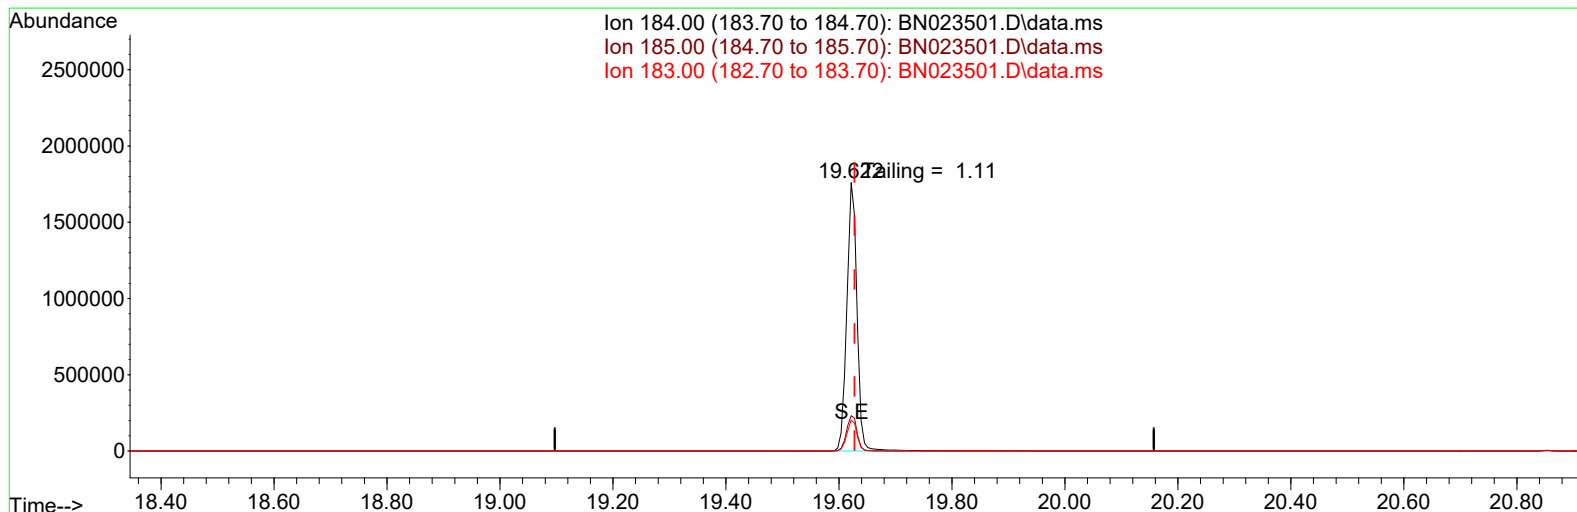

TIC: BN023501.D\data.ms

(77) Benzidine

19.622min (-0.006) 0.00 ng

response 2203733

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.20
183.00	13.20	11.51
0.00	0.00	0.00