


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN122722\  
 Data File : BN023484.D  
 Acq On : 27 Dec 2022 12:08  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN122722.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Dec 28 03:57:20 2022

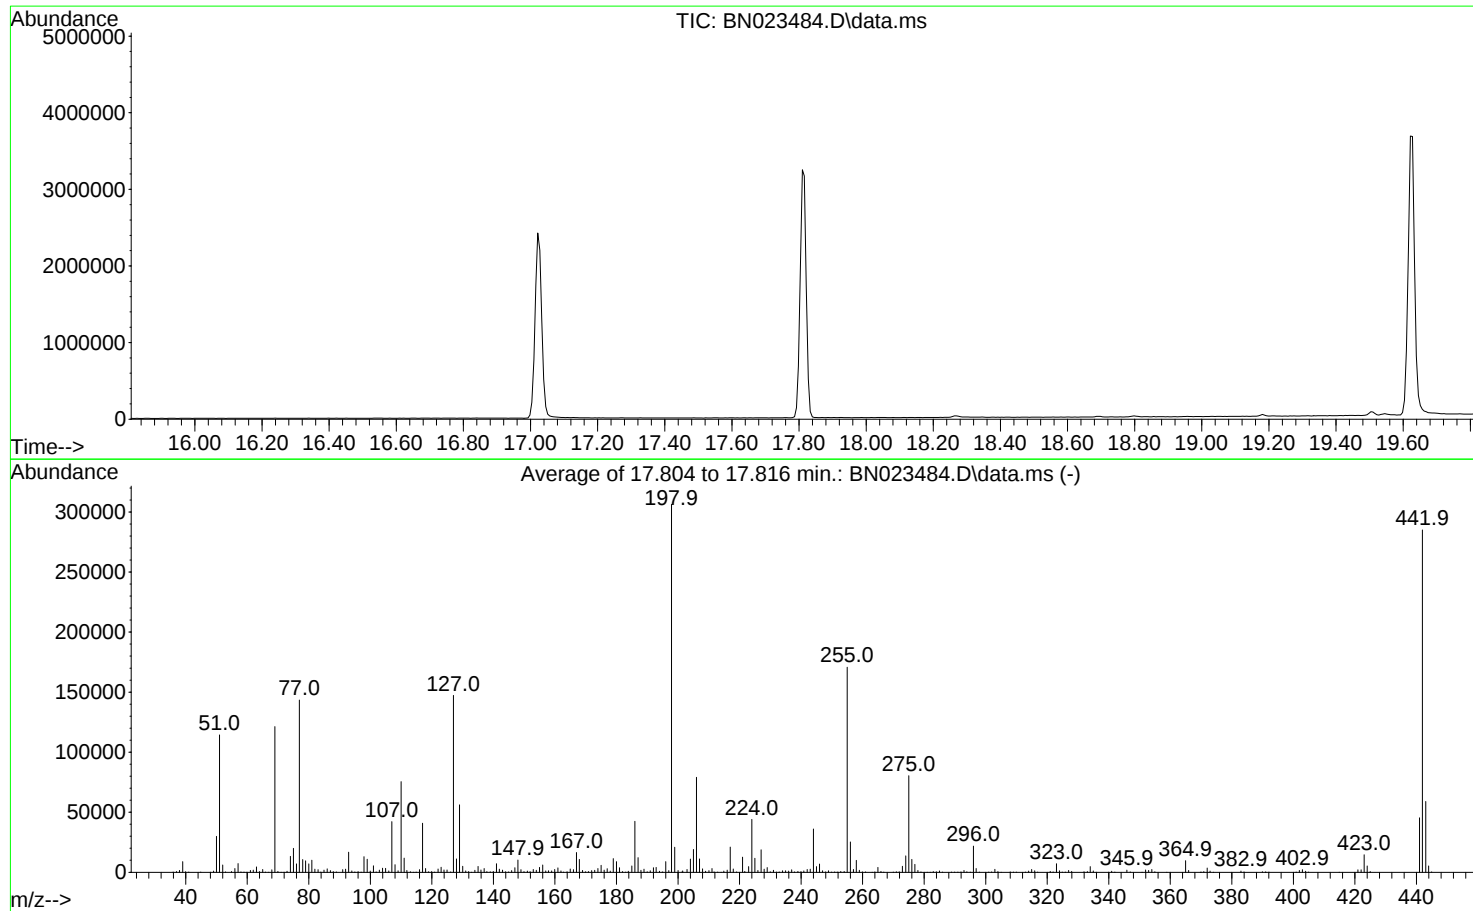




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 37.4         | 114435     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 2076       | PASS                |
| 69             | 198             | 0.00            | 100             | 39.6         | 121308     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 753        | PASS                |
| 127            | 198             | 10              | 80              | 48.1         | 147269     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 1355       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 306304     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 20817      | PASS                |
| 275            | 198             | 10              | 60              | 26.2         | 80397      | PASS                |
| 365            | 198             | 1               | 100             | 3.2          | 9704       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.8         | 45365      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 285016     | PASS                |
| 443            | 442             | 15              | 24              | 20.7         | 58987      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN122722\  
 Data File : BN023484.D  
 Acq On : 27 Dec 2022 12:08  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Dec 28 07:03:15 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 28 07:03:10 2022  
 Response via : Initial Calibration

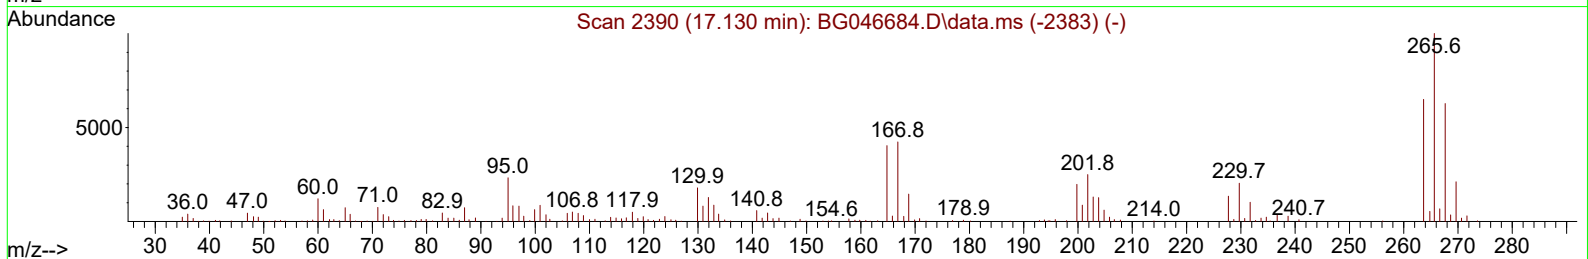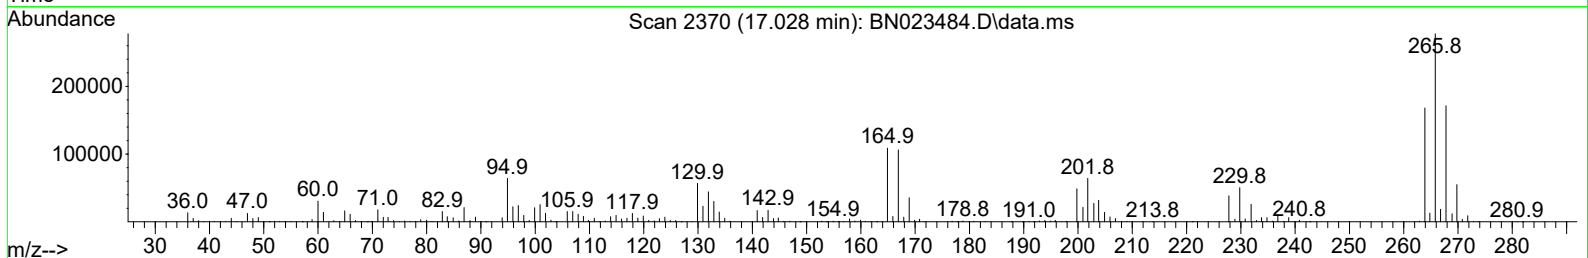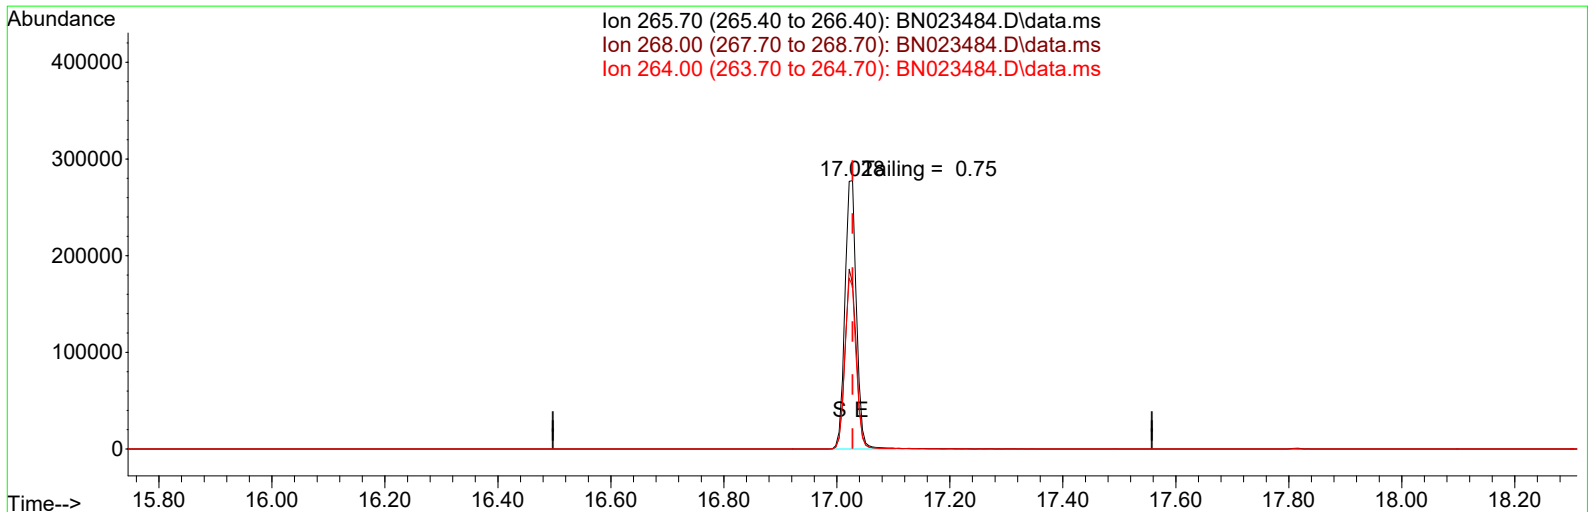

TIC: BN023484.D\data.ms

**(70) Pentachlorophenol (C)**

17.028min ( 0.000) 21448.91 ng




response 392872

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.73  |
| 264.00 | 61.60  | 60.56  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN122722\  
 Data File : BN023484.D  
 Acq On : 27 Dec 2022 12:08  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Dec 28 07:03:15 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 28 07:03:10 2022  
 Response via : Initial Calibration

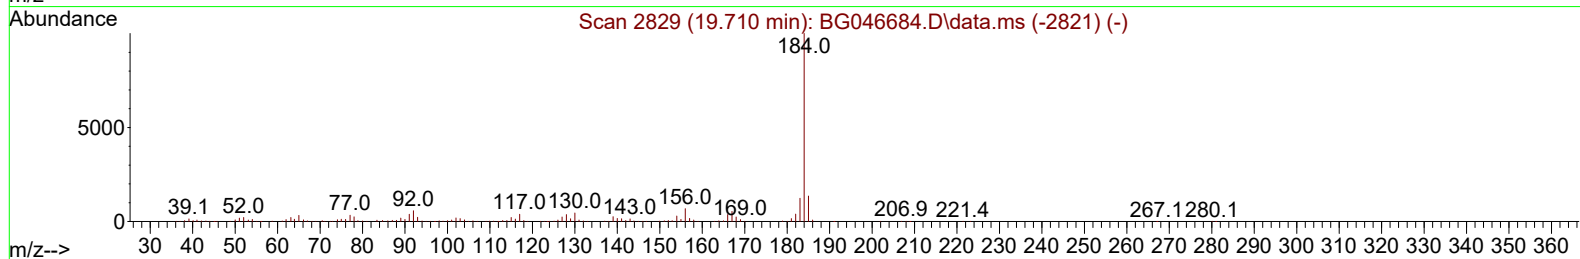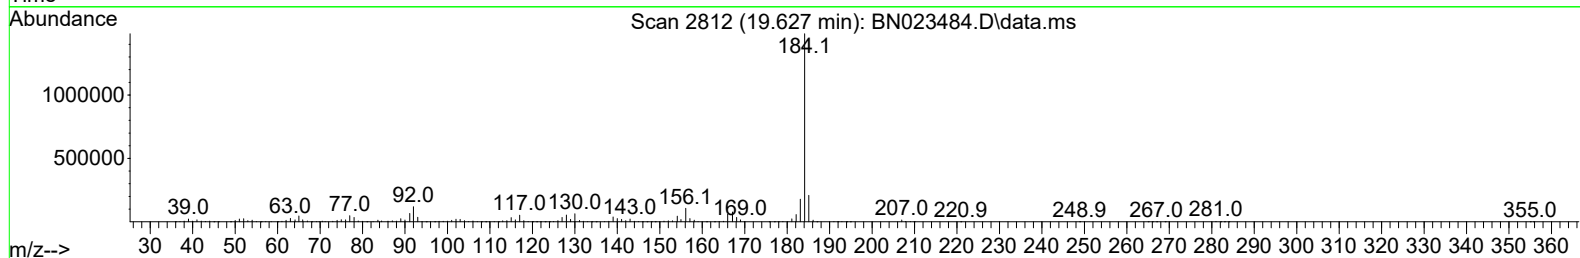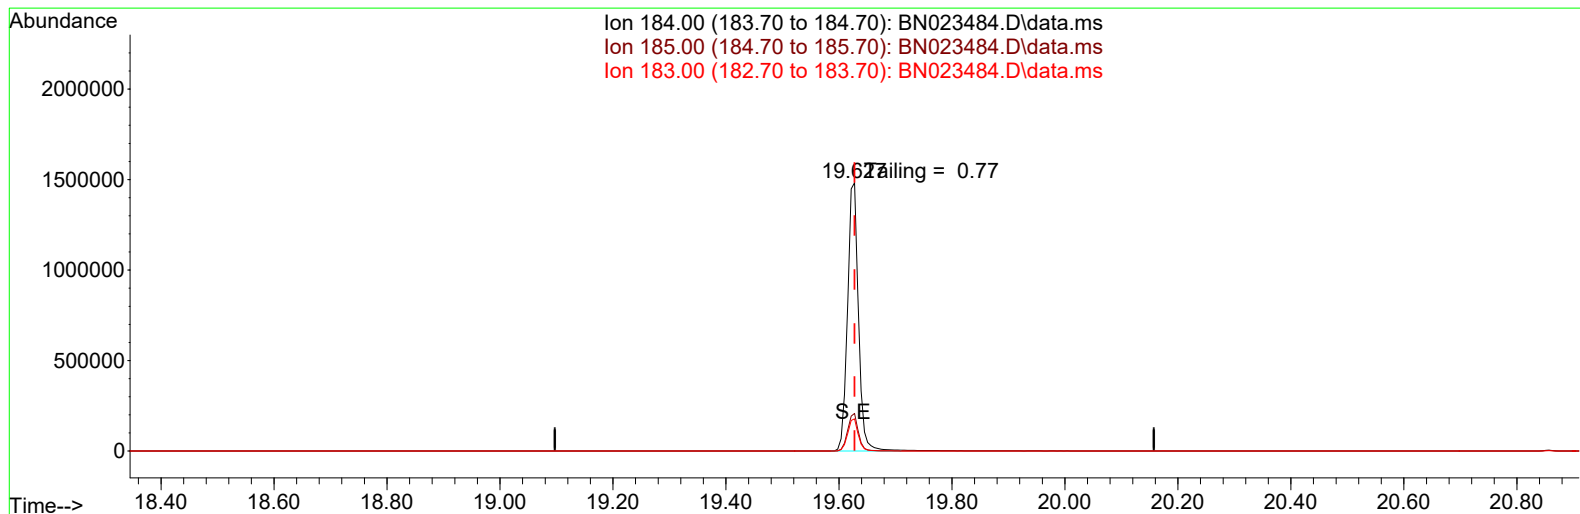

TIC: BN023484.D\data.ms

**(77) Benzidine**

19.627min ( 0.000) 0.00 ng

response 1998419

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.04  |
| 183.00 | 13.20  | 11.98  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/27/2022    | BNA_N            | <u>BN023484.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1031143          | 20.857             |
| DDD           | 25879            | 20.416             |
| DDE           | 576              | 19.91              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 26455         | 1057598          | 2.50               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP