


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122722\
 Data File : BN023501.D
 Acq On : 28 Dec 2022 00:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 03:57:20 2022

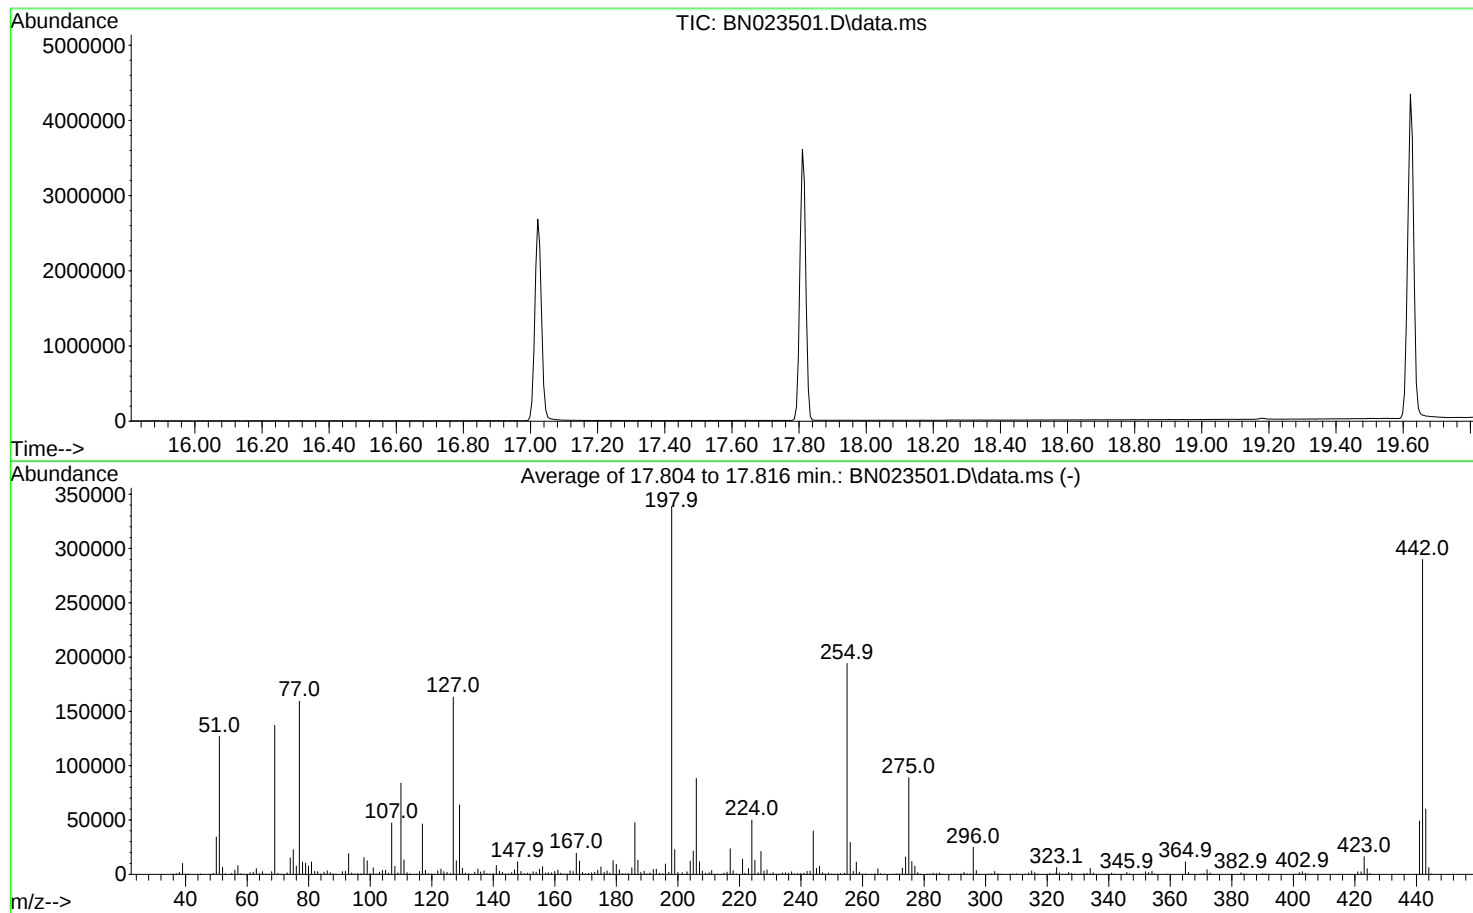




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	126885	PASS
68	69	0.00	2	1.8	2423	PASS
69	198	0.00	100	40.5	137112	PASS
70	69	0.00	2	0.6	755	PASS
127	198	10	80	48.2	163115	PASS
197	198	0.00	2	0.6	1911	PASS
198	198	100	100	100.0	338731	PASS
199	198	5	9	6.7	22771	PASS
275	198	10	60	26.2	88861	PASS
365	198	1	100	3.4	11494	PASS
441	198	0.01	100	14.5	49141	PASS
442	442	50	100	100.0	289963	PASS
443	442	15	24	20.8	60205	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122722\
 Data File : BN023501.D
 Acq On : 28 Dec 2022 00:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 28 07:04:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 07:03:10 2022
 Response via : Initial Calibration

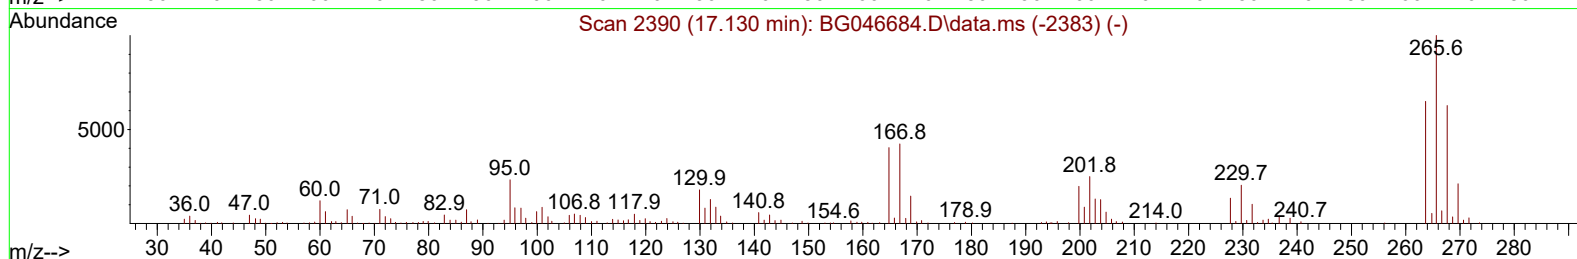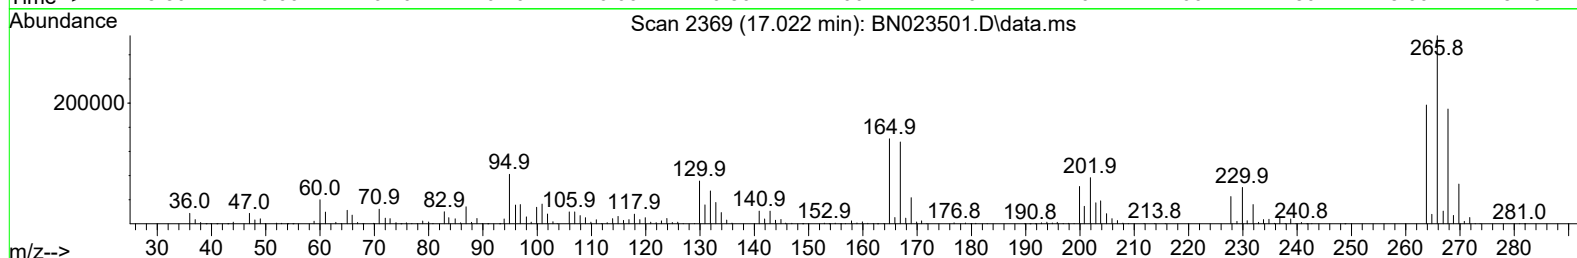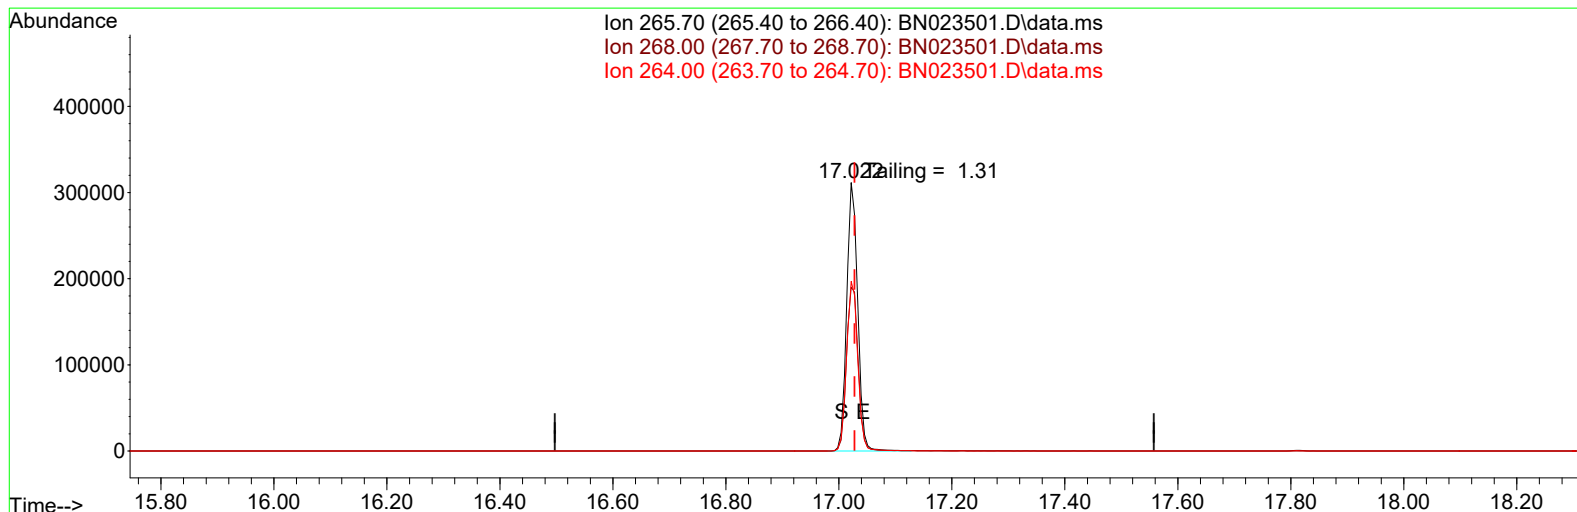

TIC: BN023501.D\data.ms

(70) Pentachlorophenol (C)

17.022min (-0.006) 22654.06 ng




response 420991

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.08
264.00	61.60	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122722\
 Data File : BN023501.D
 Acq On : 28 Dec 2022 00:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 28 07:04:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 07:03:10 2022
 Response via : Initial Calibration

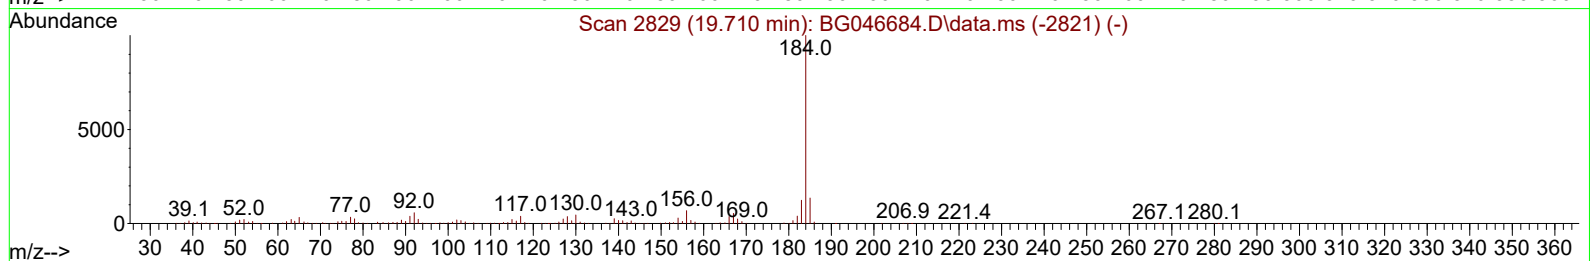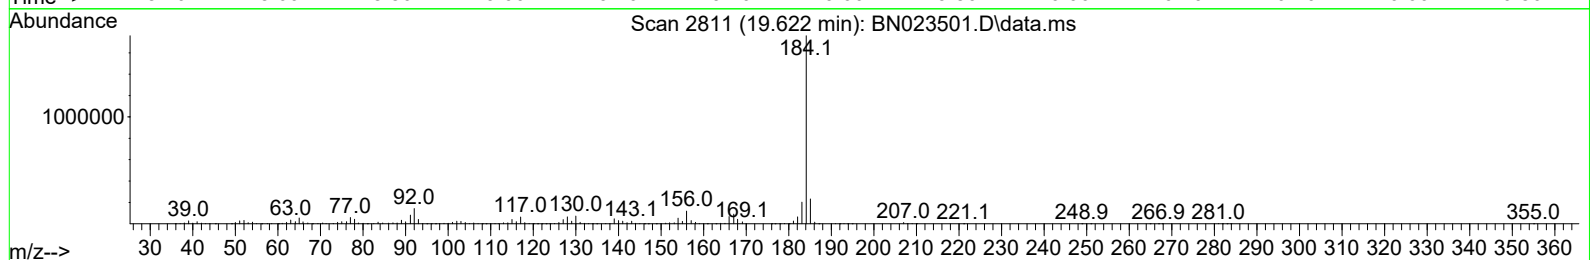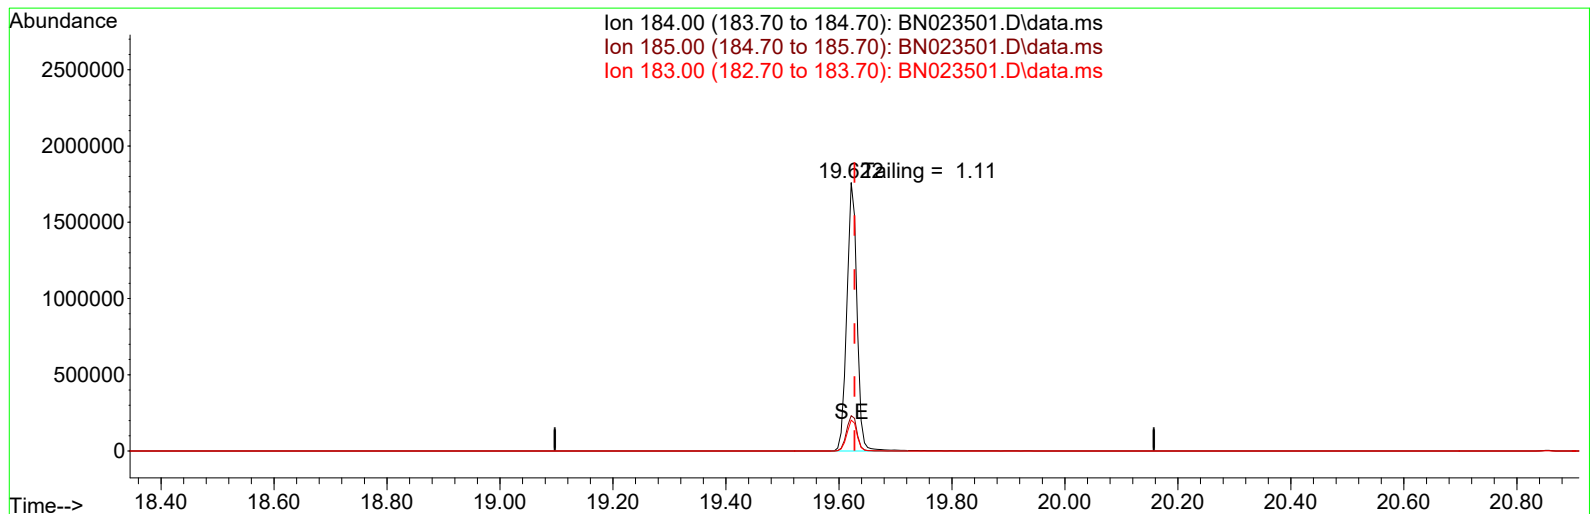

TIC: BN023501.D\data.ms

(77) Benzidine

19.622min (-0.006) 0.00 ng

response 2203733

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.20
183.00	13.20	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/27/2022	BNA_N	<u>BN023501.D</u>
Compound Name	Response	Retention Time
DDT	1157056	20.857
DDD	40107	20.416
DDE	388	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40495	1197551	3.38

Instrument :
BNA_N
ClientSampleId :
DFTPP