

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122723\
 Data File : BN029202.D
 Acq On : 27 Dec 2023 16:31
 Operator : MA/JU
 Sample : PB158020BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB158020BL

Quant Time: Dec 28 01:44:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 28 01:20:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.732	152	823	0.400	ng	0.00
7) Naphthalene-d8	10.530	136	1465	0.400	ng	# 0.01
13) Acenaphthene-d10	14.383	164	867	0.400	ng	0.01
19) Phenanthrene-d10	17.144	188	1339	0.400	ng	# 0.01
29) Chrysene-d12	21.349	240	487	0.400	ng	0.00
35) Perylene-d12	23.636	264	579	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.341	112	663	0.346	ng	0.00
5) Phenol-d6	6.944	99	625	0.291	ng	0.00
8) Nitrobenzene-d5	8.918	82	492	0.268	ng	0.01
11) 2-Methylnaphthalene-d10	12.129	152	722	0.285	ng	0.00
14) 2,4,6-Tribromophenol	15.902	330	171	0.256	ng	0.02
15) 2-Fluorobiphenyl	13.014	172	1277	0.275	ng	0.01
27) Fluoranthene-d10	19.178	212	722	0.265	ng	0.00
31) Terphenyl-d14	19.787	244	453	0.300	ng	0.00
Target Compounds						
20) 4,6-Dinitro-2-methylph...	15.484	198	3	0.108	ng	# 33
34) Bis(2-ethylhexyl)phtha...	21.268	149	108	0.026	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122723\
Data File : BN029202.D
Acq On : 27 Dec 2023 16:31
Operator : MA/JU
Sample : PB158020BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB158020BL


Quant Time: Dec 28 01:44:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 28 01:20:47 2023
Response via : Initial Calibration

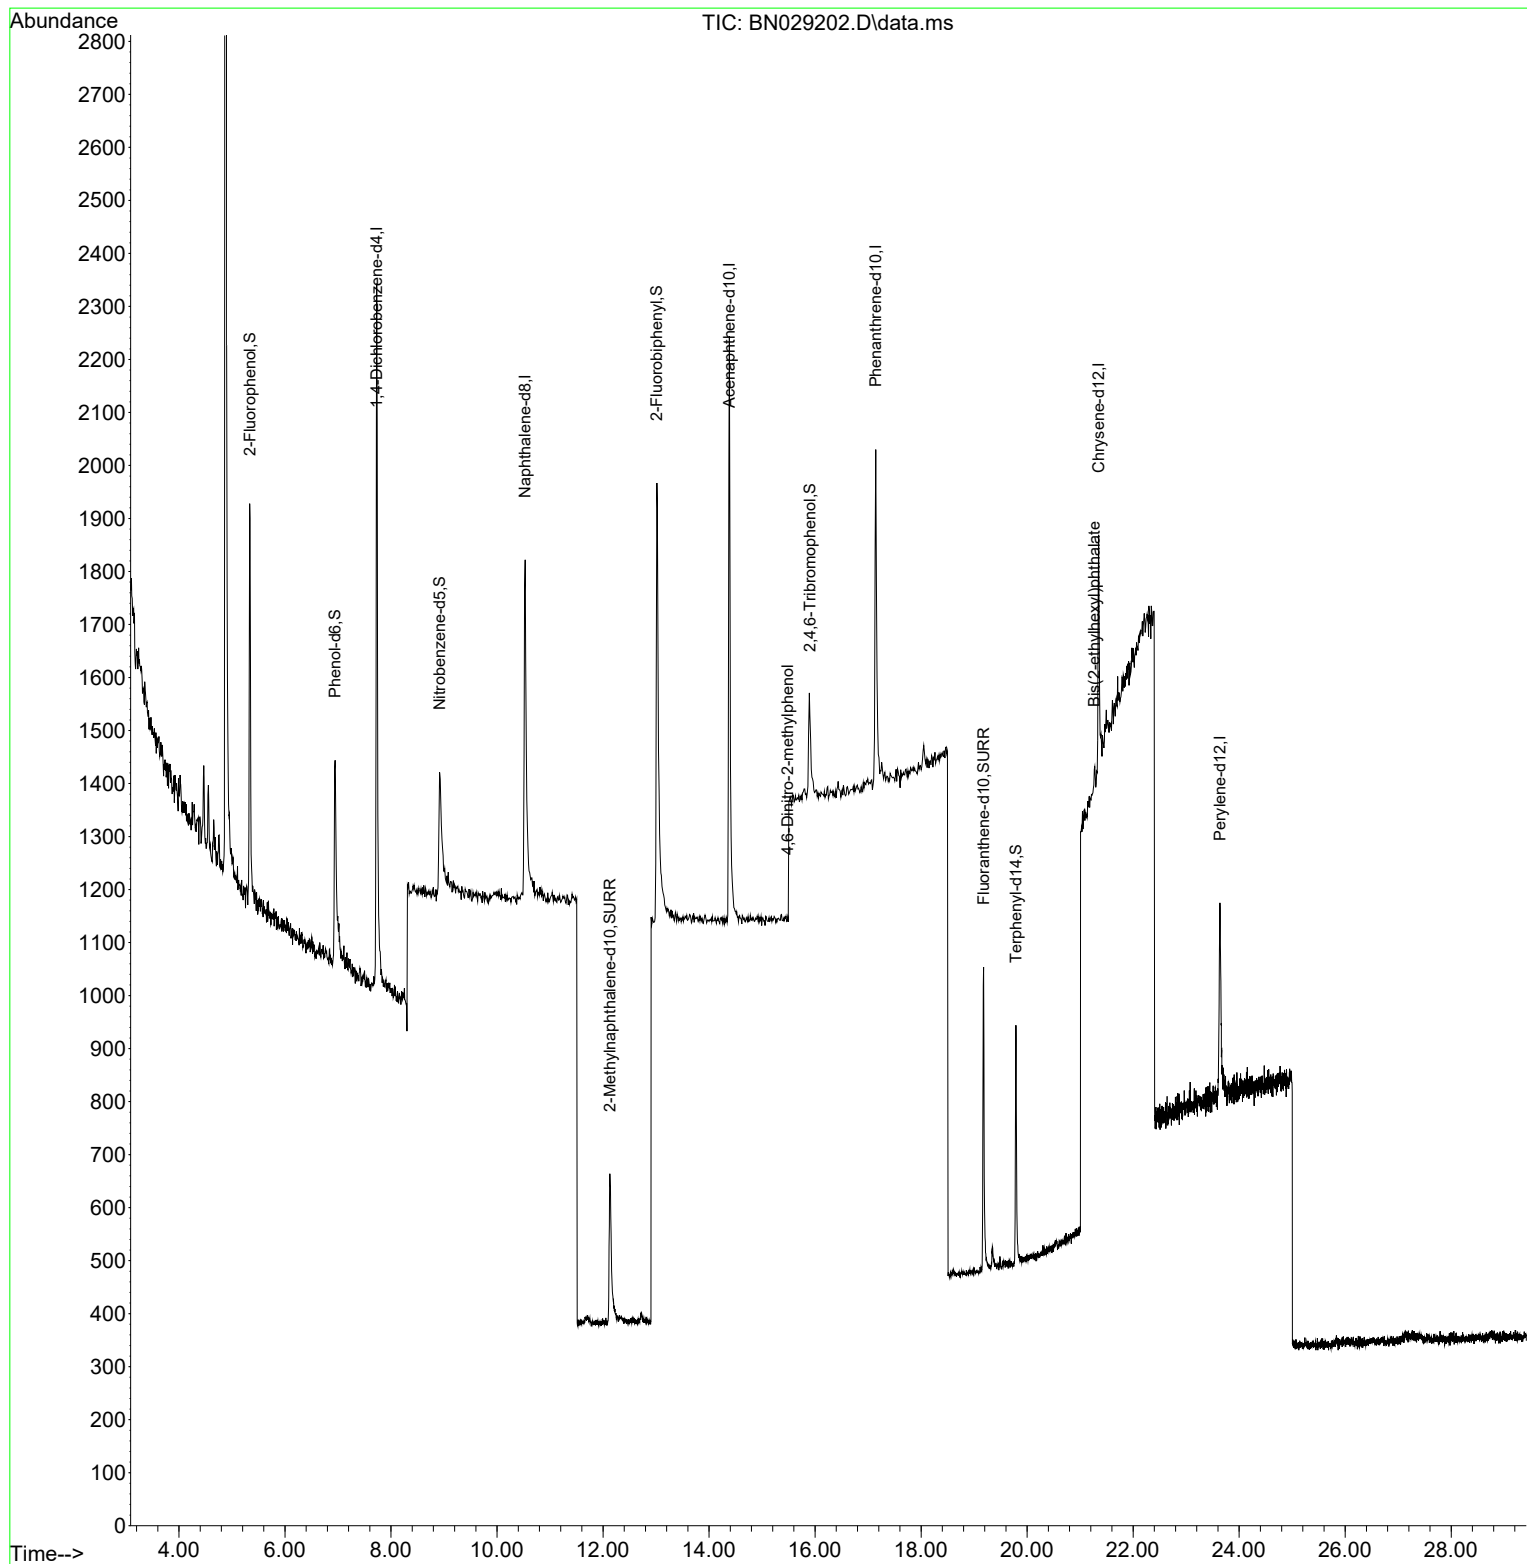



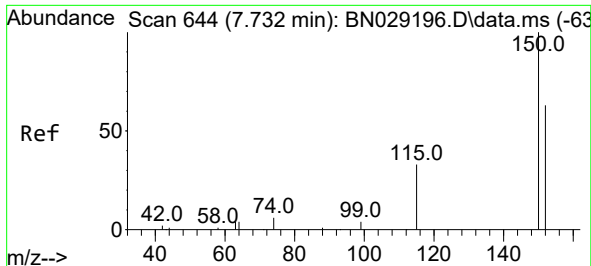


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.732 min Scan# 644
Delta R.T. -0.000 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31

Instrument :
BNA_N
ClientSampleId :
PB158020BL



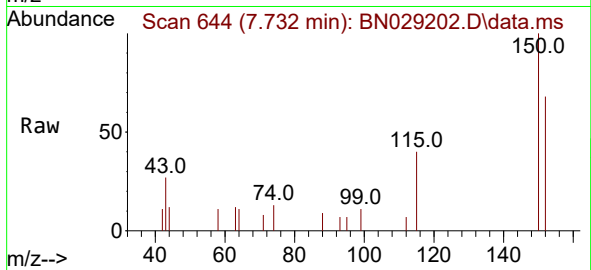



Tgt Ion:152 Resp: 823
Ion Ratio Lower Upper
152 100
150 147.2 122.2 183.2
115 59.5 48.2 72.4

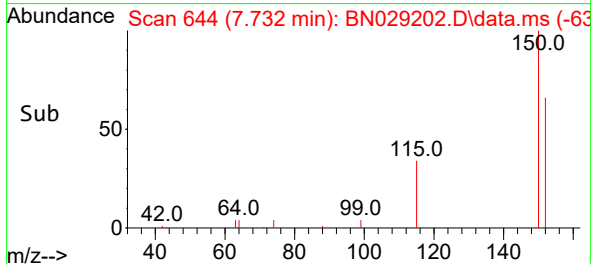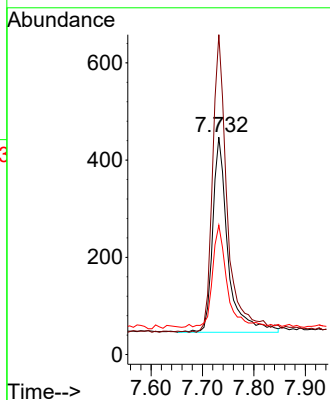

#4
2-Fluorophenol
Concen: 0.346 ng
RT: 5.341 min Scan# 313
Delta R.T. 0.007 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31

Tgt Ion:112 Resp: 663
Ion Ratio Lower Upper
112 100
64 47.1 38.8 58.2
63 38.5 30.6 45.8


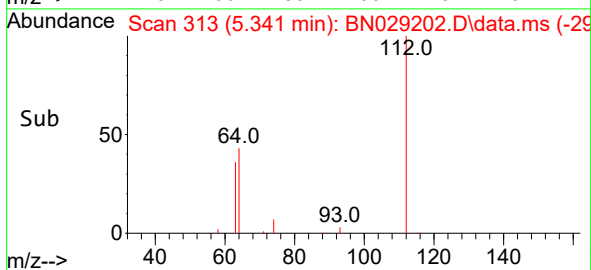
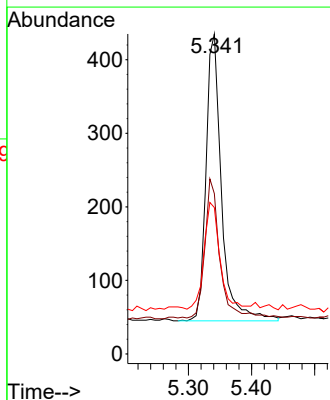
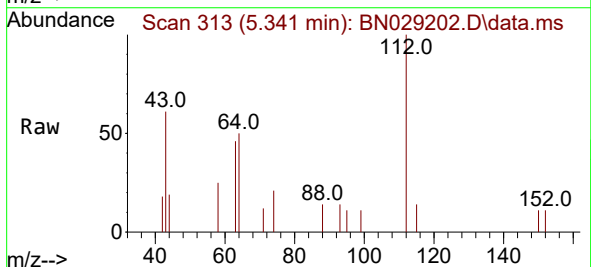


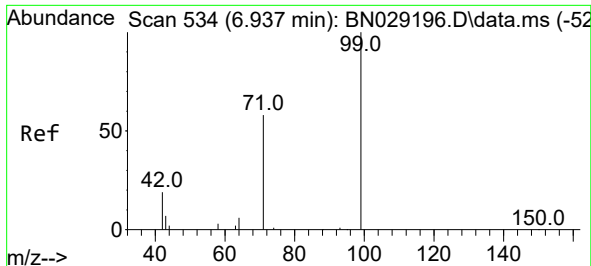

#5
Phenol-d6
Concen: 0.291 ng
RT: 6.944 min Scan# 511
Delta R.T. 0.007 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31




Instrument :
BNA_N
ClientSampleId :
PB158020BL


Tgt Ion: 99 Resp: 625
Ion Ratio Lower Upper
99 100
42 15.8 18.3 27.5#
71 57.0 48.6 73.0

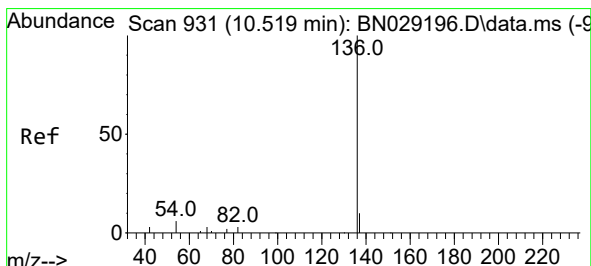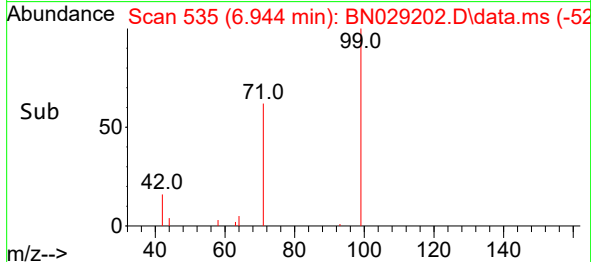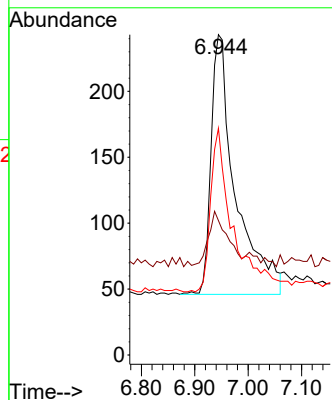

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.530 min Scan# 932
Delta R.T. 0.011 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31

Tgt Ion: 136 Resp: 1465
Ion Ratio Lower Upper
136 100
137 19.1 13.0 19.4
54 14.0 9.8 14.6
68 11.9 7.4 11.2#


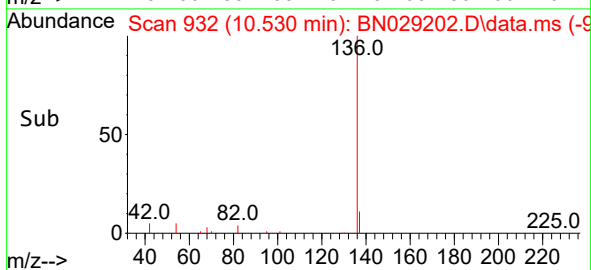
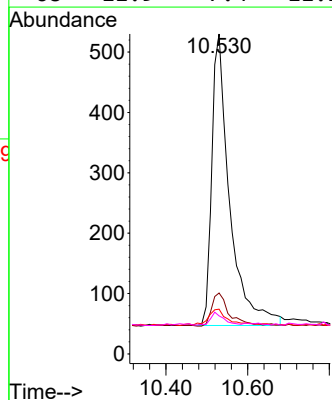
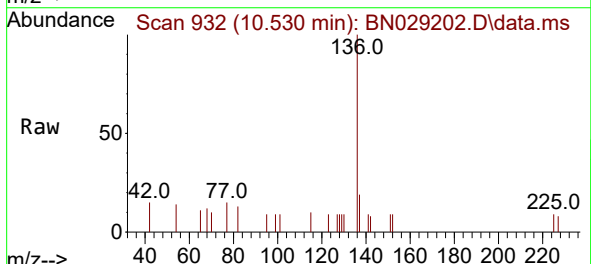


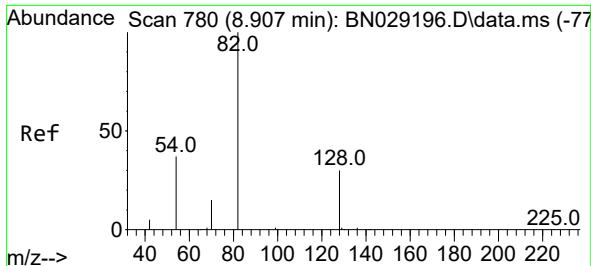

#8
Nitrobenzene-d5
Concen: 0.268 ng
RT: 8.918 min Scan# 781
Delta R.T. 0.011 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31




Instrument :
BNA_N
ClientSampleId :
PB158020BL


Tgt Ion: 82 Resp: 492
Ion Ratio Lower Upper
82 100
128 53.3 34.2 51.2#
54 52.1 38.8 58.2

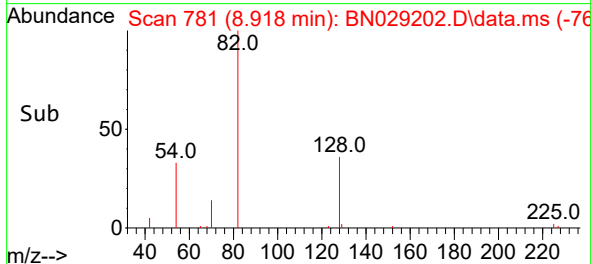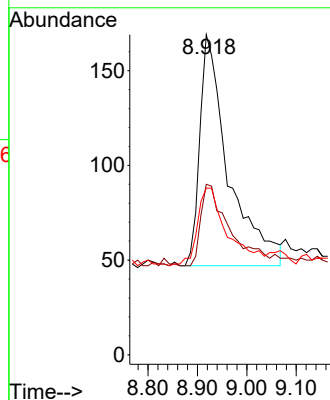

#11
2-Methylnaphthalene-d10
Concen: 0.285 ng
RT: 12.129 min Scan# 1187
Delta R.T. 0.008 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31

Tgt Ion:152 Resp: 722
Ion Ratio Lower Upper
152 100
151 18.6 16.6 24.8

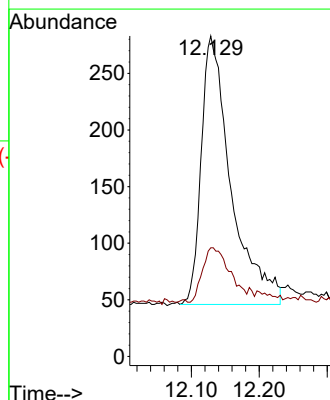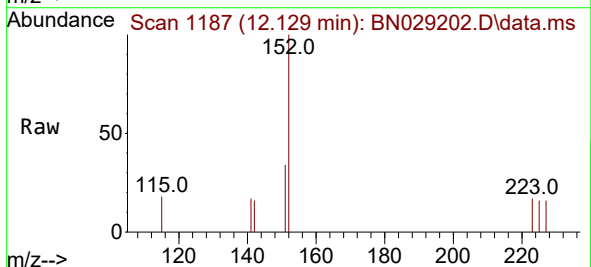



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.383 min Scan# 11

Delta R.T. 0.011 min

Lab File: BN029202.D

Acq: 27 Dec 2023 16:31

Instrument :

BNA_N

ClientSampleId :

PB158020BL





Tgt Ion:164 Resp: 867

Ion Ratio Lower Upper

164 100

162 107.3 91.8 137.8

160 60.0 49.4 74.2

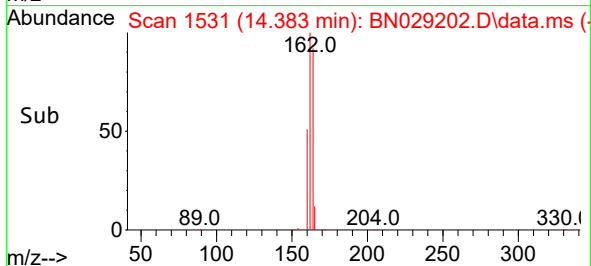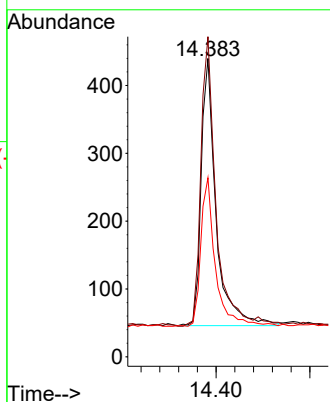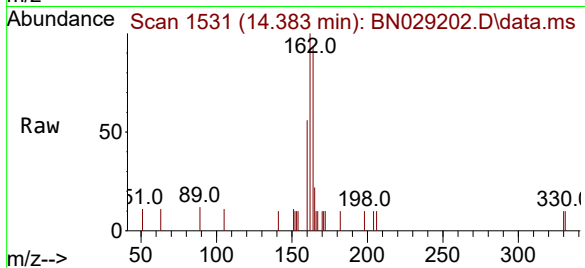

#14

2,4,6-Tribromophenol

Concen: 0.256 ng

RT: 15.902 min Scan# 1668

Delta R.T. 0.025 min

Lab File: BN029202.D

Acq: 27 Dec 2023 16:31




Tgt Ion:330 Resp: 171


Ion Ratio Lower Upper

330 100

332 100.6 74.4 111.6

141 0.0 46.7 70.1#


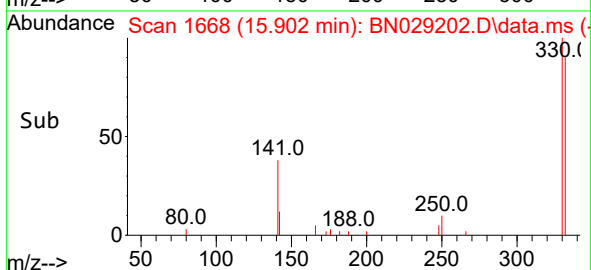
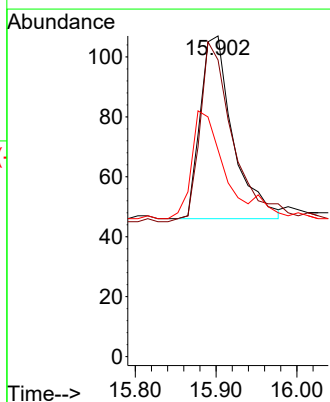
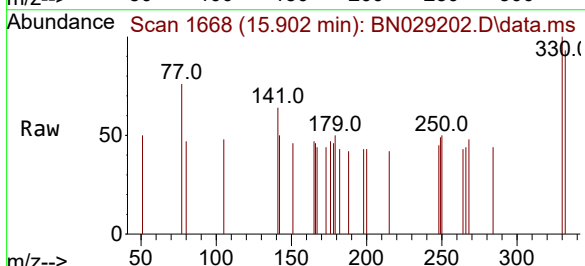




#15
2-Fluorobiphenyl
Concen: 0.275 ng
RT: 13.014 min Scan# 1402
Delta R.T. 0.011 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31




Instrument :
BNA_N
ClientSampleId :
PB158020BL


Tgt Ion:172 Resp: 1277
Ion Ratio Lower Upper
172 100
171 40.4 32.8 49.2
170 31.7 24.0 36.0

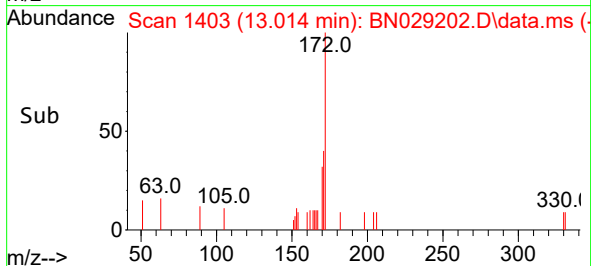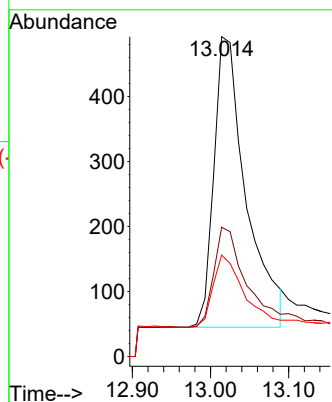

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.144 min Scan# 1768
Delta R.T. 0.012 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31

Tgt Ion:188 Resp: 1339
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 15.3 8.8 13.2#


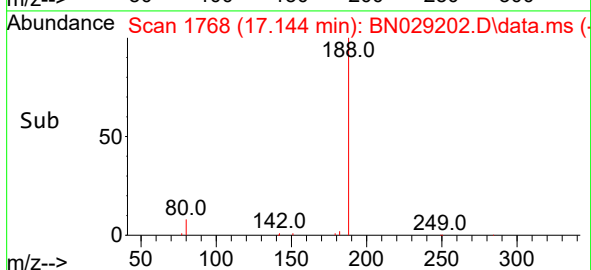
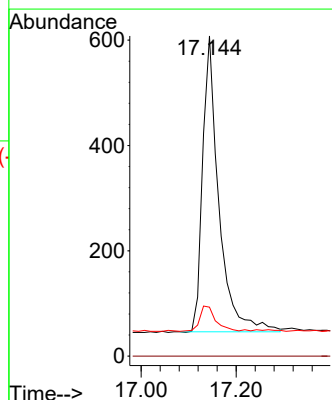
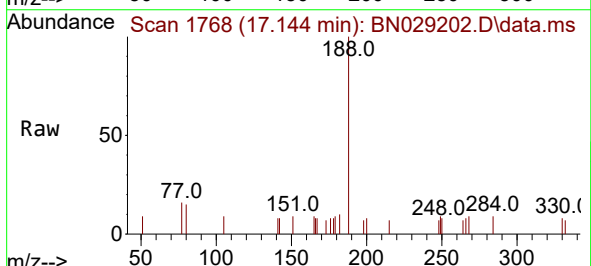




#20
4,6-Dinitro-2-methylphenol
Concen: 0.108 ng
RT: 15.484 min Scan# 1
Delta R.T. -0.046 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31




Instrument :
BNA_N
ClientSampleId :
PB158020BL


Tgt Ion:198 Resp: 3
Ion Ratio Lower Upper
198 100
51 121.7 47.4 71.2#
105 110.9 54.5 81.7#

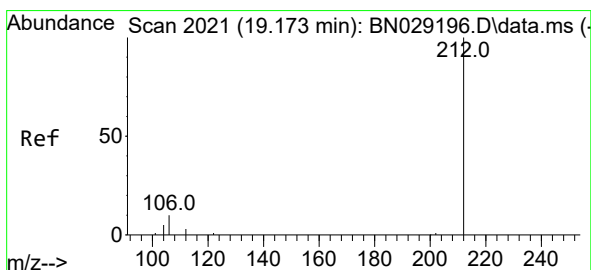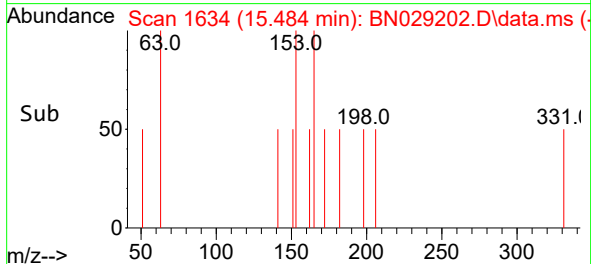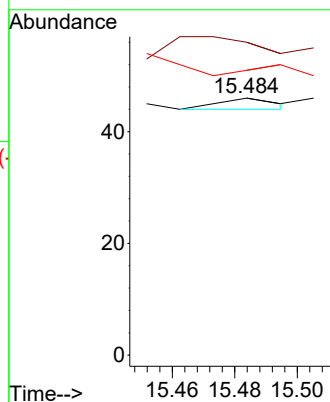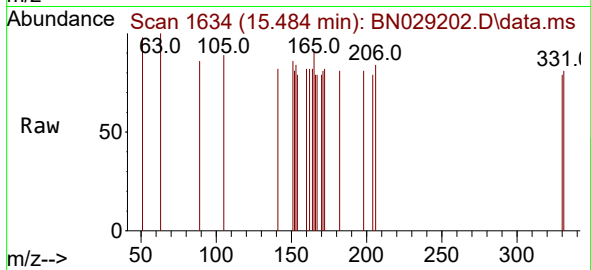

#27
Fluoranthene-d10
Concen: 0.265 ng
RT: 19.178 min Scan# 2022
Delta R.T. 0.005 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31

Tgt Ion:212 Resp: 722
Ion Ratio Lower Upper
212 100
106 11.4 9.7 14.5
104 7.9 6.3 9.5

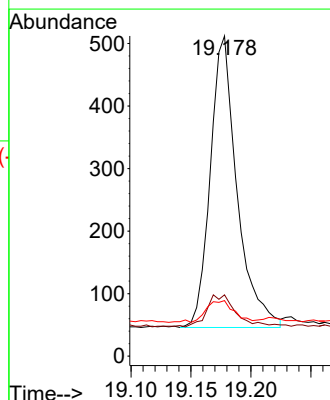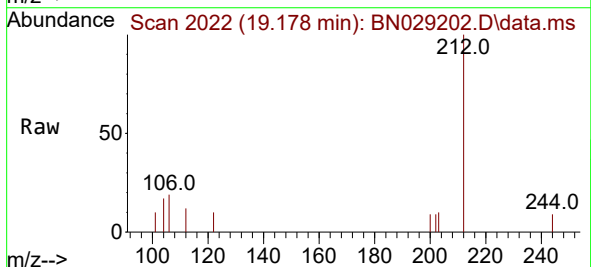

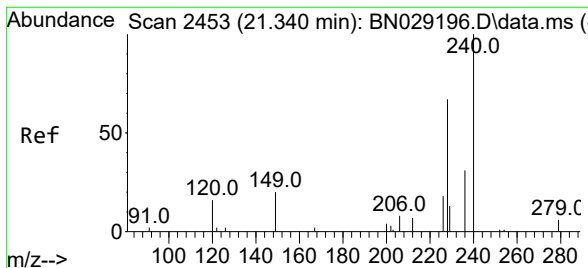

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.349 min Scan# 2454

Delta R.T. 0.009 min

Lab File: BN029202.D

Acq: 27 Dec 2023 16:31

Instrument :

BNA_N

ClientSampleId :

PB158020BL





Tgt Ion:240 Resp: 487

Ion Ratio Lower Upper

240 100

120 33.9 24.6 36.8

236 46.9 32.0 48.0

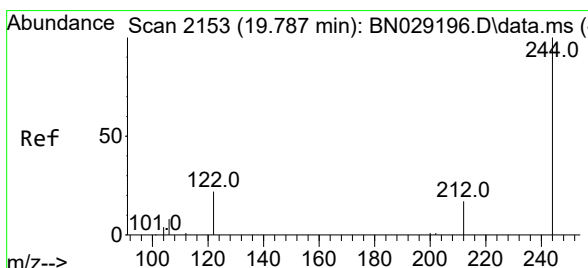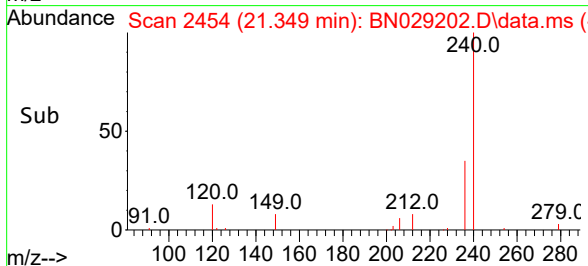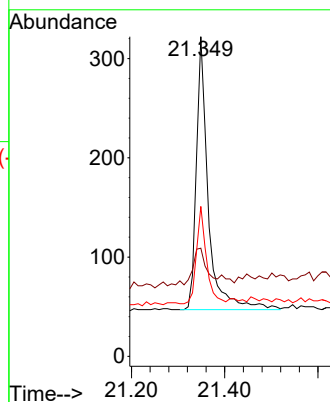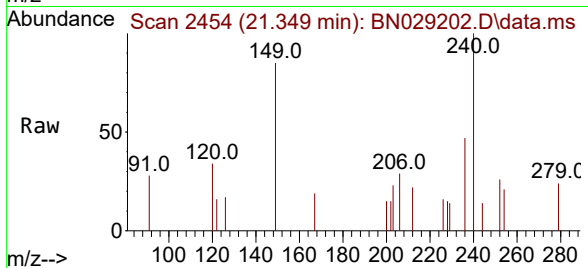

#31

Terphenyl-d14

Concen: 0.300 ng

RT: 19.787 min Scan# 2153

Delta R.T. -0.000 min

Lab File: BN029202.D

Acq: 27 Dec 2023 16:31




Tgt Ion:244 Resp: 453


Ion Ratio Lower Upper

244 100

212 28.9 20.1 30.1

122 34.8 23.9 35.9


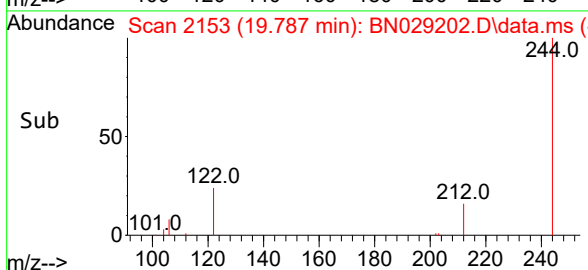
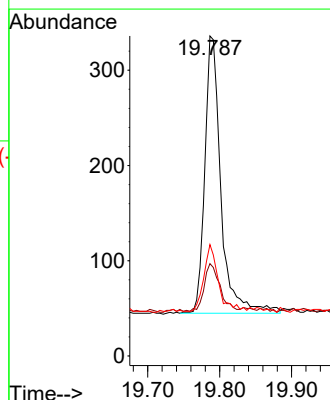
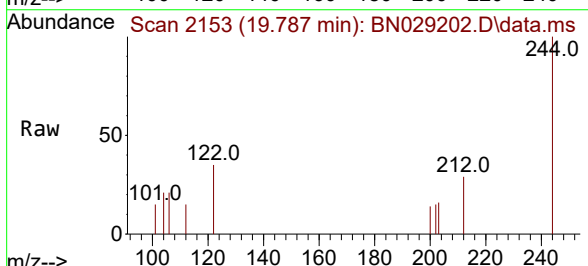


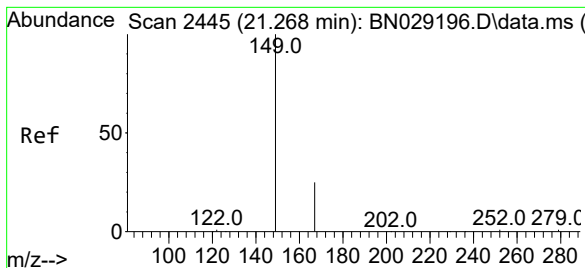

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.026 ng
RT: 21.268 min Scan# 2445
Delta R.T. 0.000 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31

Instrument :
BNA_N
ClientSampleId :
PB158020BL

Tgt Ion:149 Resp: 108
Ion Ratio Lower Upper
149 100
167 19.4 20.7 31.1#
279 6.5 2.4 3.6#

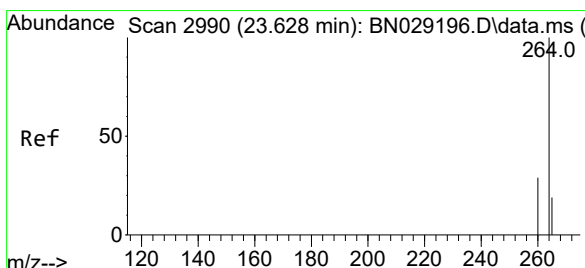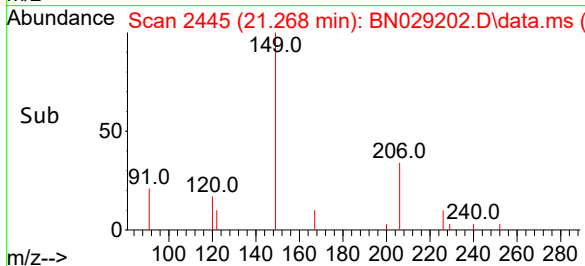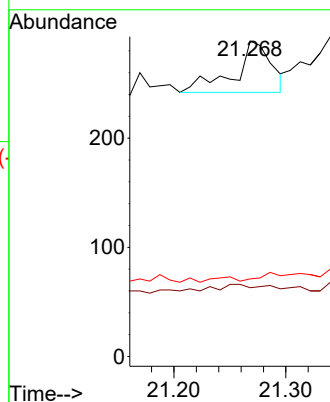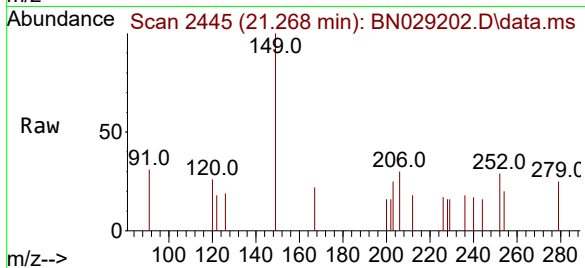

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.636 min Scan# 2993
Delta R.T. 0.009 min
Lab File: BN029202.D
Acq: 27 Dec 2023 16:31

Tgt Ion:264 Resp: 579
Ion Ratio Lower Upper
264 100
260 38.7 30.2 45.4
265 131.2 88.1 132.1

