
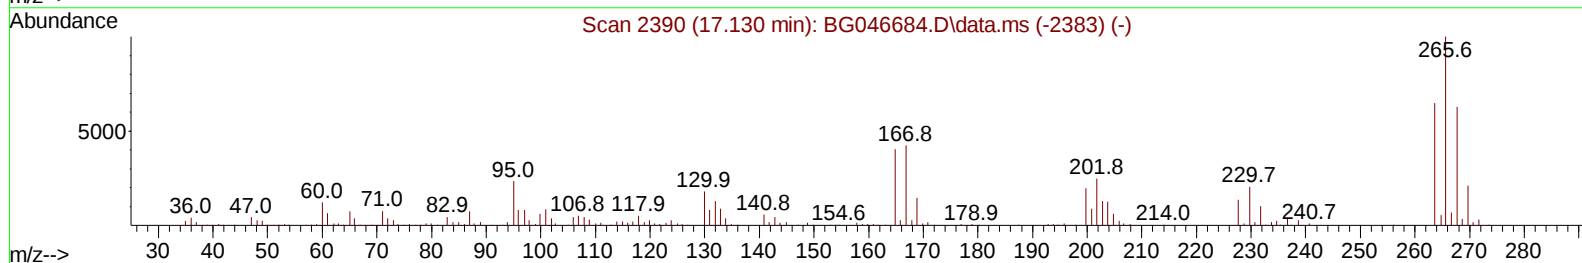
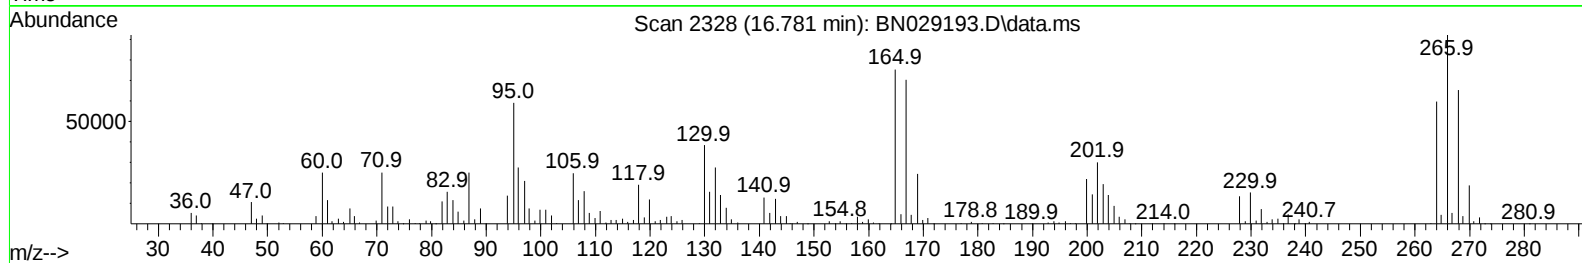


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122723\
Data File : BN029193.D
Acq On : 27 Dec 2023 08:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 04:58:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

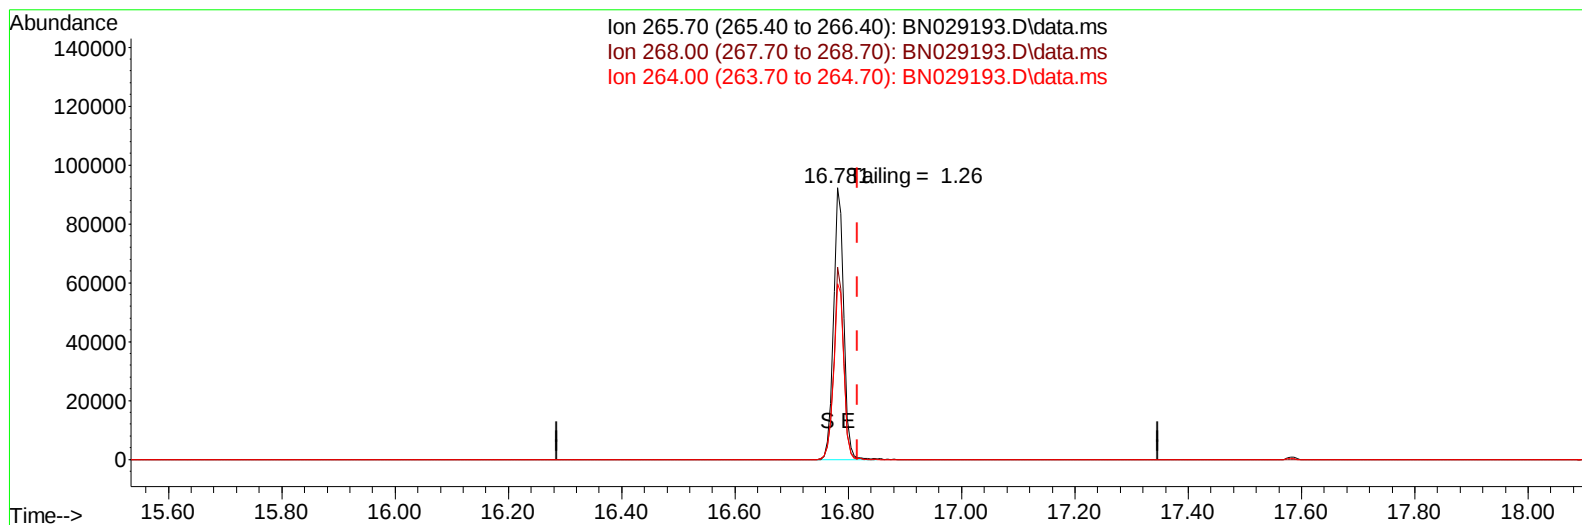

TIC: BN029193.D\data.ms

(70) Pentachlorophenol (C)




16.781min (-0.035) 10055.12 ng

response 115840

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.95
264.00	61.60	64.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122723\
Data File : BN029193.D
Acq On : 27 Dec 2023 08:19
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 04:58:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

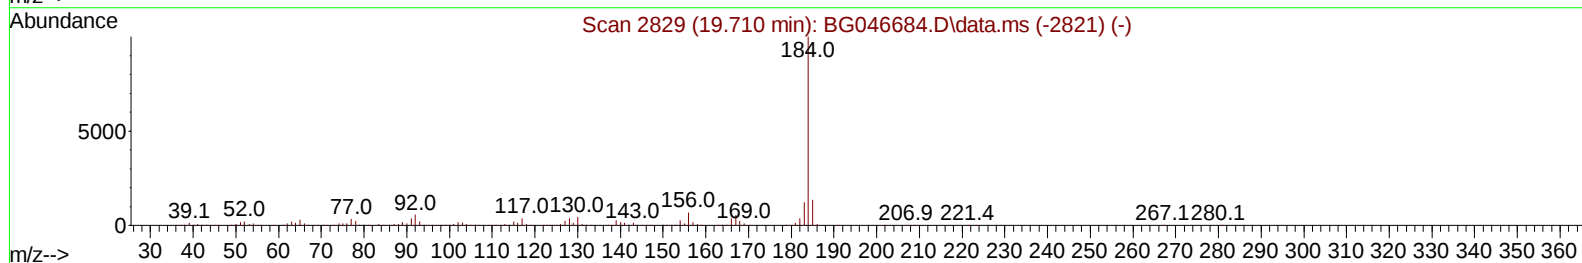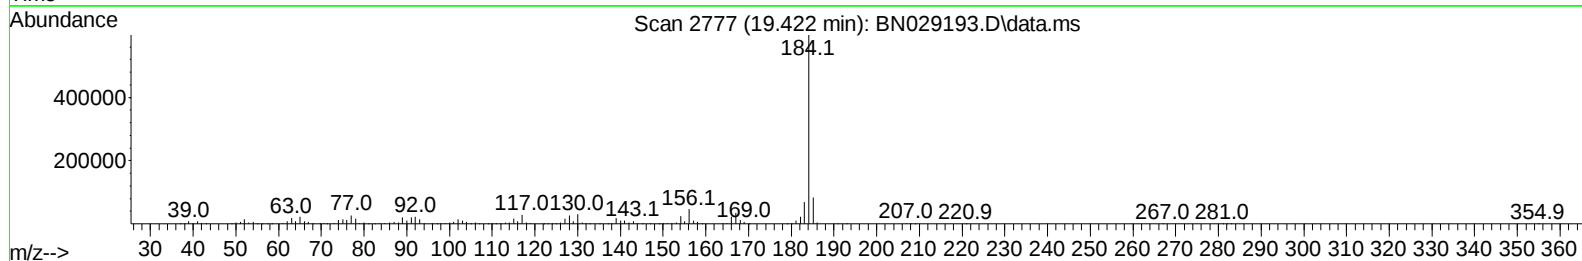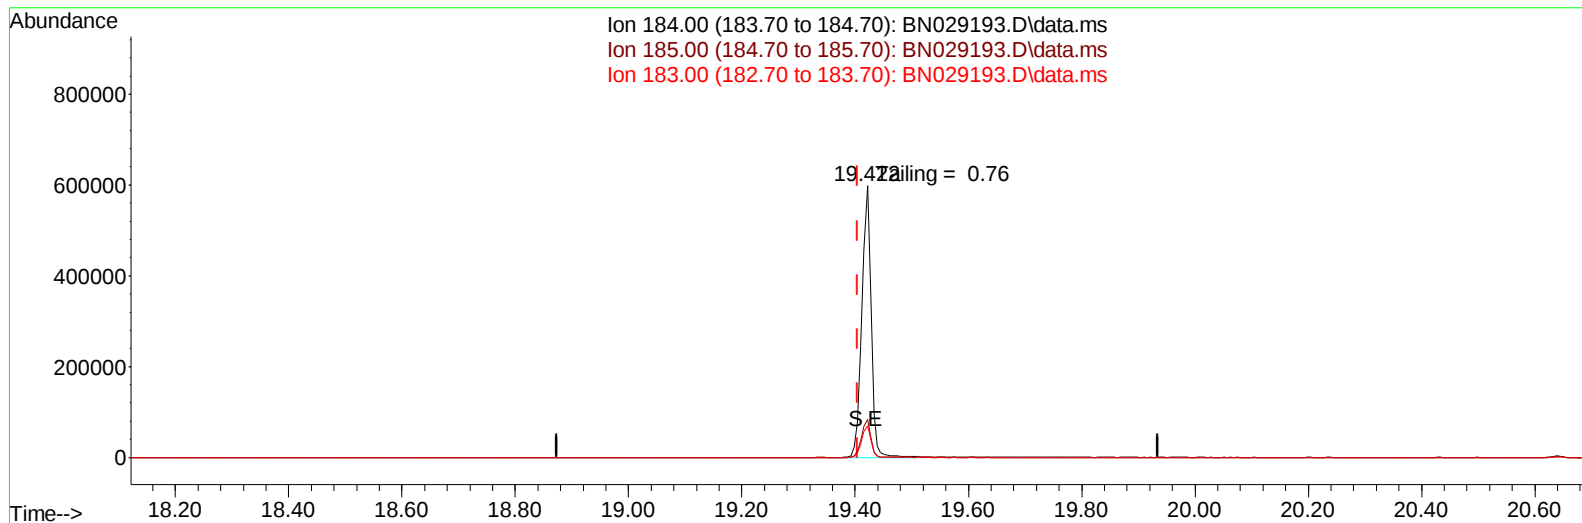

TIC: BN029193.D\data.ms

(77) Benzidine

19.422min (+ 0.018) 0.00 ng

response 677906

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	11.59
0.00	0.00	0.00