

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
 Data File : BN009211.D
 Acq On : 28 Dec 2019 01:05
 Operator : JU
 Sample : K6276-19
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 28 04:26:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 27 23:08:48 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	2262	0.40	ng/ul	0.00
2) Naphthalene-d8	10.27	136	8089	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.14	164	4603	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.89
16) Chrysene-d12	21.09	240	7883	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	8057	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.86	152	3226	0.22	ng/ul	0.00
14) Fluoranthene-d10	18.92	212	8212	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.29	202	1365	0.034	ng/ul#	1
21) Benzo(b)fluoranthene	22.59	252	969	0.026	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
Data File : BN009211.D
Acq On : 28 Dec 2019 01:05
Operator : JU
Sample : K6276-19
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 28 04:26:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 23:08:48 2019
Response via : Initial Calibration

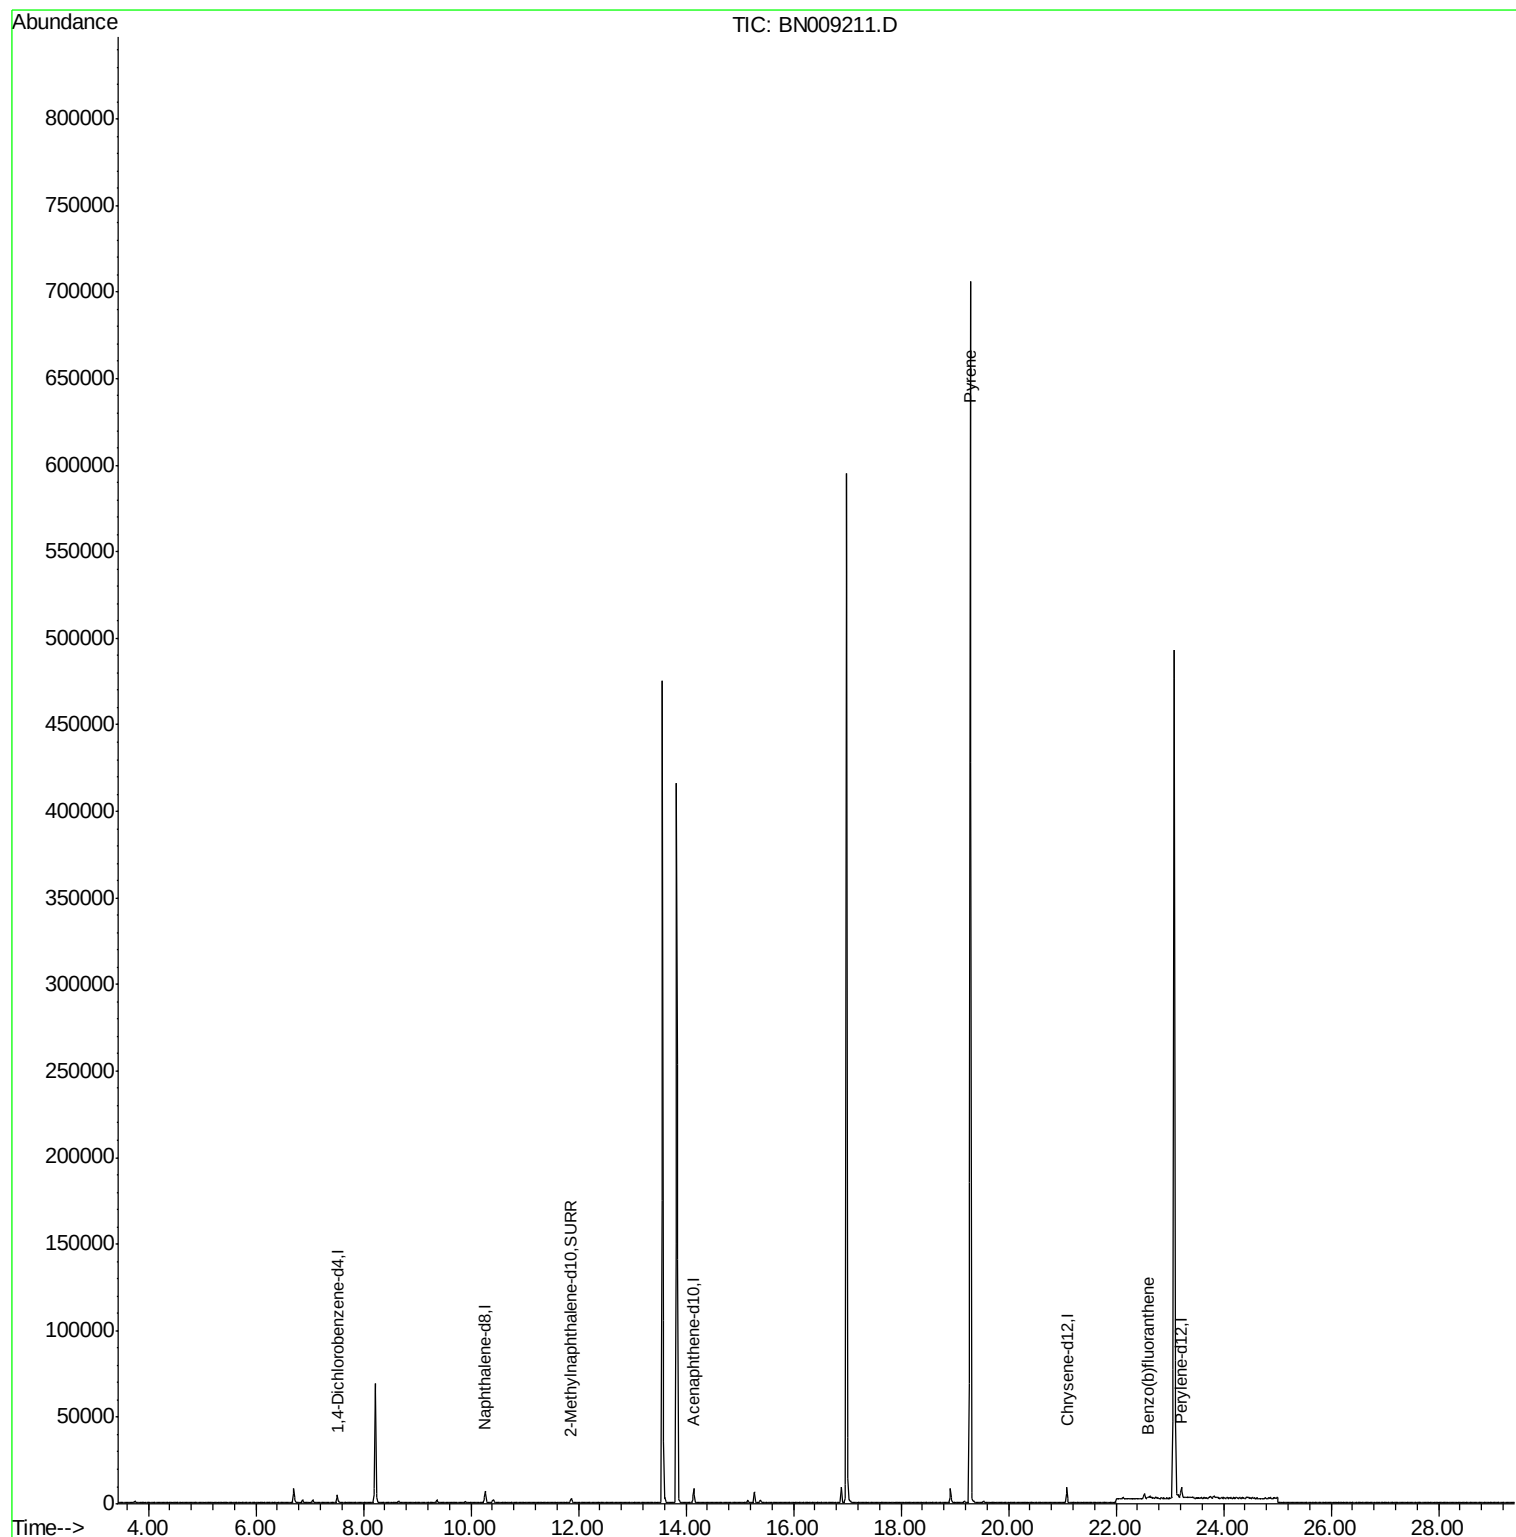


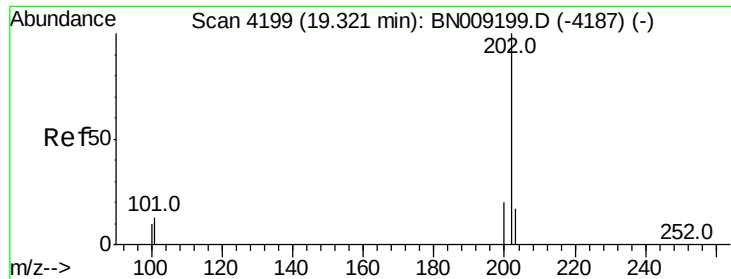




#17
Pvrene
Concen: 0.034 ng/ul
RT: 19.29 min Scan# 4192
Delta R.T. -0.03 min
Lab File: BN009211.D
Acq: 28 Dec 2019 01:05

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 1365
Ion Ratio Lower Upper
202 100
101 169.1 10.9 16.3#
100 1133.0 9.0 13.6#

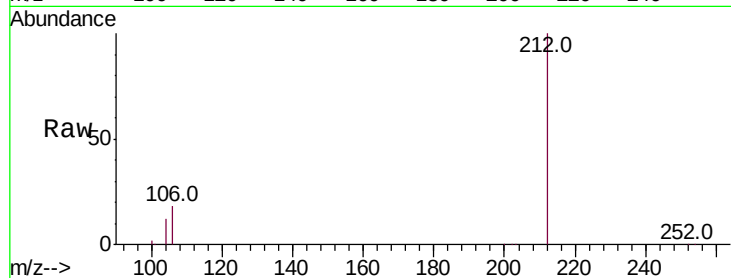


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

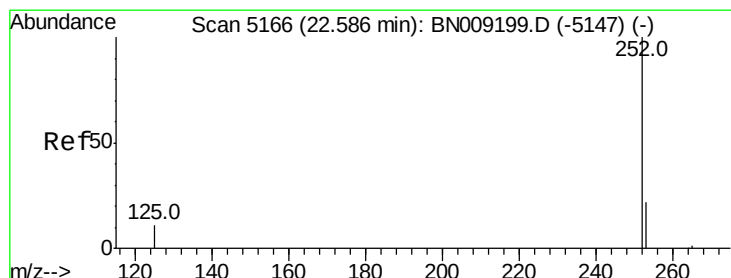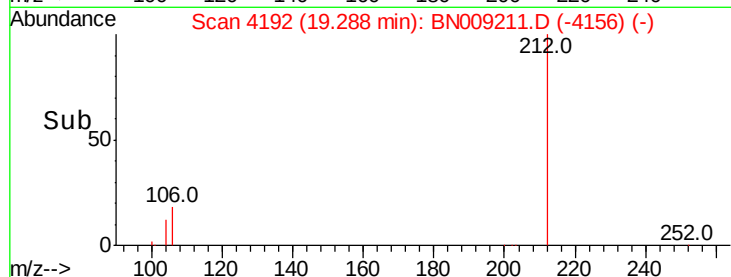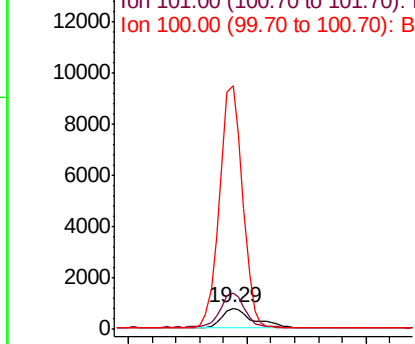

#21
Benzo(b)fluoranthene
Concen: 0.026 ng/ul
RT: 22.59 min Scan# 5166
Delta R.T. -0.00 min
Lab File: BN009211.D
Acq: 28 Dec 2019 01:05

Tgt Ion:252 Resp: 969
Ion Ratio Lower Upper
252 100
253 67.8 0.0 48.2#
125 72.0 0.0 30.0#

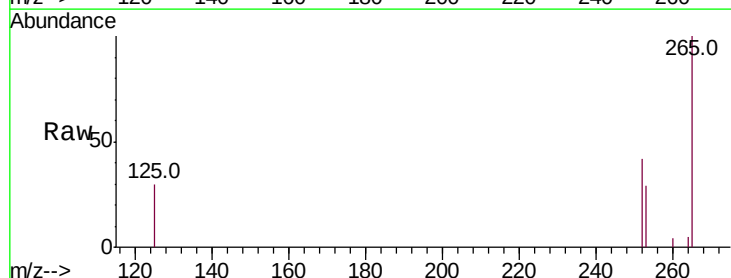

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

