

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
 Data File : BN009212.D
 Acq On : 28 Dec 2019 01:41
 Operator : JU
 Sample : K6276-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 28 04:26:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 27 23:08:48 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	2263	0.40	ng/ul	0.00
2) Naphthalene-d8	10.27	136	8204	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.14	164	4561	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.89
16) Chrysene-d12	21.09	240	7865	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	8024	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.86	152	3398	0.23	ng/ul	0.00
14) Fluoranthene-d10	18.93	212	8533	0.00	ng/ul	0.00
Target Compounds				Ovalue		
9) Fluorene	15.14	166	1143	0.051	ng/ul#	16
17) Pyrene	19.29	202	1368	0.034	ng/ul#	1
21) Benzo(b)fluoranthene	22.59	252	936	0.025	ng/ul#	1
23) Benzo(a)pyrene	23.08	252	2695	0.082	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
Data File : BN009212.D
Acq On : 28 Dec 2019 01:41
Operator : JU
Sample : K6276-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 28 04:26:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 23:08:48 2019
Response via : Initial Calibration

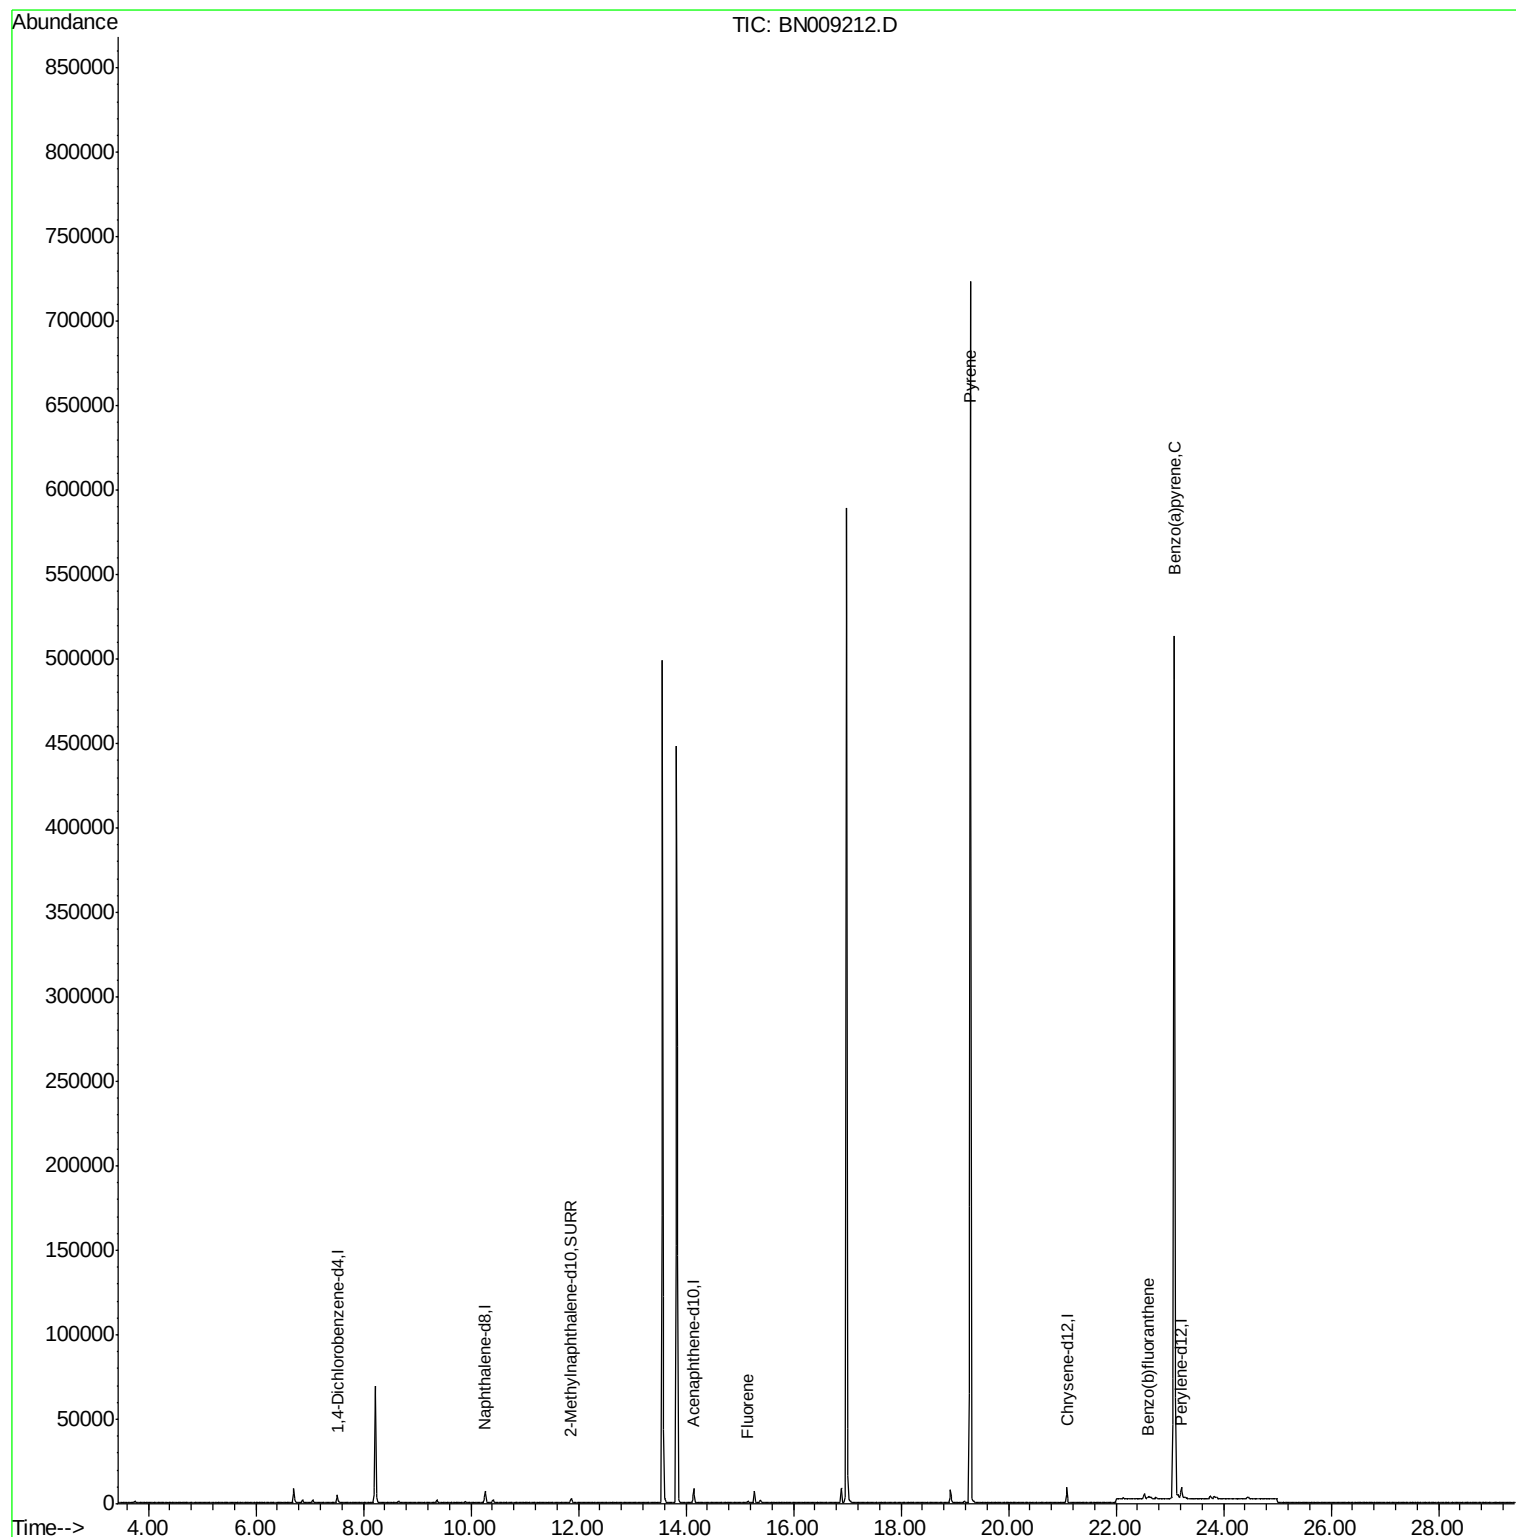

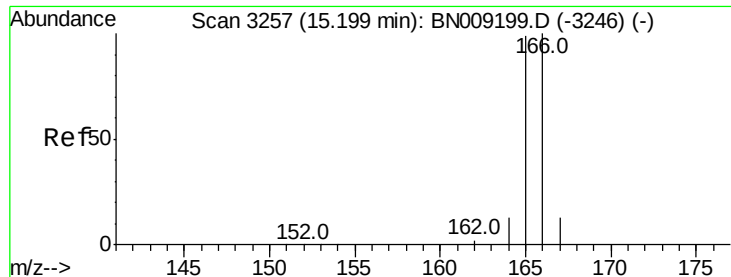

#9

Fluorene

Concen: 0.051 ng/ul

RT: 15.14 min Scan# 3245

Delta R.T. -0.06 min

Lab File: BN009212.D

Acq: 28 Dec 2019 01:41

Instrument :

BNA_N

ClientSampleId :


Tot Ion:166 Resp: 1143

Ion Ratio Lower Upper


166 100

165 11.3 78.2 117.4#



167 36.0 11.0 16.6#

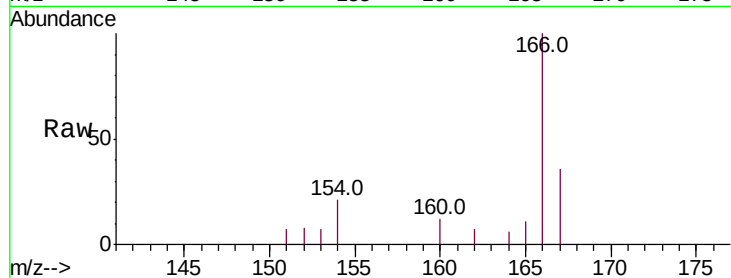

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

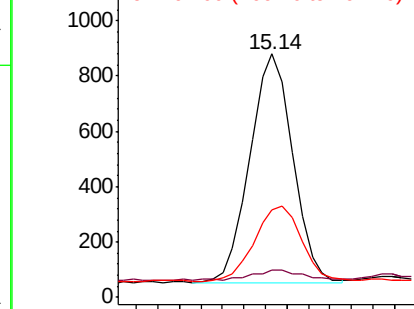

Time-->

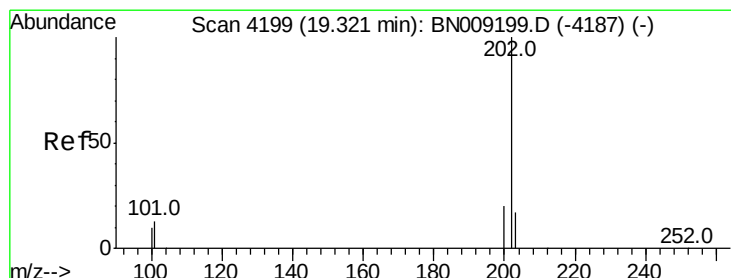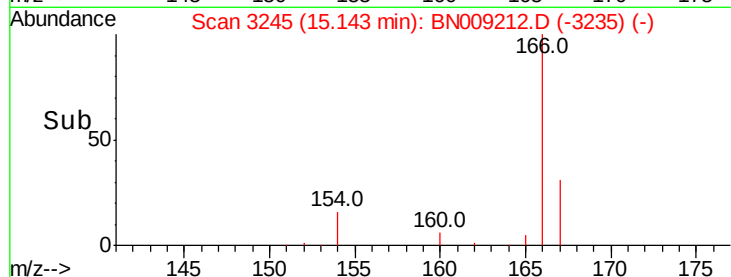

#17

Pyrene

Concen: 0.034 ng/ul

RT: 19.29 min Scan# 4192

Delta R.T. -0.03 min

Lab File: BN009212.D

Acq: 28 Dec 2019 01:41


Tgt Ion:202 Resp: 1368

Ion Ratio Lower Upper


202 100

101 173.4 10.9 16.3#


100 1151.8 9.0 13.6#

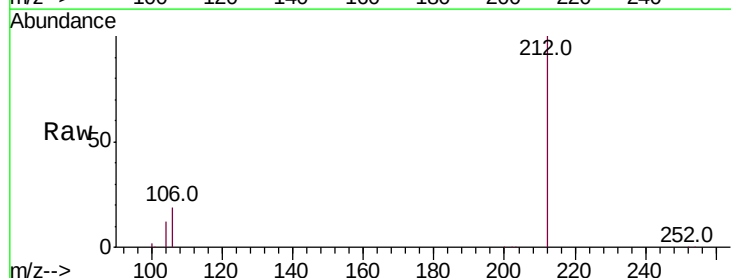


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

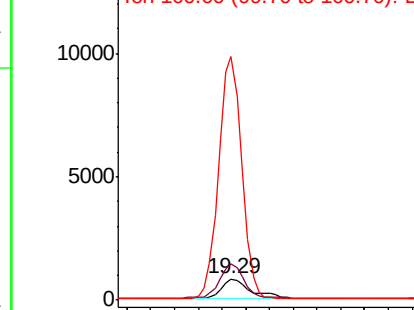

Time-->

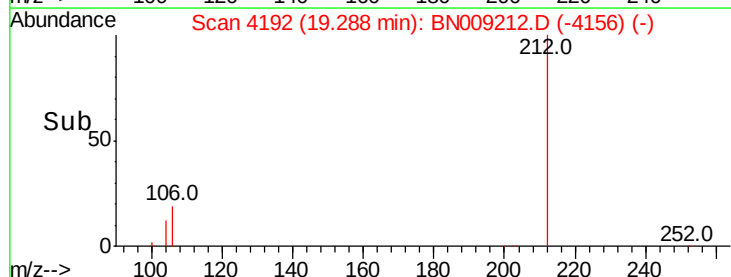

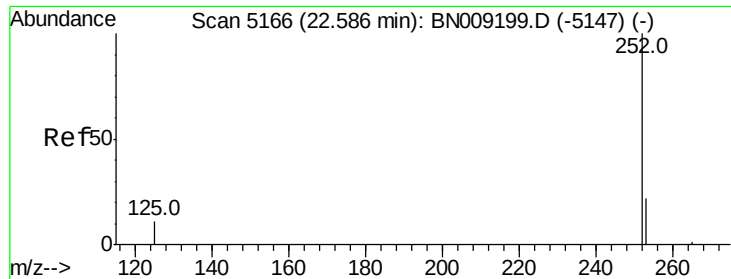

#21

Benzo(b)fluoranthene

Concen: 0.025 ng/ul

RT: 22.59 min Scan# 5166

Delta R.T. -0.00 min

Lab File: BN009212.D

Acq: 28 Dec 2019 01:41

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 936

Ion Ratio Lower Upper

252 100

253 68.9 0.0 48.2#




125 71.0 0.0 30.0#

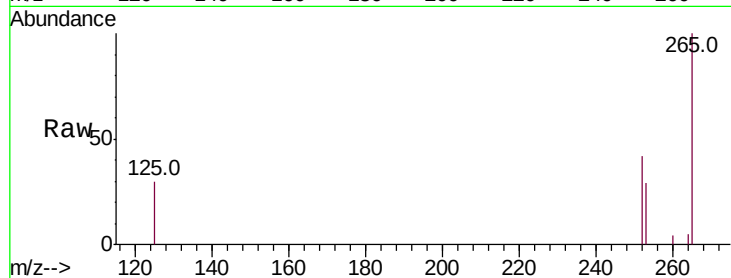

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

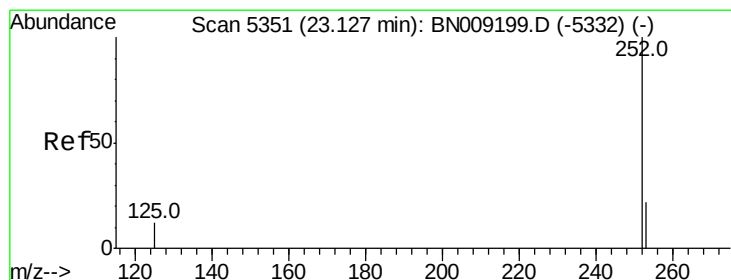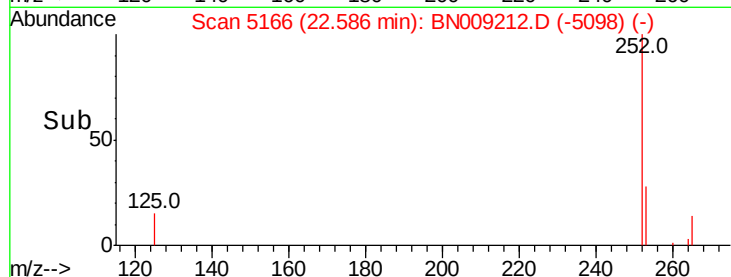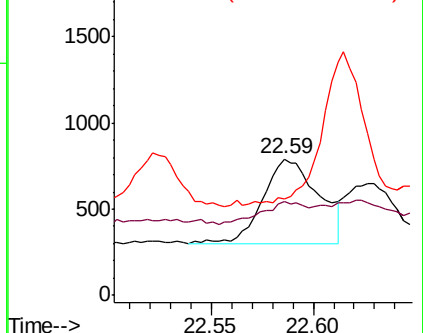

#23

Benzo(a)pyrene

Concen: 0.082 ng/ul

RT: 23.08 min Scan# 5336

Delta R.T. -0.04 min

Lab File: BN009212.D

Acq: 28 Dec 2019 01:41


Tgt Ion:252 Resp: 2695

Ion Ratio Lower Upper

252 100

253 47.9 20.2 30.4#

125 47.9 13.2 19.8#

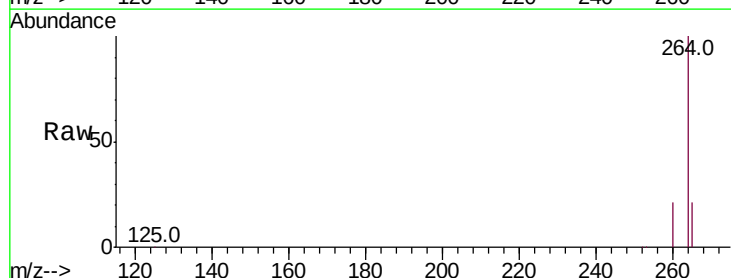

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

