

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
Data File : BN009200.D
Acq On : 27 Dec 2019 18:28
Operator : JU
Sample : PB125532BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK32

Manual Integrations
APPROVED

mohammad
12/29/2019 5:30:42 PM

Quant Time: Dec 29 07:52:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 23:08:48 2019
Response via : Initial Calibration

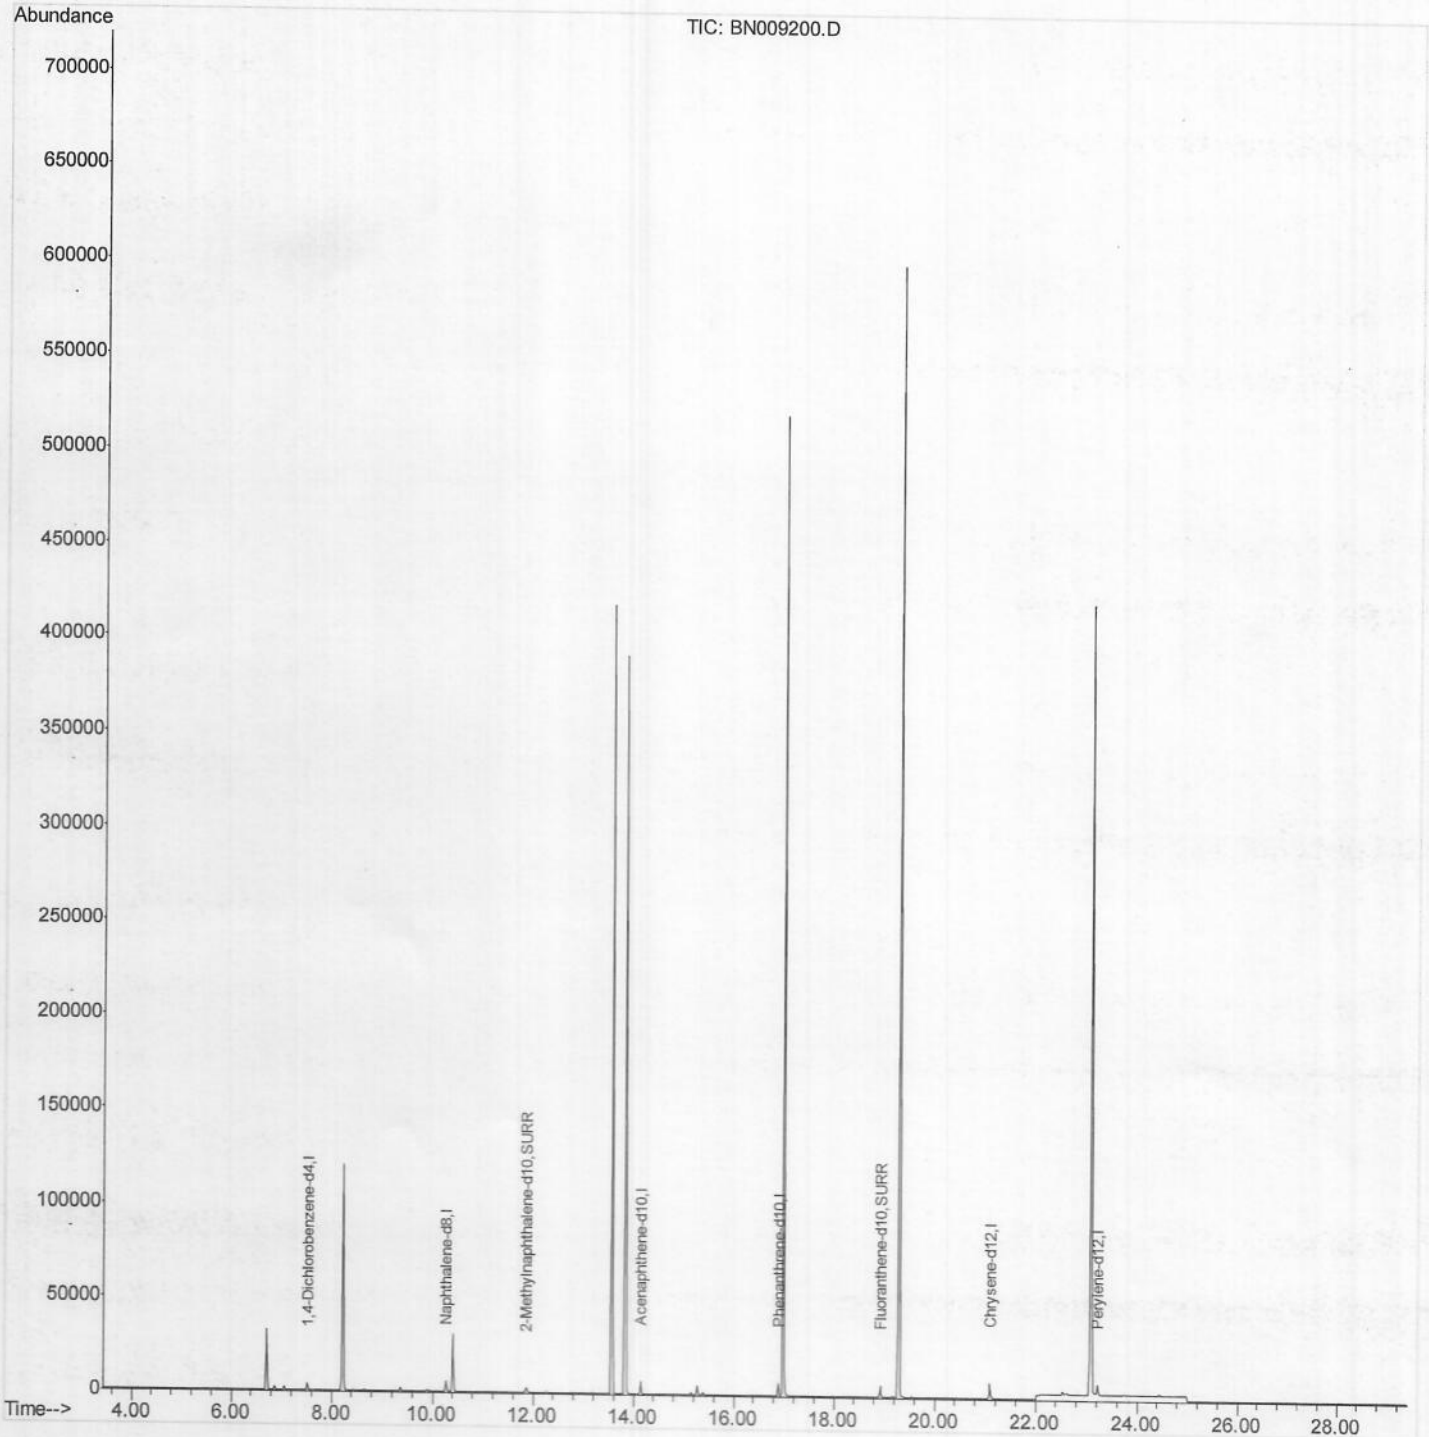

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
 Data File : BN009200.D
 Acq On : 27 Dec 2019 18:28
 Operator : JU
 Sample : PB125532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK32

Manual Integrations
 APPROVED

mohammad
 12/29/2019 5:30:42 PM

Quant Time: Dec 27 23:11:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 27 23:08:48 2019
 Response via : Initial Calibration

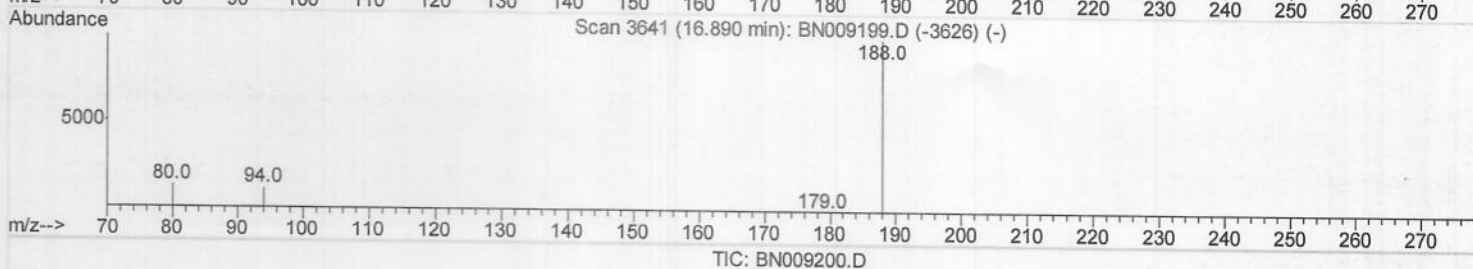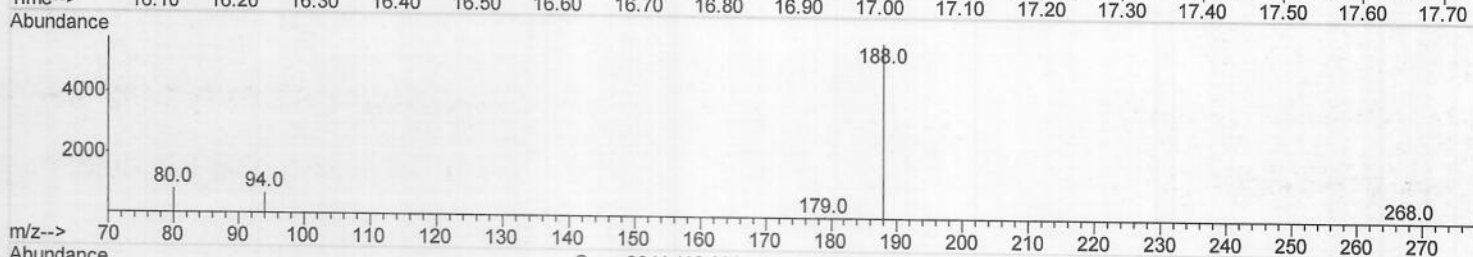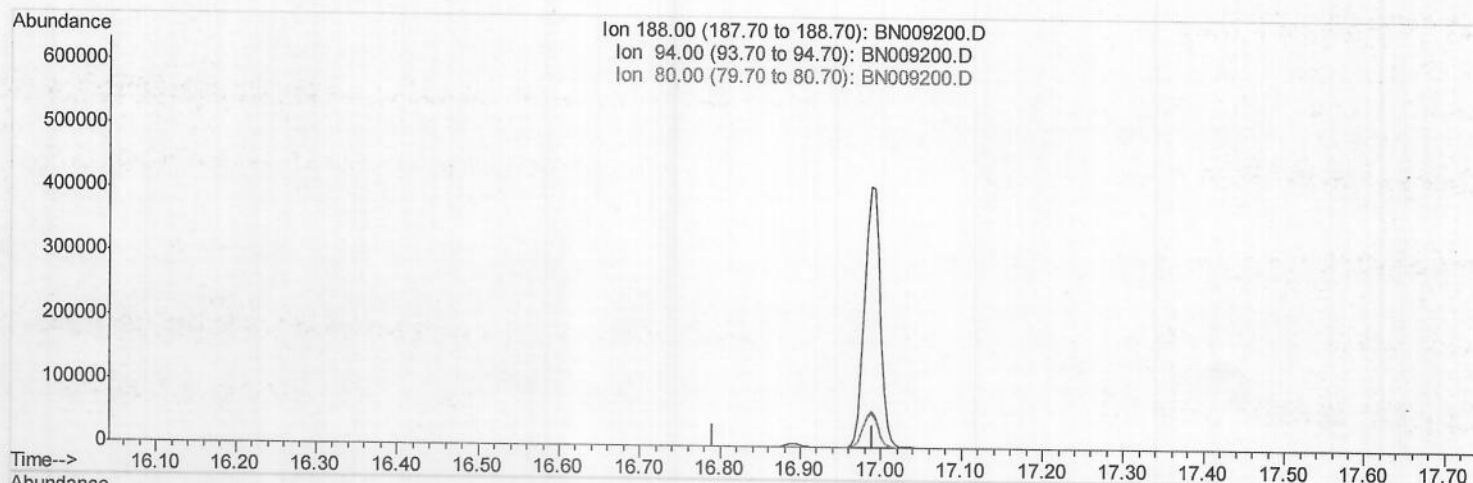

TIC: BN009200.D

(10) Phenanthrene-d10 (I)

16.890min (-16.890) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
 Data File : BN009200.D
 Acq On : 27 Dec 2019 18:28
 Operator : JU
 Sample : PB125532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 SBLK32

Manual Integrations
 APPROVED

mohammad
 12/29/2019 5:30:42 PM

Quant Time: Dec 27 23:11:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 27 23:08:48 2019
 Response via : Initial Calibration

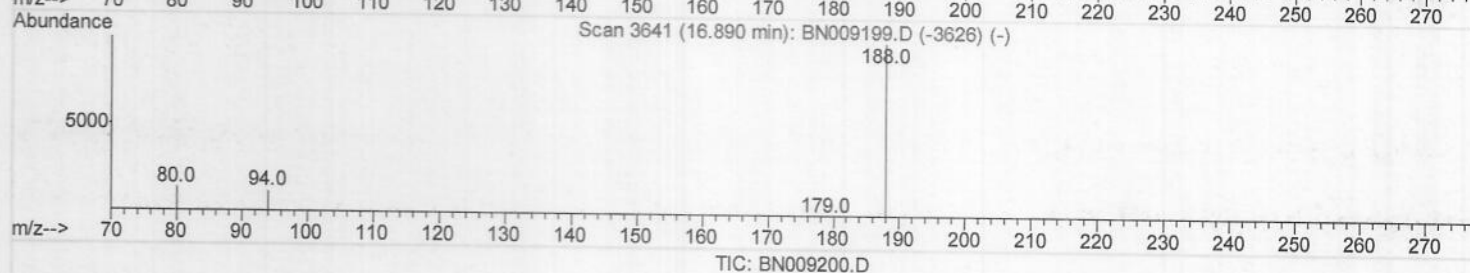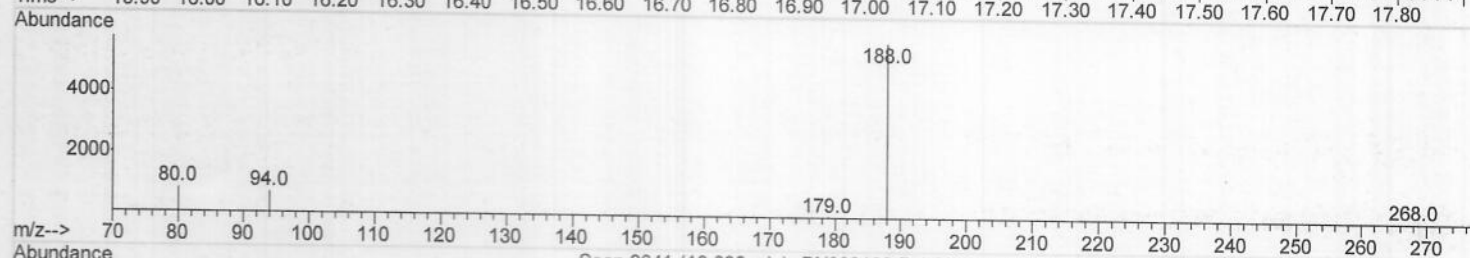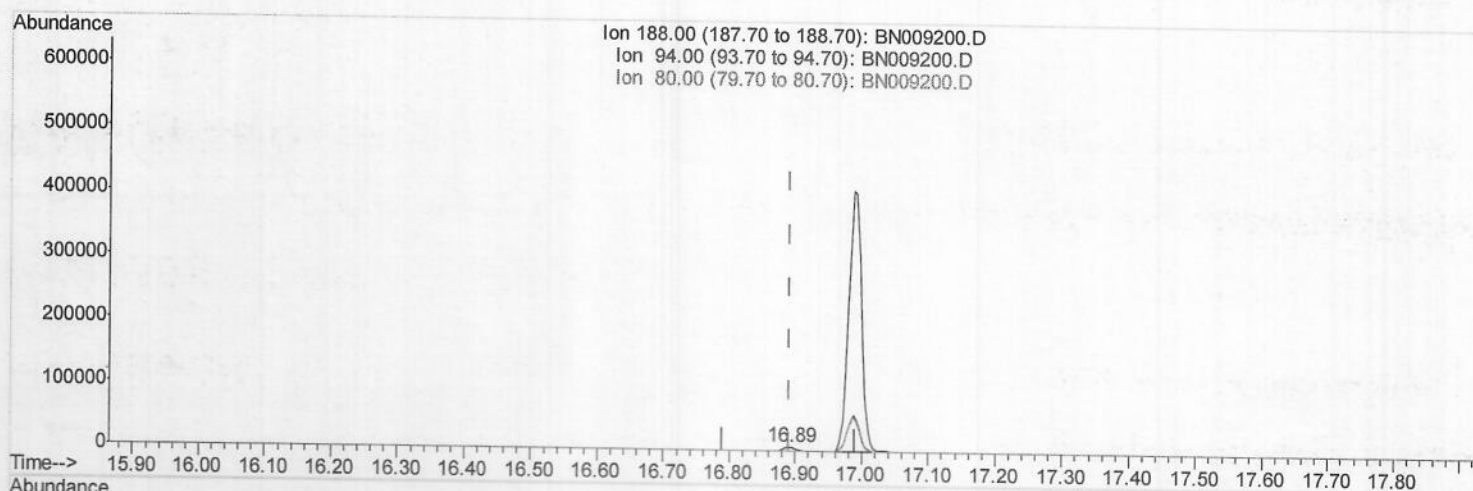

(10) Phenanthrene-d10 (I)

16.890min (-0.000) 0.40ng/ul m) > JU 12/29/19

response 8042

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	12.59
80.00	13.70	14.63
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
 Data File : BN009200.D
 Acq On : 27 Dec 2019 18:28
 Operator : JU
 Sample : PB125532BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK32

Manual Integrations
 APPROVED

mohammad
 12/29/2019 5:30:42 PM

Quant Time: Dec 29 07:52:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 27 23:08:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	1862	0.40	ng/ul	0.00
2) Naphthalene-d8	10.27	136	6661	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.14	164	3809	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.89	188	8042m	0.40	ng/ul	0.00
16) Chrysene-d12	21.09	240	6850	0.40	ng/ul	0.00
20) Perylene-d12	23.22	264	6686	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.86	152	3291	0.28	ng/ul	0.00
14) Fluoranthene-d10	18.93	212	6743	0.28	ng/ul	0.00

Target Compounds

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 12/29/19