


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
Data File : BN009220.D
Acq On : 28 Dec 2019 10:19
Operator : JU
Sample : PB125494BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 29 06:30:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 29 06:16:40 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK94

Manual Integrations
APPROVED

mohammad
12/29/2019 5:31:52 PM

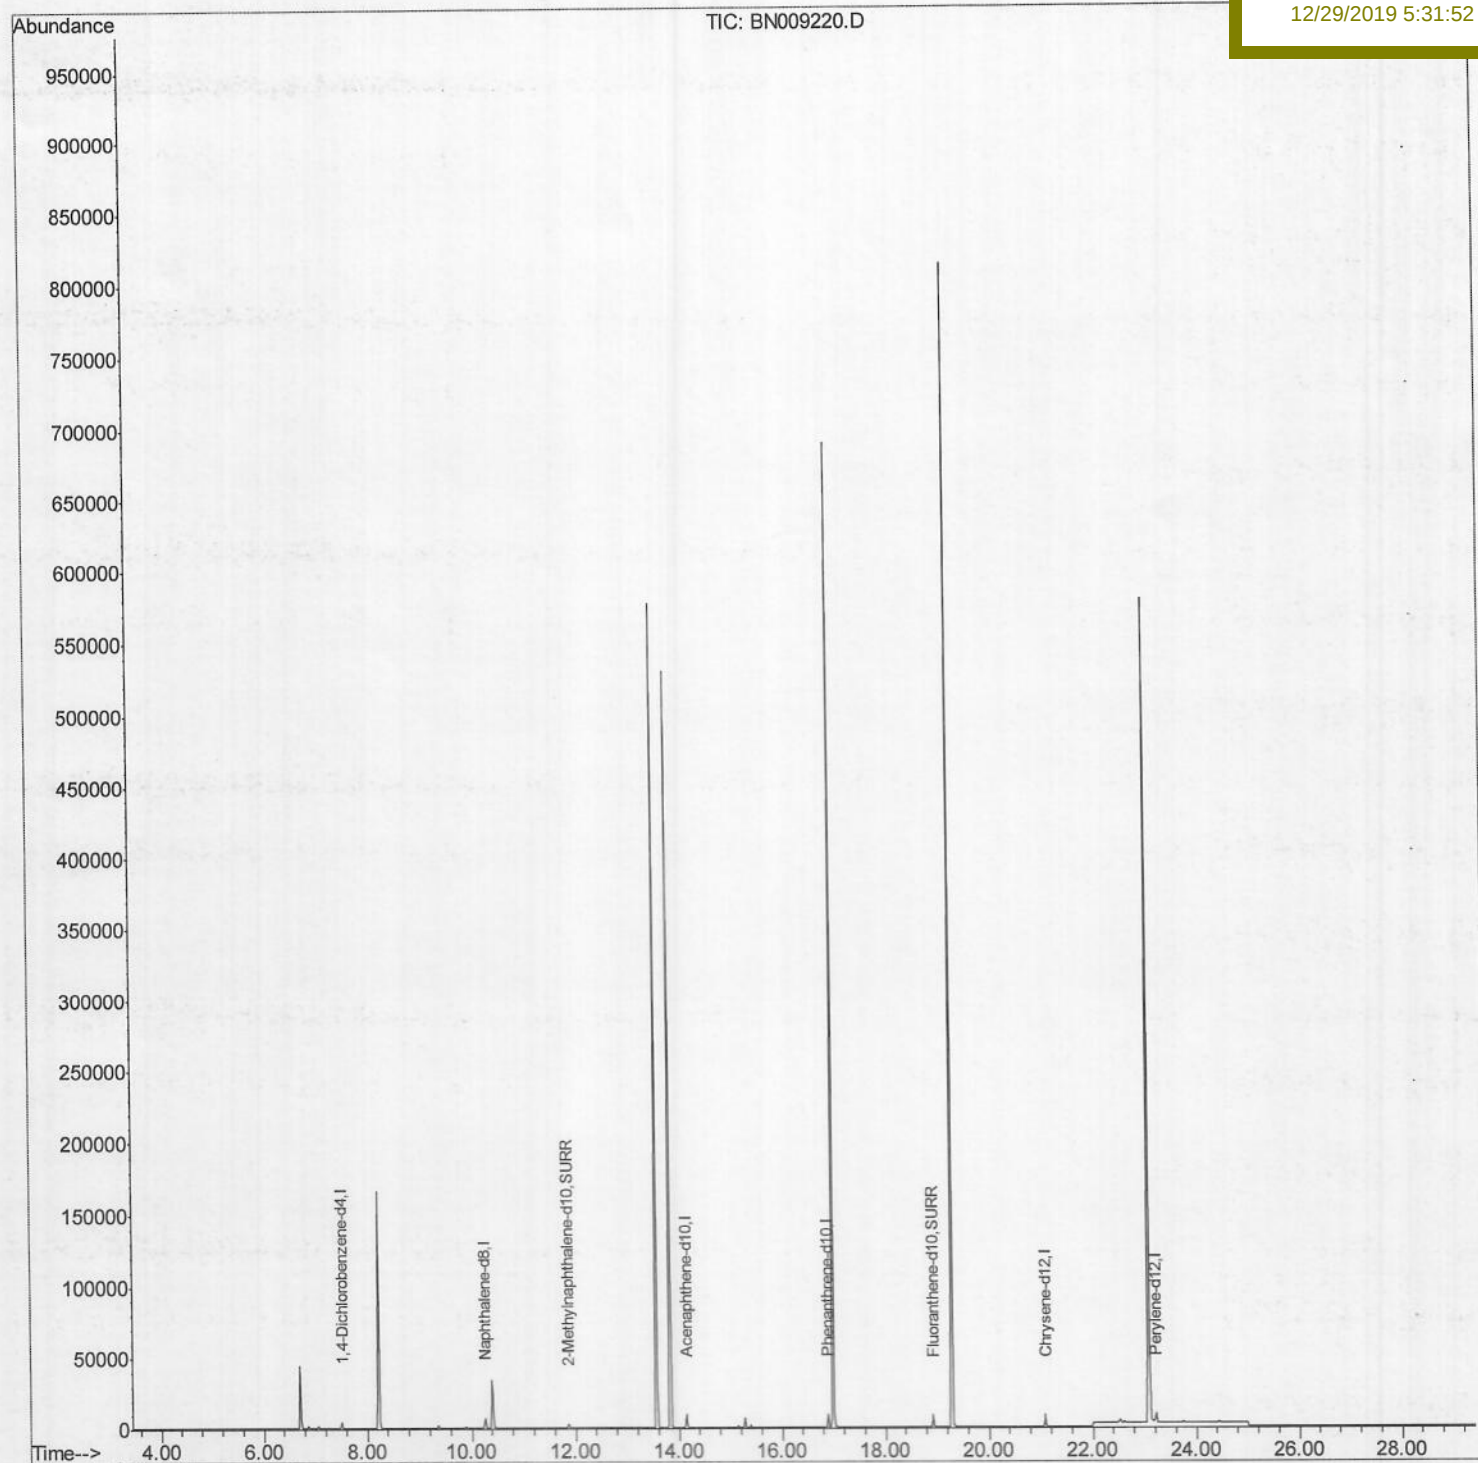

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\

Data File : BN009220.D

Acq On : 28 Dec 2019 10:19

Operator : JU

Sample : PB125494BL

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 29 06:19:18 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Dec 29 06:16:40 2019

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

SBLK94

Manual Integrations
APPROVED

mohammad

12/29/2019 5:31:52 PM

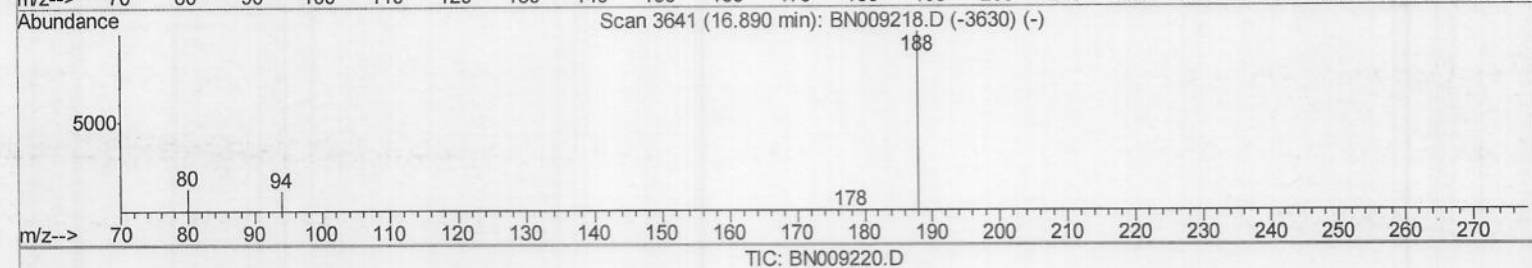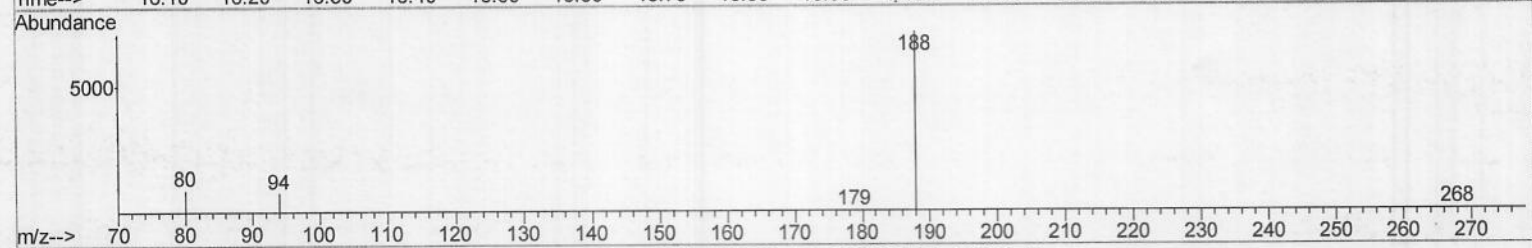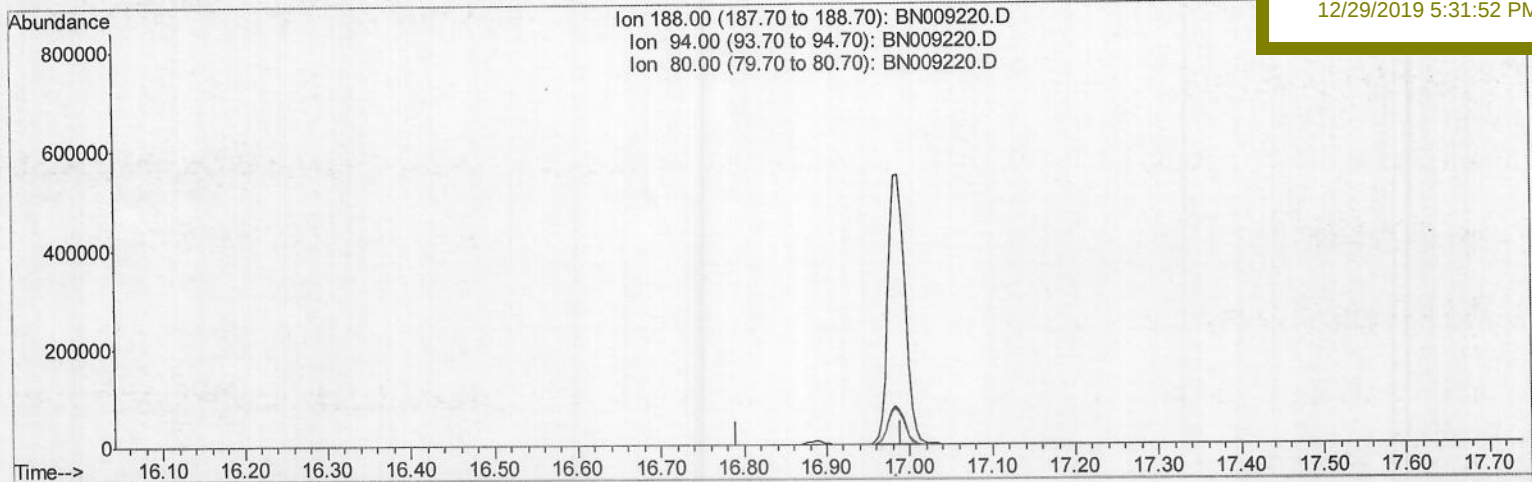

(10) Phenanthrene-d10 (I)

16.890min (-16.890) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\

Data File : BN009220.D

Acq On : 28 Dec 2019 10:19

Operator : JU

Sample : PB125494BL

Misc :

ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 29 06:19:18 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Dec 29 06:16:40 2019




Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

SBLK94

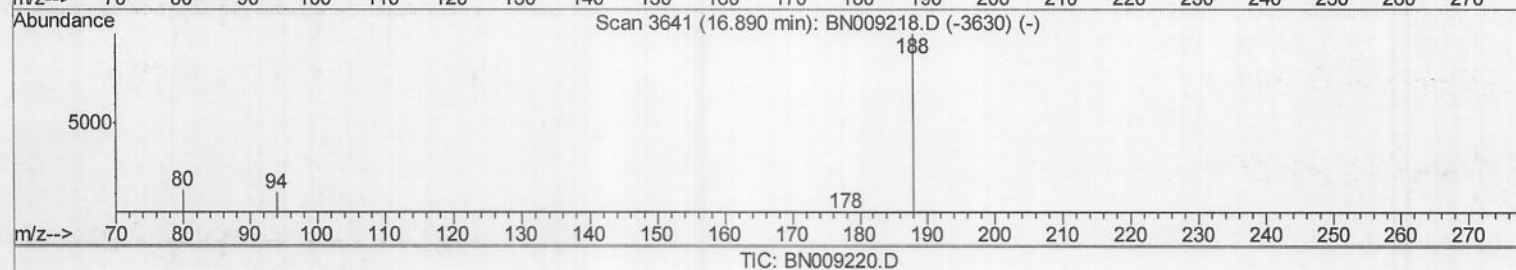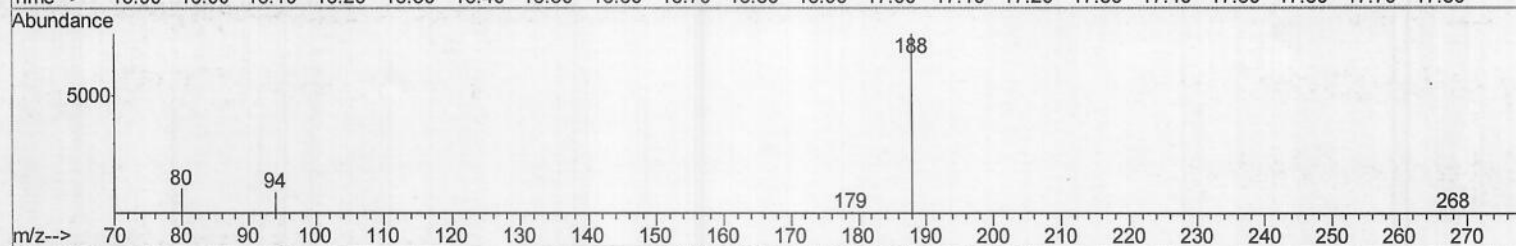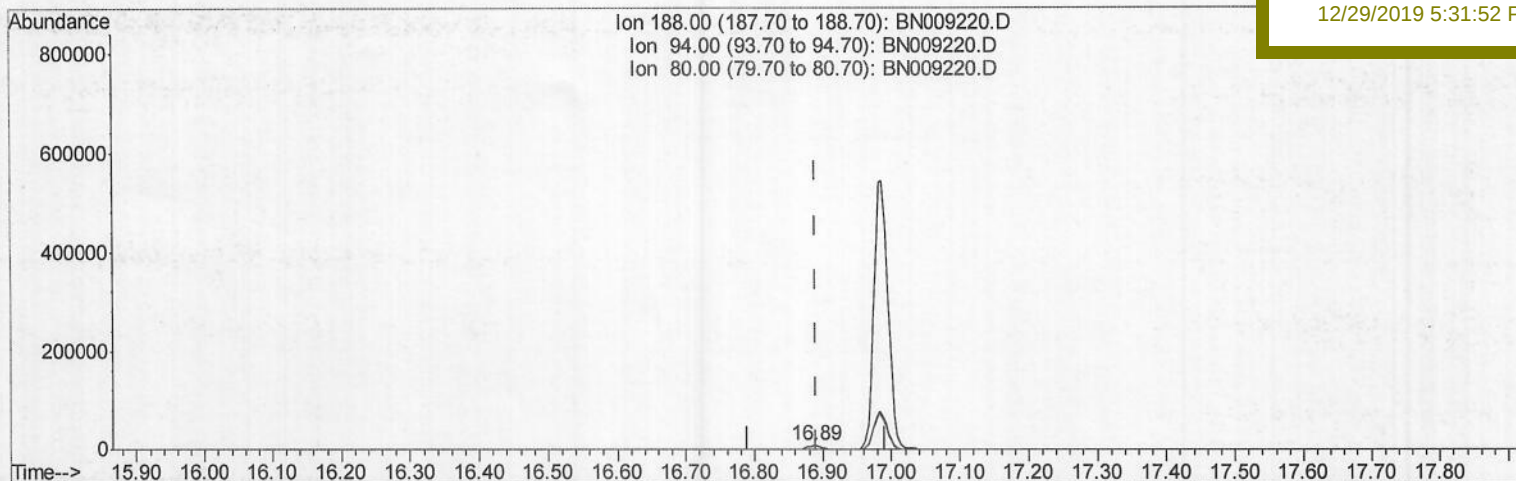Manual Integrations
APPROVEDmohammad
12/29/2019 5:31:52 PM

(10) Phenanthrene-d10 (I)

16.886min (-0.004) 0.40ng/ul m

response 10038

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	12.18
80.00	13.70	13.92
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122819\
Data File : BN009220.D
Acq On : 28 Dec 2019 10:19
Operator : JU
Sample : PB125494BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 29 06:30:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 29 06:16:40 2019
Response via : Initial Calibration

Instrument :
BNA_N
Client Sample ID :
SBLK94

Manual Integrations
APPROVED

mohammad
12/29/2019 5:31:52 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	2454	0.40	ng/ul	0.00
2) Naphthalene-d8	10.26	136	8995	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.14	164	4942	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.89	188	10038m	0.40	ng/ul	0.00
16) Chrysene-d12	21.09	240	7889	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	8293	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.86	152	4485	0.28	ng/ul	0.00
14) Fluoranthene-d10	18.92	212	9380	0.32	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 12/30/19