


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122822\
Data File : BN023517.D
Acq On : 28 Dec 2022 11:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 29 04:01:06 2022

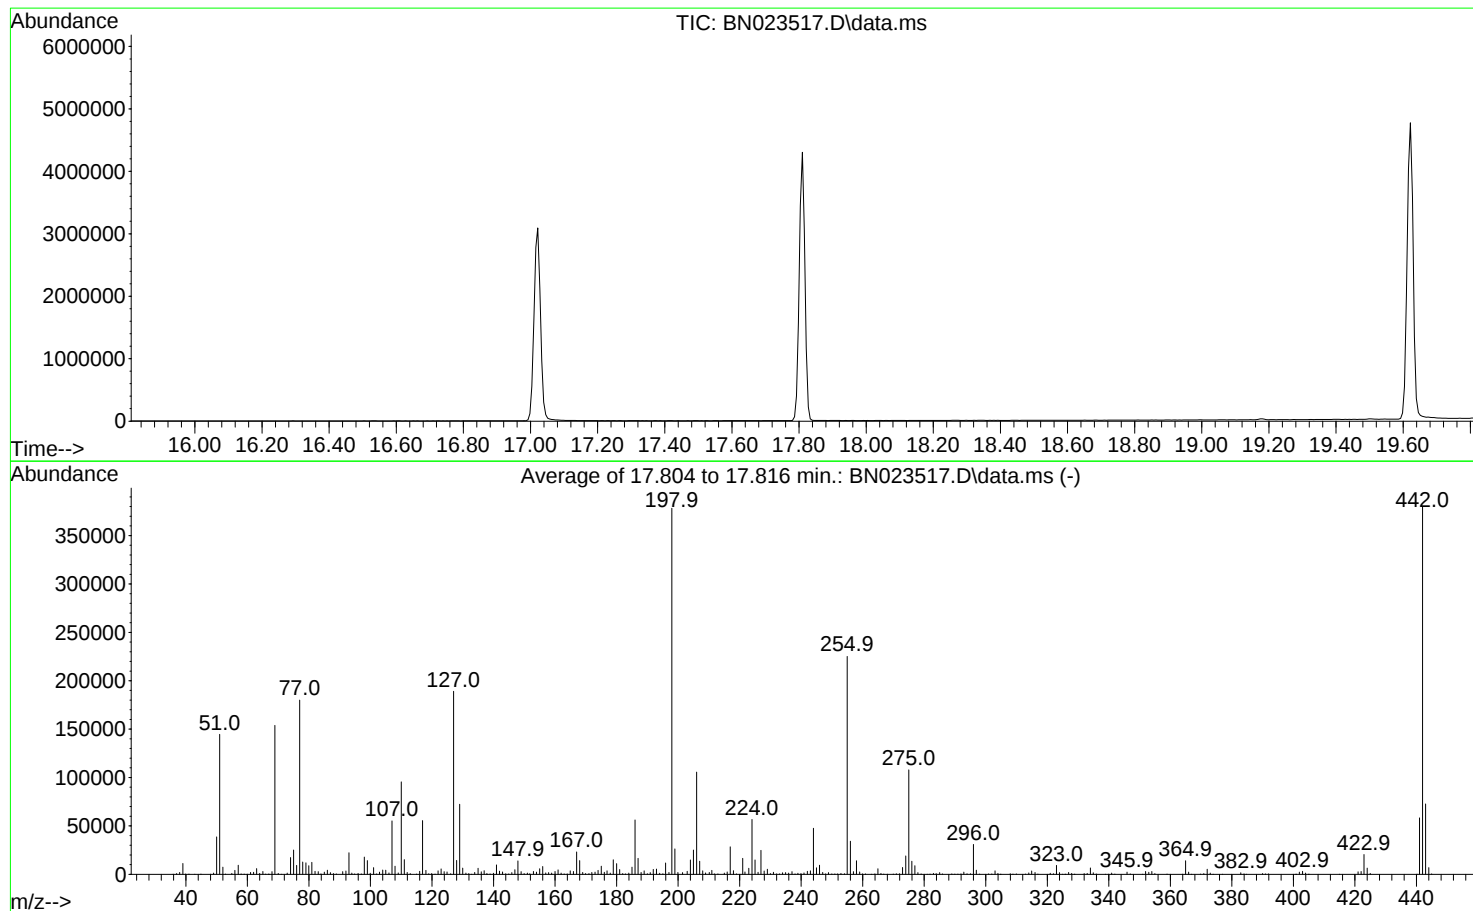




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	144600	PASS
68	69	0.00	2	1.8	2740	PASS
69	198	0.00	100	40.7	153816	PASS
70	69	0.00	2	0.5	843	PASS
127	198	10	80	50.0	189013	PASS
197	198	0.00	2	0.5	1963	PASS
198	198	100	100	100.0	378283	PASS
199	198	5	9	6.9	26280	PASS
275	198	10	60	28.5	107947	PASS
365	198	1	100	3.7	13946	PASS
441	198	0.01	100	15.4	58264	PASS
442	442	50	100	100.0	380160	PASS
443	442	15	24	19.1	72717	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122822\
 Data File : BN023517.D
 Acq On : 28 Dec 2022 11:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 29 04:49:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 29 04:49:33 2022
 Response via : Initial Calibration

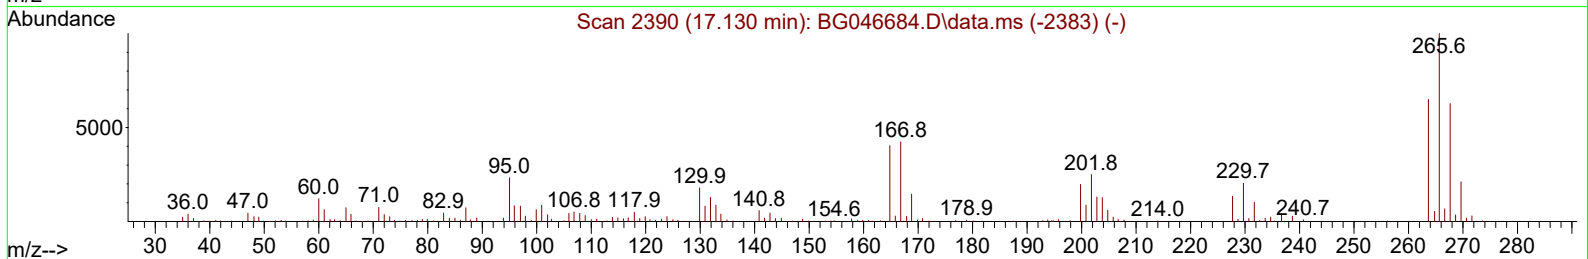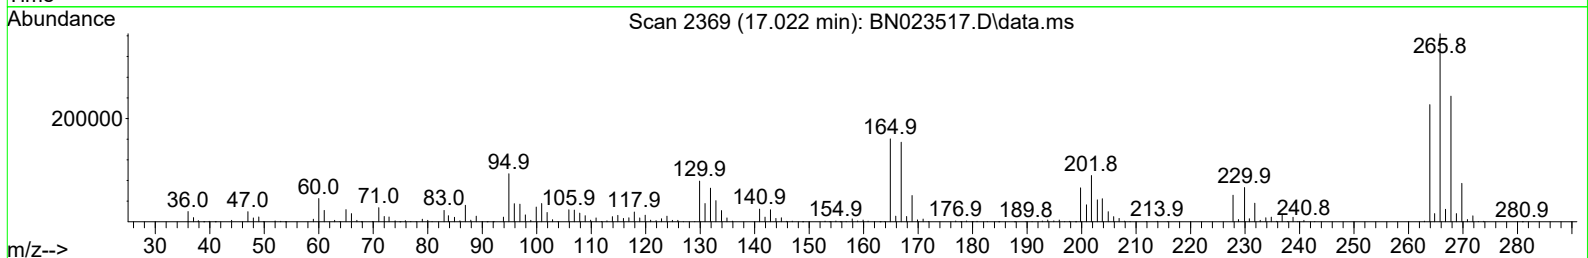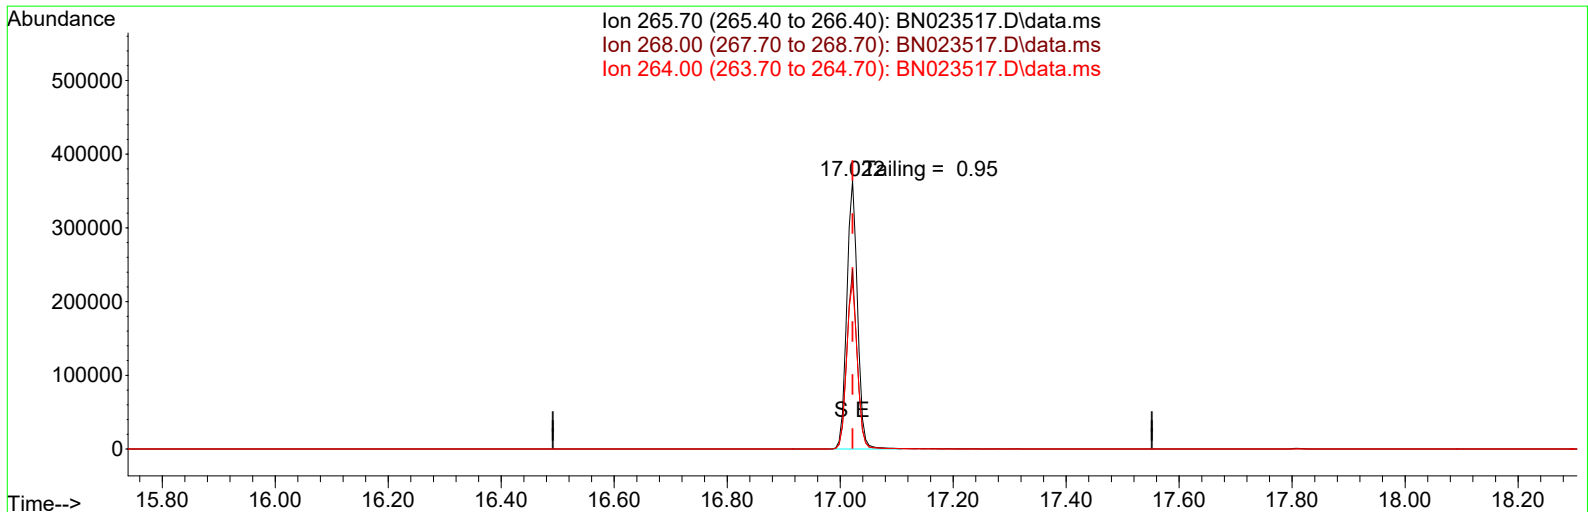

TIC: BN023517.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 22015.60 ng




response 480827

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.87
264.00	61.60	62.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122822\
Data File : BN023517.D
Acq On : 28 Dec 2022 11:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 29 04:49:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 29 04:49:33 2022
Response via : Initial Calibration

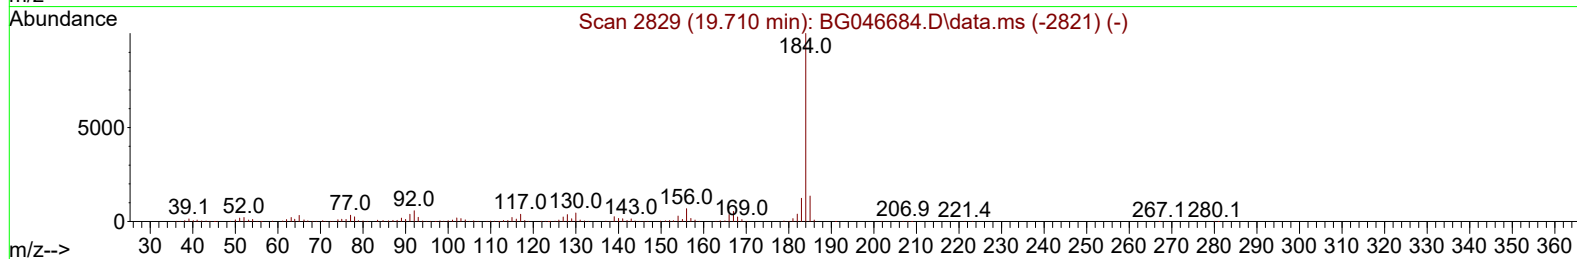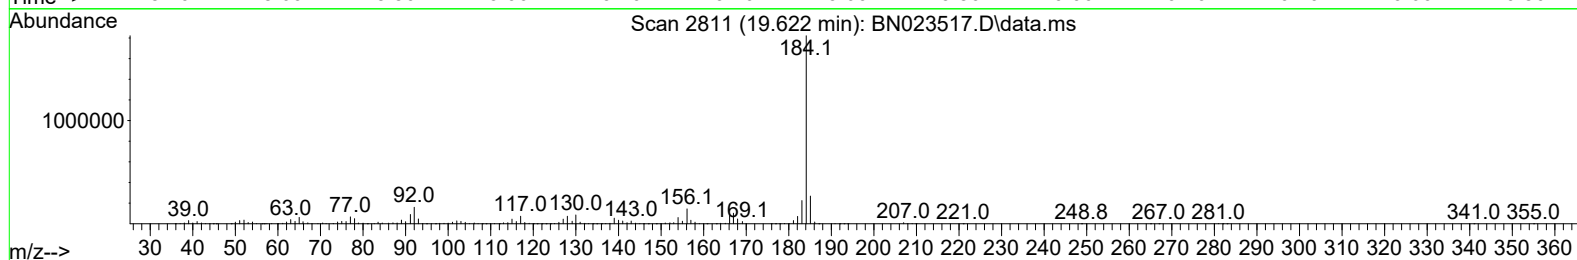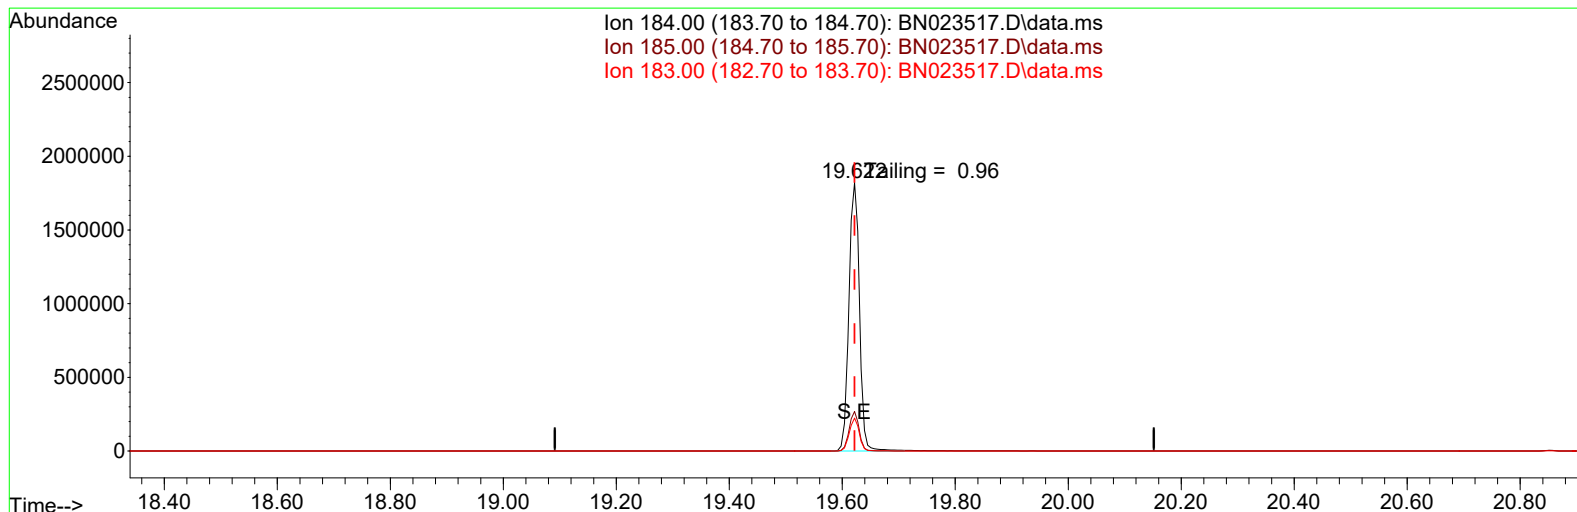

TIC: BN023517.D\data.ms

(77) Benzidine

19.622min (0.000) 0.00 ng

response 2379454

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.75
183.00	13.20	12.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/28/2022	BNA_N	<u>BN023517.D</u>
Compound Name	Response	Retention Time
DDT	1283487	20.851
DDD	25719	20.41
DDE	634	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26353	1309840	2.01

Instrument :
BNA_N
ClientSampleId :
DFTPP