
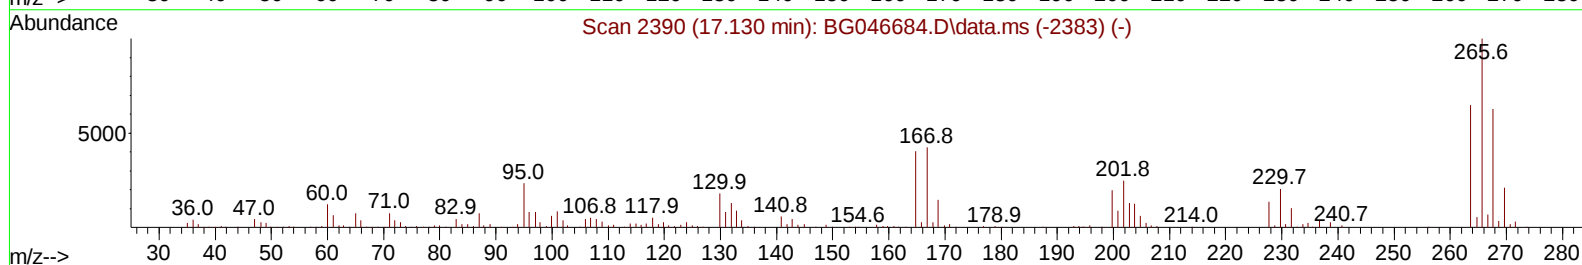
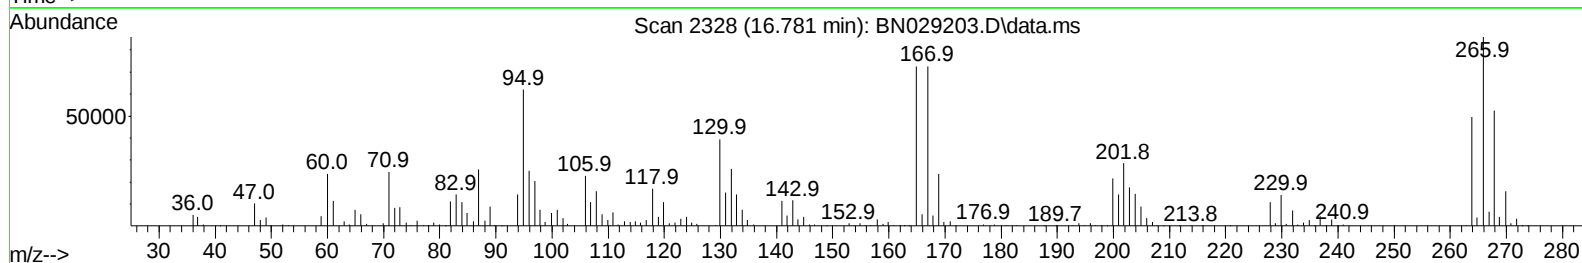


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122823\
Data File : BN029203.D
Acq On : 28 Dec 2023 08:26
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 03:57:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

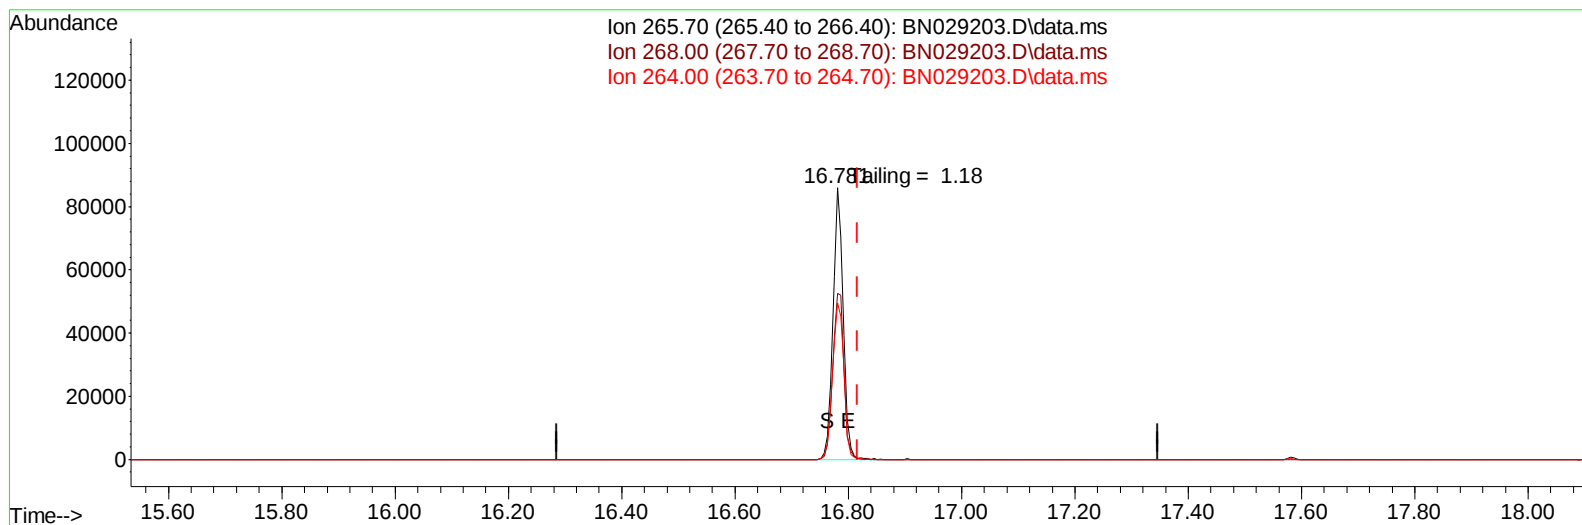




TIC: BN029203.D\data.ms

(70) Pentachlorophenol (C)**16.781min (-0.035) 10970.47 ng****response 107703**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.19
264.00	61.60	57.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122823\
Data File : BN029203.D
Acq On : 28 Dec 2023 08:26
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 29 03:57:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

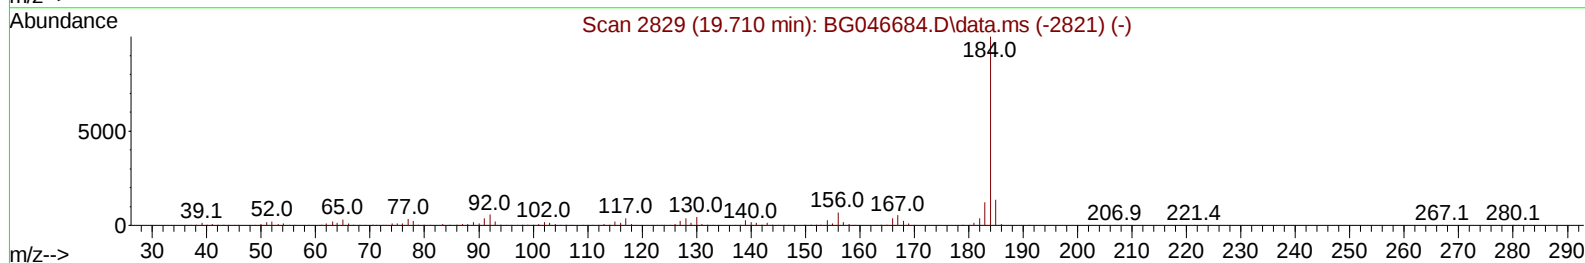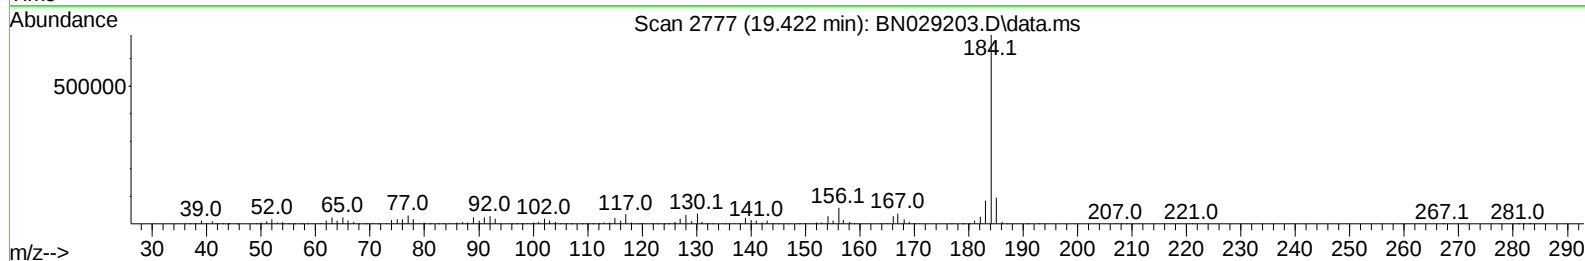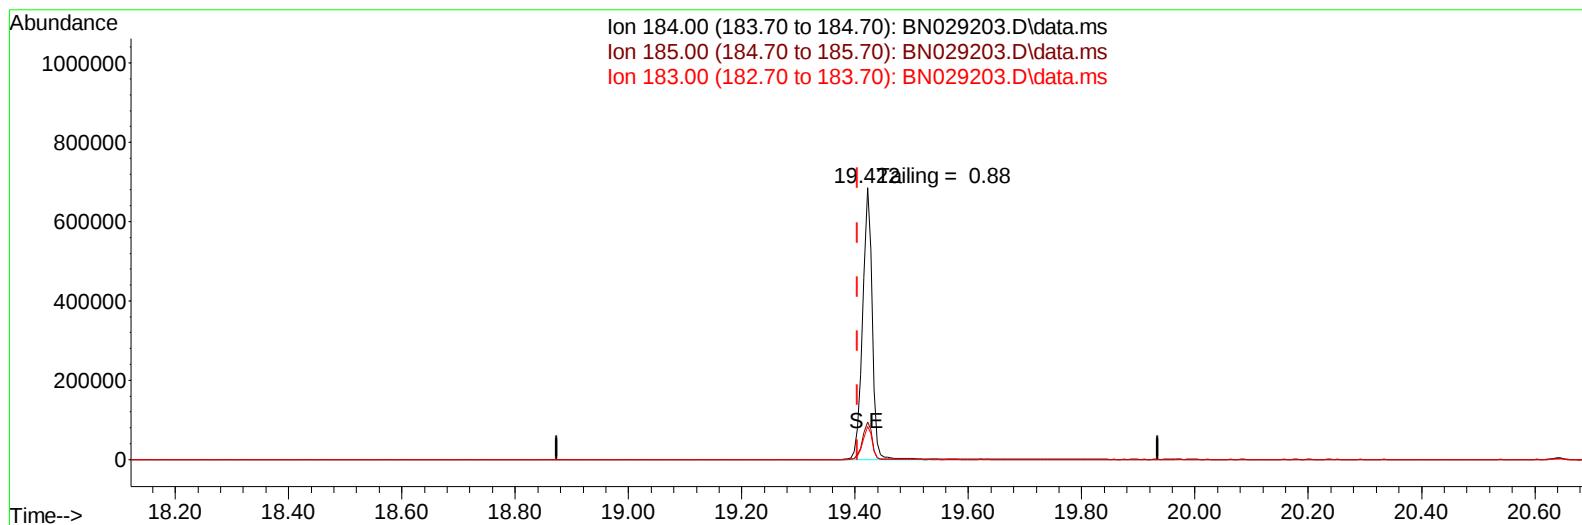

TIC: BN029203.D\data.ms

(77) Benzidine**19.422min (+ 0.018) 0.00 ng****response 797905**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	12.27
0.00	0.00	0.00