
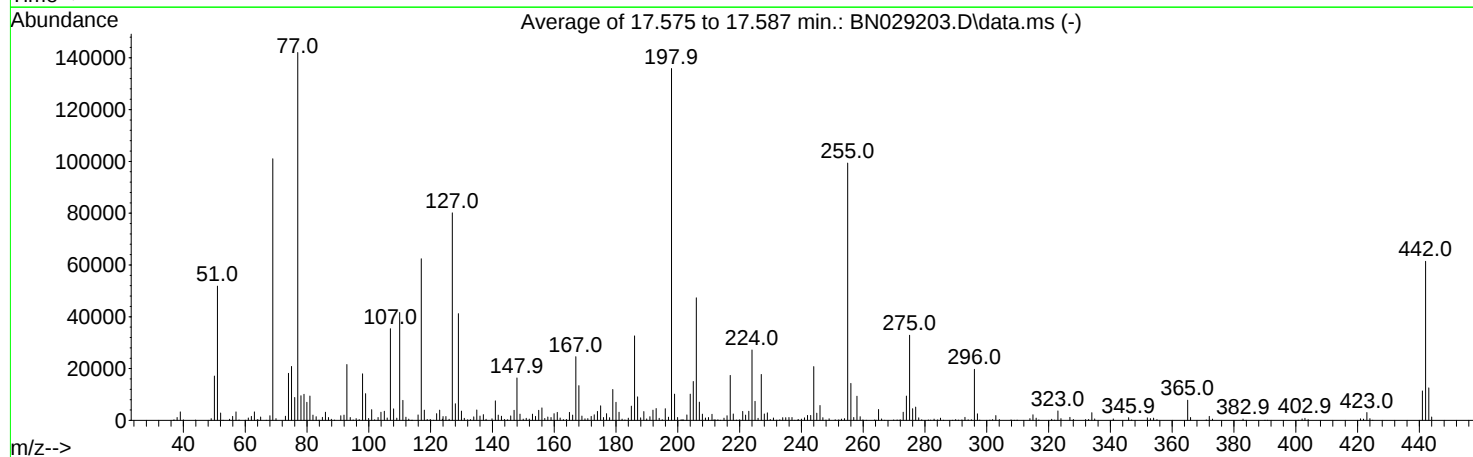


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122823\
Data File : BN029203.D
Acq On : 28 Dec 2023 08:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 28 01:20:47 2023

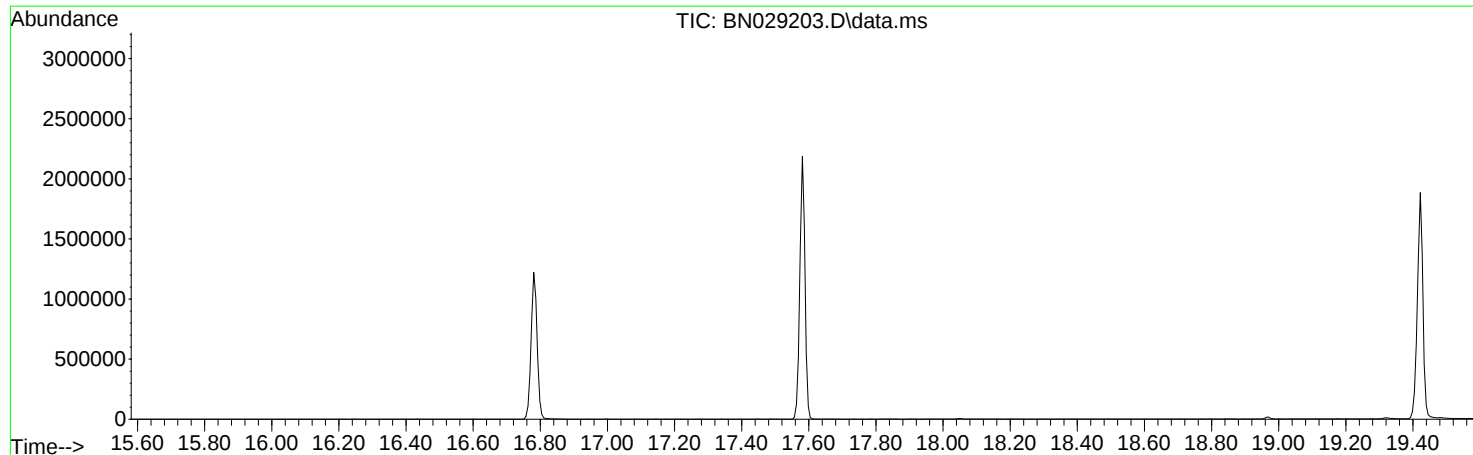




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	51816	PASS
68	69	0.00	2	1.8	1817	PASS
69	198	0.00	100	74.3	101008	PASS
70	69	0.00	2	0.7	687	PASS
127	198	10	80	59.0	80149	PASS
197	198	0.00	2	0.9	1226	PASS
198	198	100	100	100.0	135859	PASS
199	198	5	9	7.5	10146	PASS
275	198	10	60	24.2	32896	PASS
365	198	1	100	5.7	7789	PASS
441	198	0.01	100	8.4	11389	PASS
442	442	50	100	100.0	61445	PASS
443	442	15	24	20.4	12538	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122823\
Data File : BN029203.D
Acq On : 28 Dec 2023 08:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 29 03:57:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

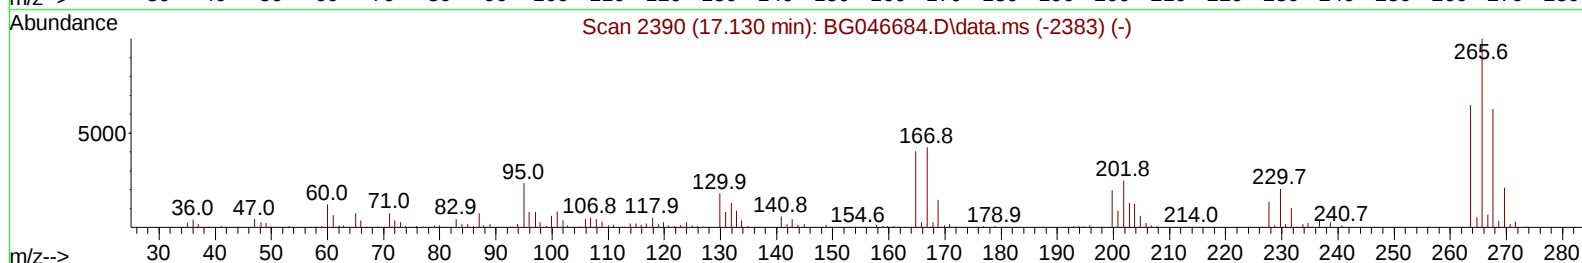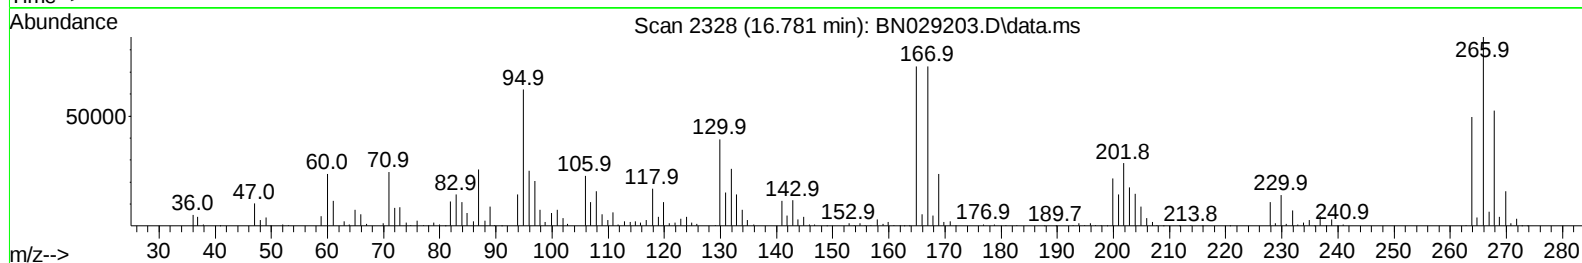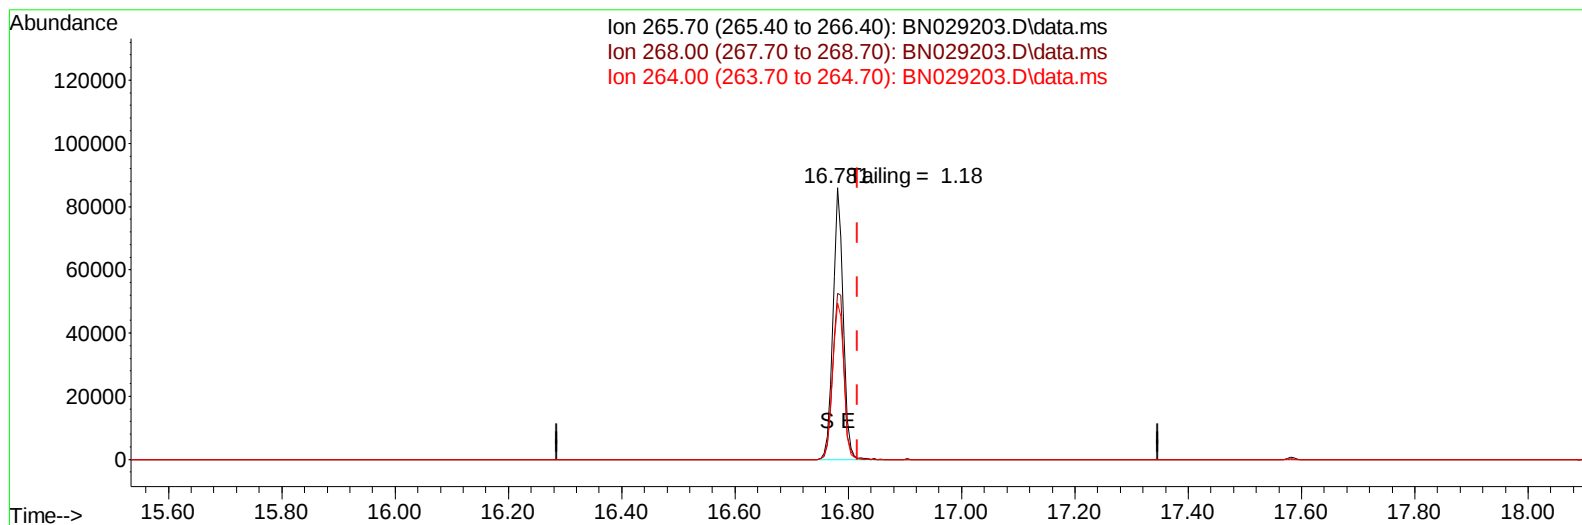

TIC: BN029203.D\data.ms

(70) Pentachlorophenol (C)

16.781min (-0.035) 10970.47 ng




response 107703

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.19
264.00	61.60	57.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122823\
Data File : BN029203.D
Acq On : 28 Dec 2023 08:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 29 03:57:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

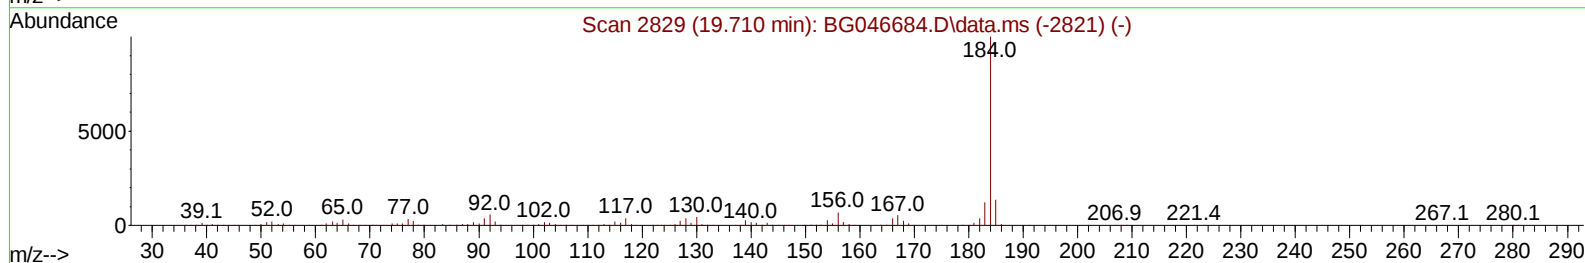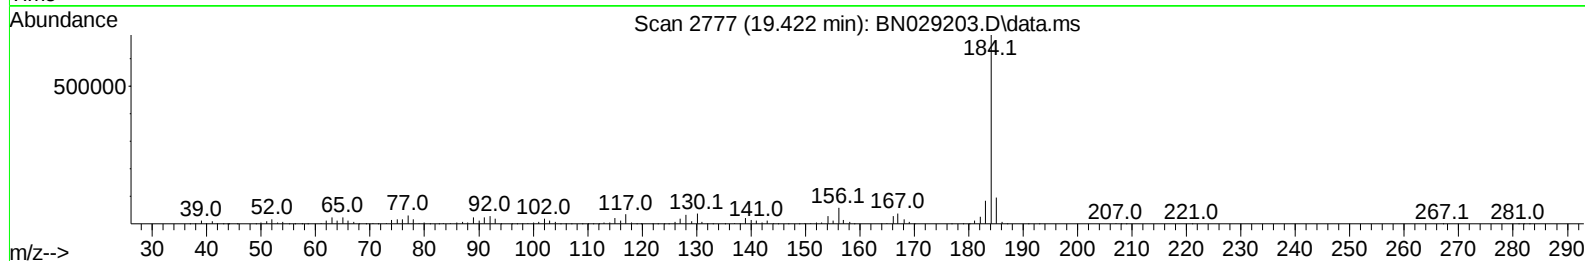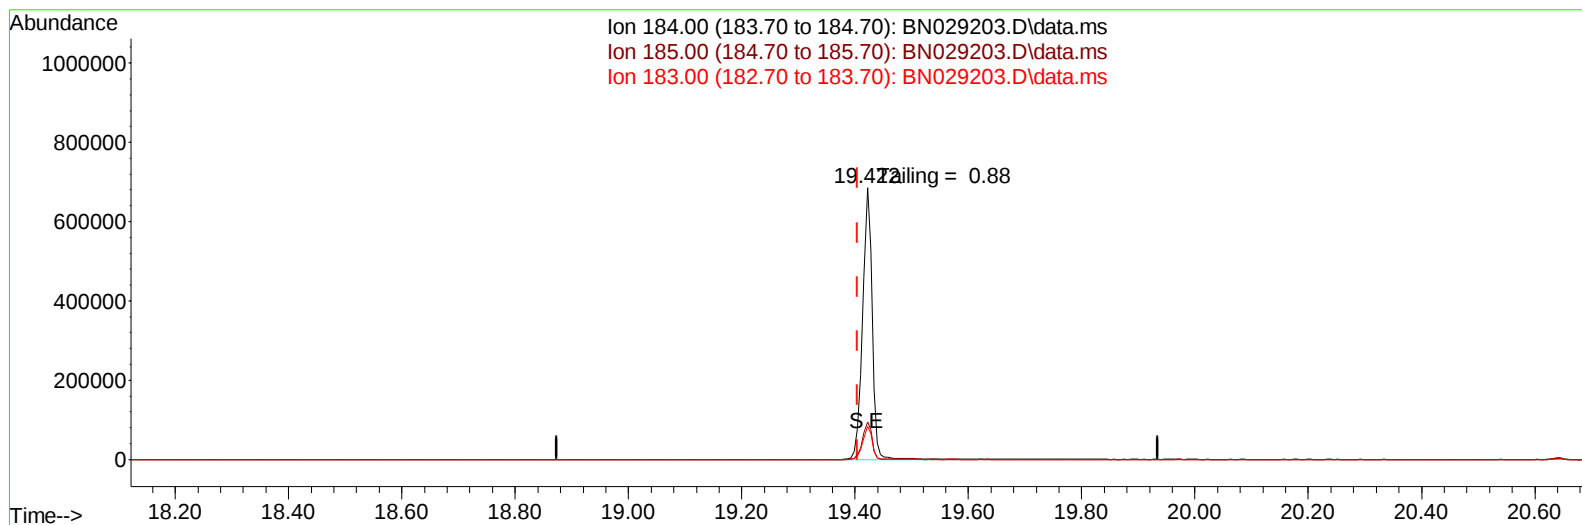

TIC: BN029203.D\data.ms

(77) Benzidine

19.422min (+ 0.018) 0.00 ng

response 797905

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	12.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/28/2023	BNA_N	<u>BN029203.D</u>
Compound Name	Response	Retention Time
DDT	384445	20.645
DDD	8049	20.198
DDE	354	19.681
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8403	392848	2.14

Instrument :
BNA_N
ClientSampleId :
DFTPP