

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN123022\
 Data File : BN023529.D
 Acq On : 30 Dec 2022 12:10
 Operator : CG/JU
 Sample : N5388-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-QT4-2022-07

Quant Time: Dec 30 21:57:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 30 21:52:41 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 01/03/2023
 Supervised By :Yogesh Patel 01/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.977	152	4507	0.400	ng/ul	0.00
4) Naphthalene-d8	10.793	136	13066	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.622	164	6695	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.373	188	13384	0.400	ng/ul	0.00
17) Chrysene-d12	21.557	240	6968	0.400	ng/ul	0.00
23) Perylene-d12	23.995	264	5038	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.332	96	3146	0.642	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.377	152	7352	0.364	ng/ul	0.00
18) Fluoranthene-d10	19.402	212	13349	0.530	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.370	88	524m	0.105	ng/ul	
5) Naphthalene	10.843	128	2643	0.069	ng/ul#	93
7) 2-Methylnaphthalene	12.454	142	1602	0.065	ng/ul	100
8) 1-Methylnaphthalene	12.674	142	1601	0.063	ng/ul	100
10) Acenaphthylene	14.345	152	1985	0.067	ng/ul#	93
11) Acenaphthene	14.687	153	1807	0.072	ng/ul	99
12) Fluorene	15.672	166	1887	0.067	ng/ul#	97
14) Pentachlorophenol	17.023	266	197	0.053	ng/ul	97
15) Phenanthrene	17.411	178	2981	0.068	ng/ul	93
16) Anthracene	17.504	178	2209	0.061	ng/ul#	89
19) Fluoranthene	19.430	202	3061	0.091	ng/ul#	94
20) Pyrene	19.792	202	3035	0.089	ng/ul#	92
21) Benzo(a)anthracene	21.543	228	1765	0.065	ng/ul	95
22) Chrysene	21.595	228	2017	0.073	ng/ul	96
24) Benzo(b)fluoranthene	23.250	252	1778	0.068	ng/ul#	38
25) Benzo(k)fluoranthene	23.302	252	1534	0.063	ng/ul#	37
26) Benzo(a)pyrene	23.887	252	1415	0.069	ng/ul#	4
27) Indeno(1,2,3-cd)pyrene	26.543	276	1601	0.066	ng/ul#	94
28) Dibenzo(a,h)anthracene	26.560	278	1108	0.059	ng/ul#	41
29) Benzo(g,h,i)perylene	27.322	276	1577	0.080	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN123022\
Data File : BN023529.D
Acq On : 30 Dec 2022 12:10
Operator : CG/JU
Sample : N5388-01
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07

Quant Time: Dec 30 21:57:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 30 21:52:41 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

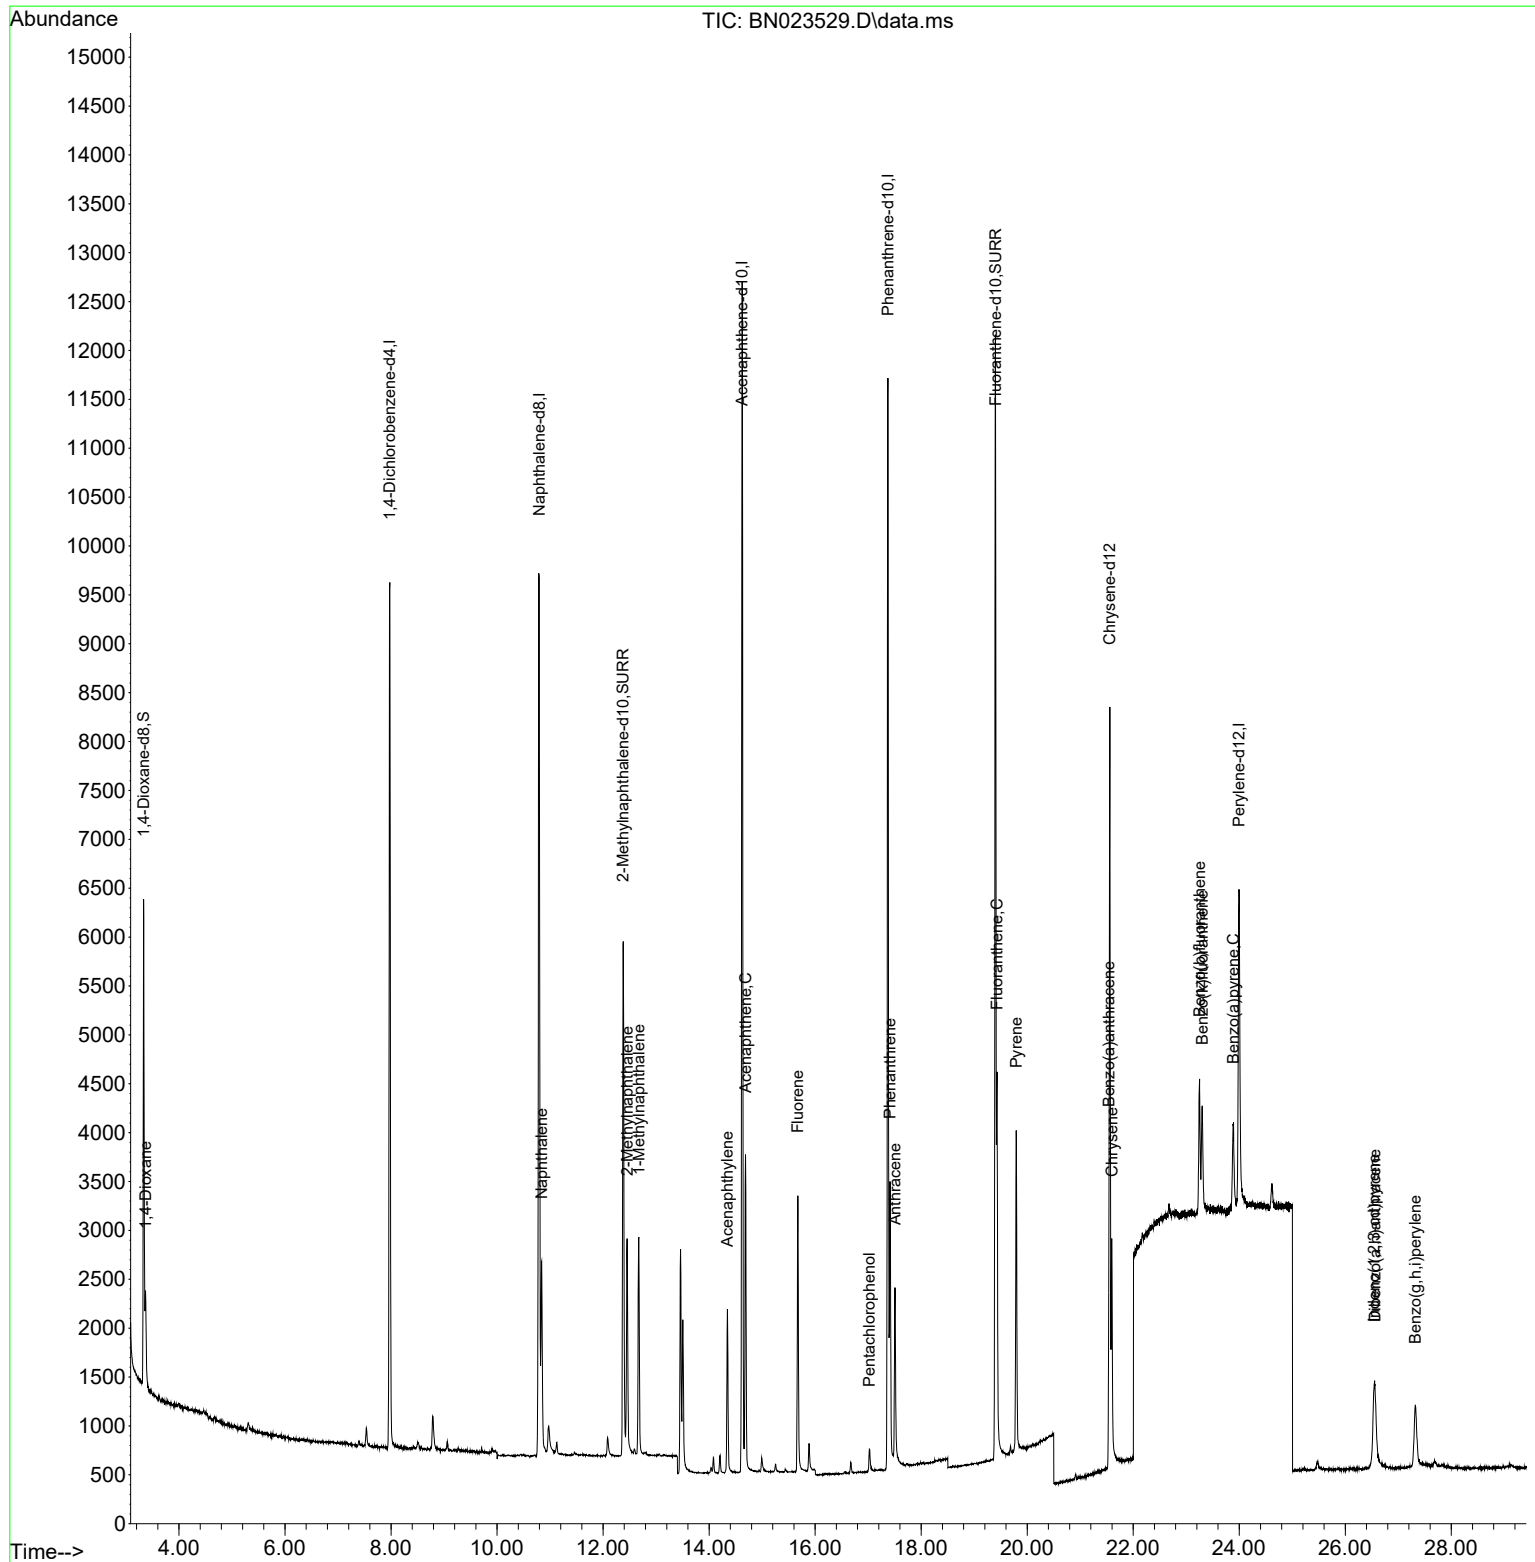



#2
1,4-Dioxane
Concen: 0.105 ng/ul m
RT: 3.370 min Scan# 61
Delta R.T. -0.004 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07



Tgt Ion: 88 Resp: 524
Ion Ratio Lower Upper
88 100
43 38.6 28.4 42.6
58 41.3 45.6 68.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

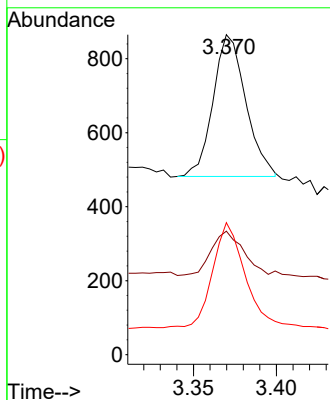

#5
Naphthalene
Concen: 0.069 ng/ul
RT: 10.843 min Scan# 1796
Delta R.T. 0.006 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10


Tgt Ion:128 Resp: 2643
Ion Ratio Lower Upper
128 100
129 14.5 9.0 13.4#
127 15.5 10.7 16.1

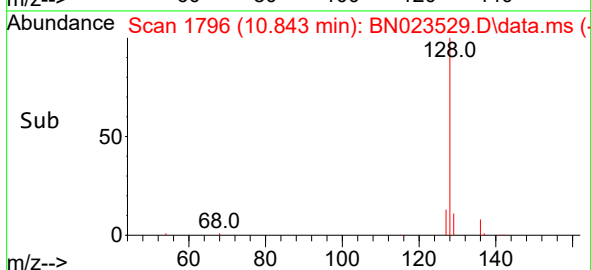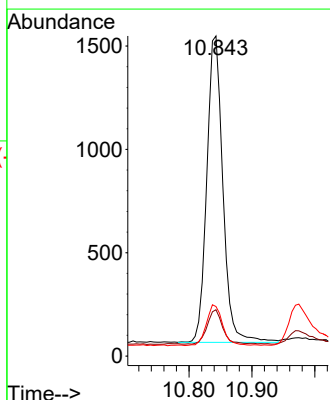



#7
2-Methylnaphthalene
Concen: 0.065 ng/ul
RT: 12.454 min Scan# 2088
Delta R.T. 0.006 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07




Tgt Ion:142 Resp: 1601
Ion Ratio Lower Upper
142 100
141 89.1 71.4 107.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

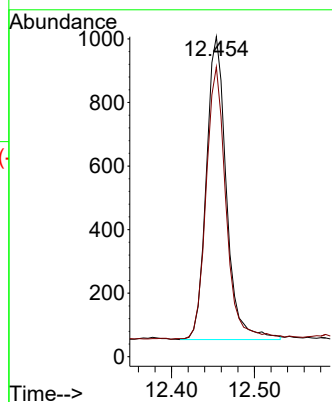


#8
1-Methylnaphthalene
Concen: 0.063 ng/ul
RT: 12.674 min Scan# 2129
Delta R.T. 0.006 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Tgt Ion:142 Resp: 1601
Ion Ratio Lower Upper
142 100
141 92.7 74.0 111.0

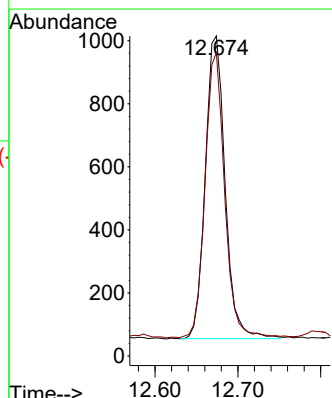



#10
Acenaphthylene
Concen: 0.067 ng/ul
RT: 14.345 min Scan# 2465
Delta R.T. 0.000 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07




Tgt Ion:152 Resp: 1985
Ion Ratio Lower Upper
152 100
151 23.3 16.1 24.1
153 16.3 10.9 16.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

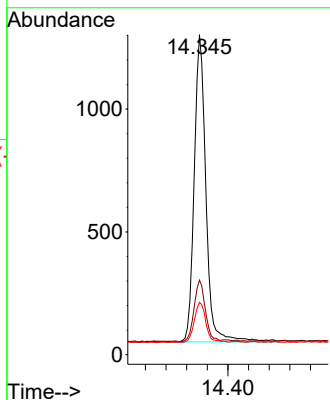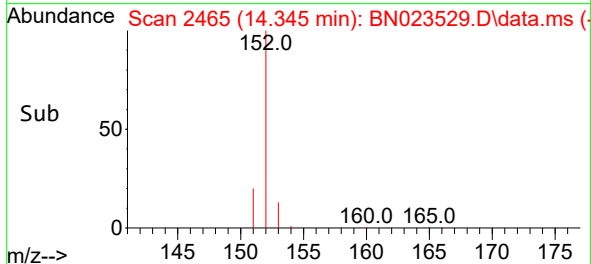


#11
Acenaphthene
Concen: 0.072 ng/ul
RT: 14.687 min Scan# 2539
Delta R.T. 0.000 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10

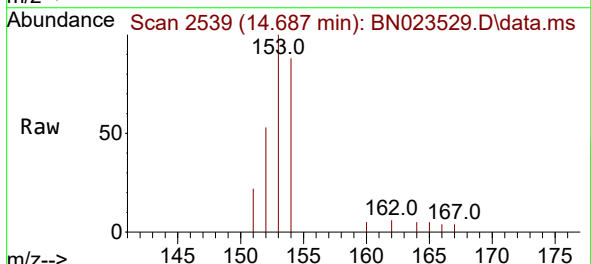


Tgt Ion:153 Resp: 1807
Ion Ratio Lower Upper
153 100
152 52.9 41.0 61.4
154 87.8 69.5 104.3

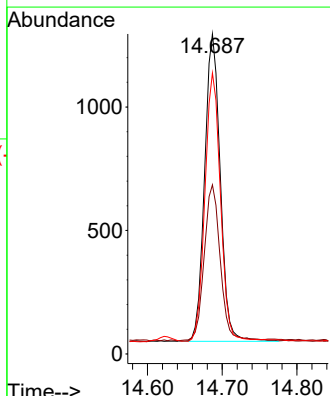



#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.672 min Scan# 2752
Delta R.T. 0.000 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07



Tgt Ion:166 Resp: 188
Ion Ratio Lower Upper
166 100
165 101.1 79.1 118.7
167 17.0 11.0 16.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

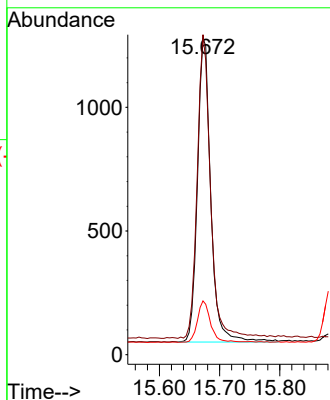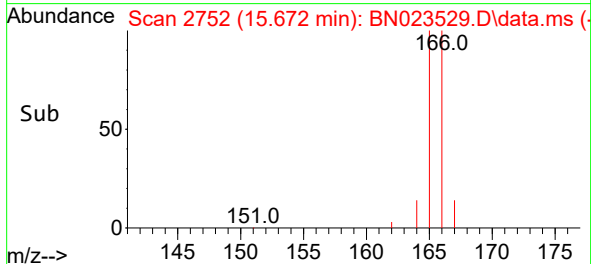

#14
Pentachlorophenol
Concen: 0.053 ng/ul
RT: 17.023 min Scan# 3065
Delta R.T. 0.000 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10


Tgt Ion:266 Resp: 197
Ion Ratio Lower Upper
266 100
264 63.5 49.8 74.6
268 60.4 51.4 77.0

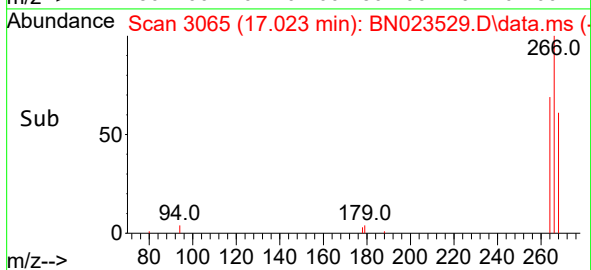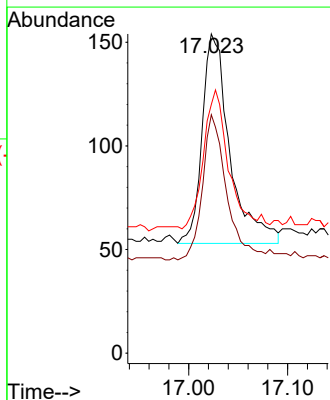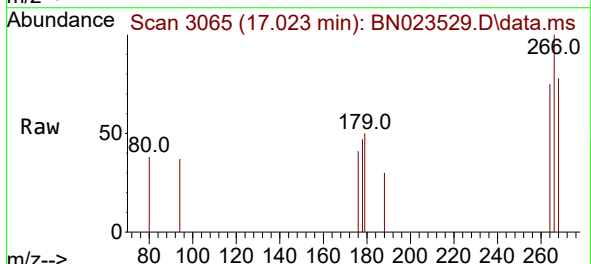

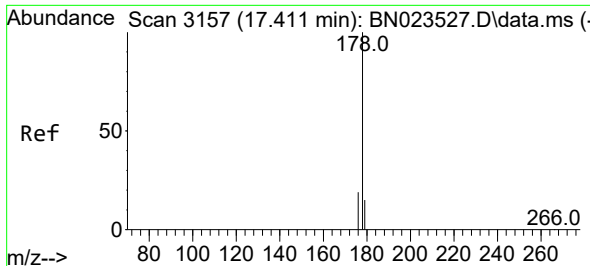

#15
Phenanthrene
Concen: 0.068 ng/ul
RT: 17.411 min Scan# 3157
Delta R.T. 0.000 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07

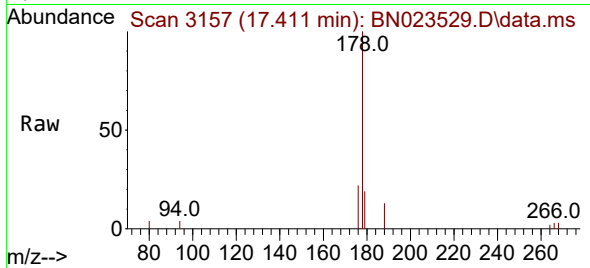


Tgt Ion:178 Resp: 298
Ion Ratio Lower Upper
178 100
179 18.7 12.5 18.7
176 22.3 15.7 23.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

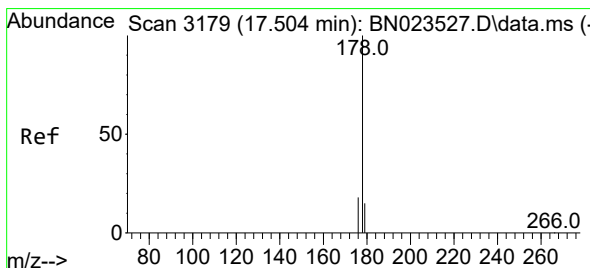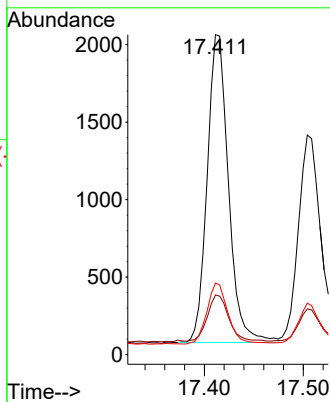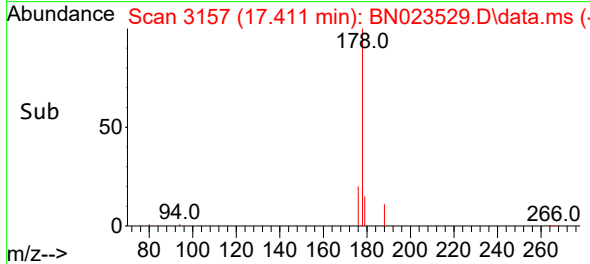


#16
Anthracene
Concen: 0.061 ng/ul
RT: 17.504 min Scan# 3179
Delta R.T. 0.000 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10

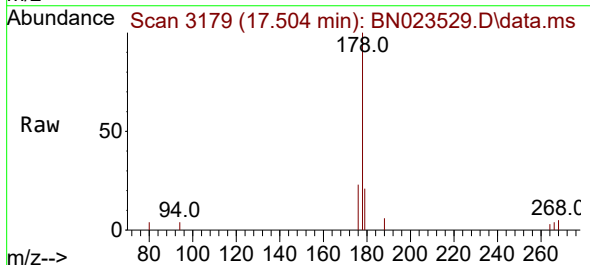


Tgt Ion:178 Resp: 2209
Ion Ratio Lower Upper
178 100
179 20.8 12.6 18.8#
176 23.4 15.4 23.0#

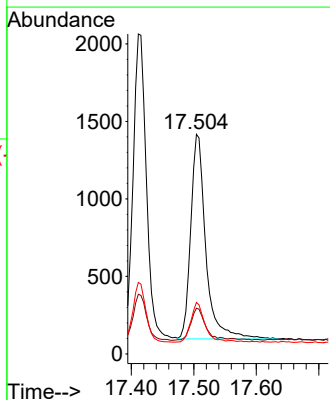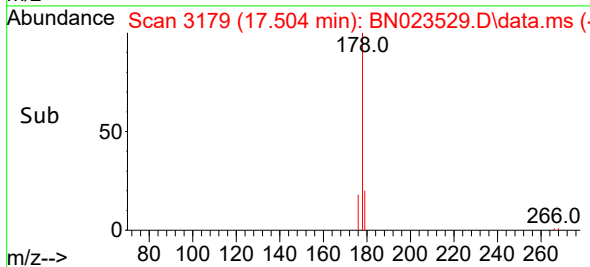

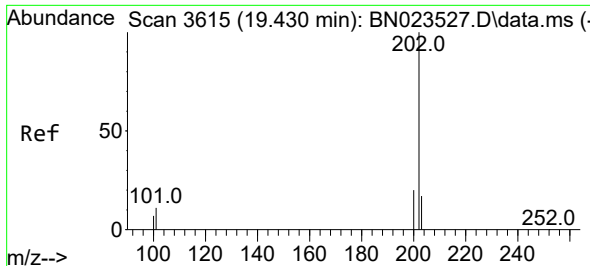

#19
Fluoranthene
Concen: 0.091 ng/ul
RT: 19.430 min Scan# 3615
Delta R.T. 0.000 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07

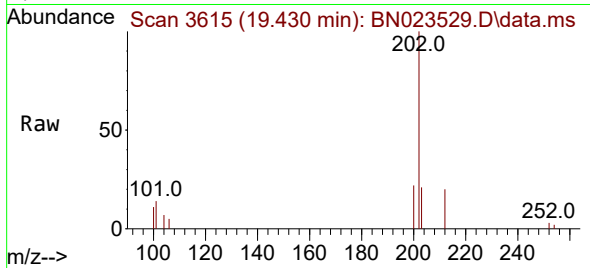


Tgt Ion:202 Resp: 3061
Ion Ratio Lower Upper
202 100
101 14.3 9.4 14.2
100 10.9 7.0 10.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

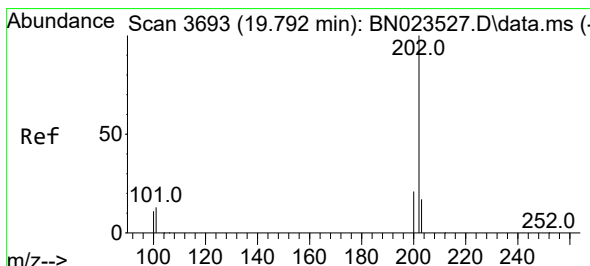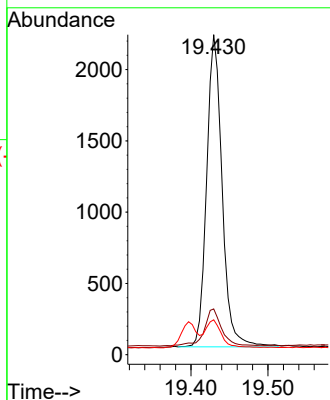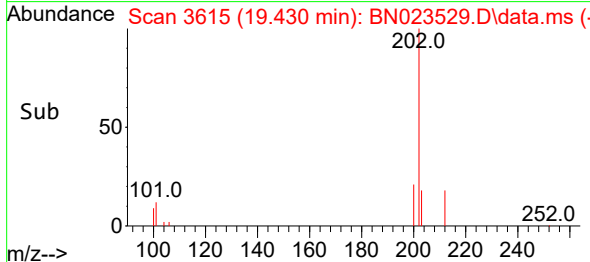


#20
Pyrene
Concen: 0.089 ng/ul
RT: 19.792 min Scan# 3693
Delta R.T. 0.000 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10

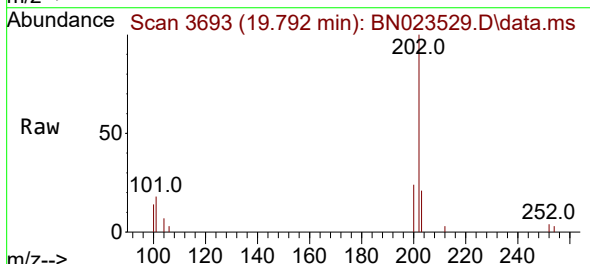


Tgt Ion:202 Resp: 3035
Ion Ratio Lower Upper
202 100
101 17.6 11.3 16.9#
100 14.1 9.0 13.4#

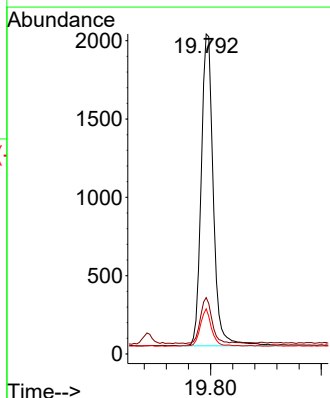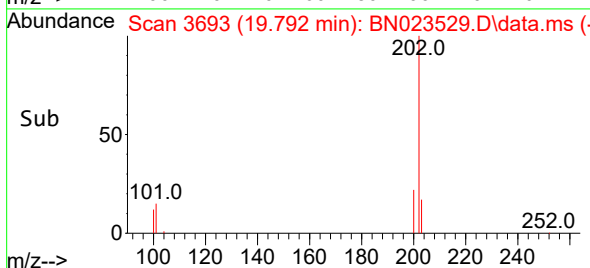



#21
Benzo(a)anthracene
Concen: 0.065 ng/ul
RT: 21.543 min Scan# 41
Delta R.T. 0.003 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07




Tgt Ion:228 Resp: 176
Ion Ratio Lower Upper
228 100
229 22.5 15.6 23.4
226 30.1 22.2 33.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

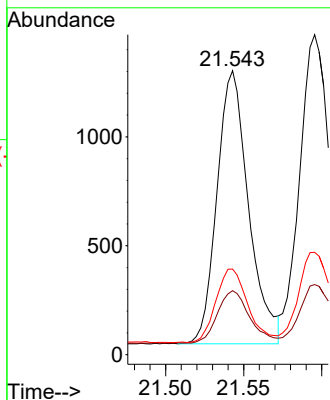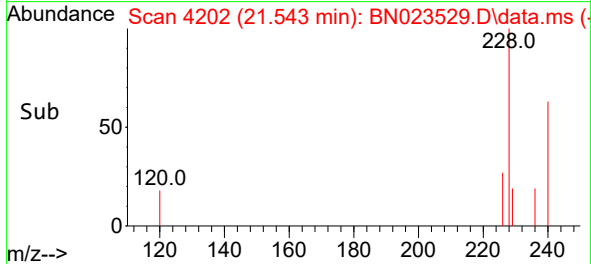


#22
Chrysene
Concen: 0.073 ng/ul
RT: 21.595 min Scan# 4220
Delta R.T. 0.003 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10

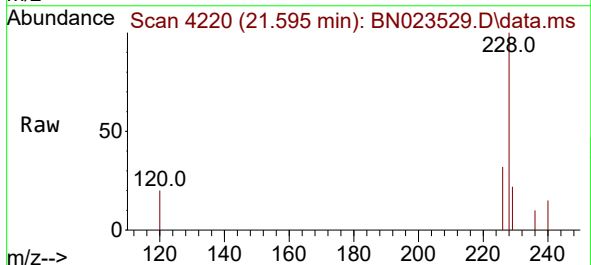


Tgt Ion:228 Resp: 2017
Ion Ratio Lower Upper
228 100
226 32.0 24.3 36.5
229 21.9 15.8 23.6

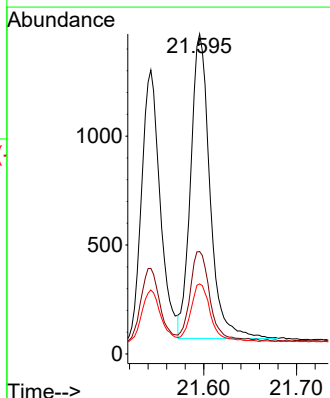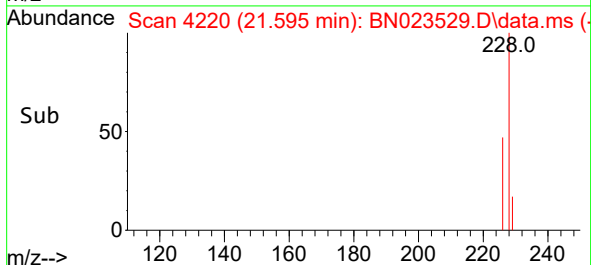



#24
Benzo(b)fluoranthene
Concen: 0.068 ng/ul
RT: 23.250 min Scan# 4784
Delta R.T. 0.006 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07




Tgt Ion:252 Resp: 1778
Ion Ratio Lower Upper
252 100
253 48.3 0.0 49.2
125 51.2 0.0 31.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

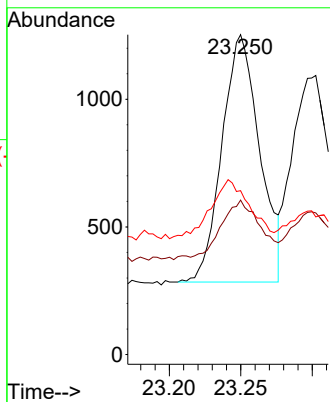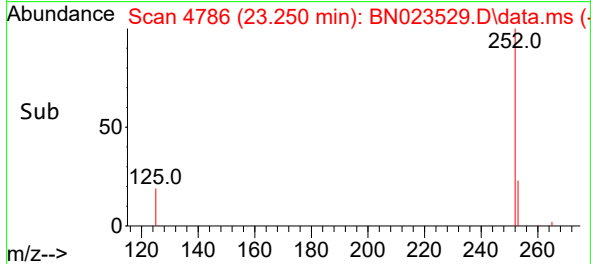


#25
Benzo(k)fluoranthene
Concen: 0.063 ng/ul
RT: 23.302 min Scan# 4804
Delta R.T. 0.009 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10

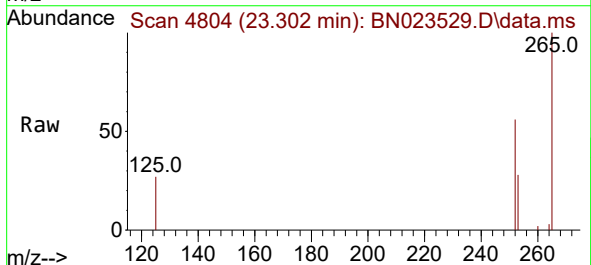

Tgt Ion:252 Resp: 1534
Ion Ratio Lower Upper
252 100
253 50.8 19.8 29.6#
125 49.3 12.6 18.8#

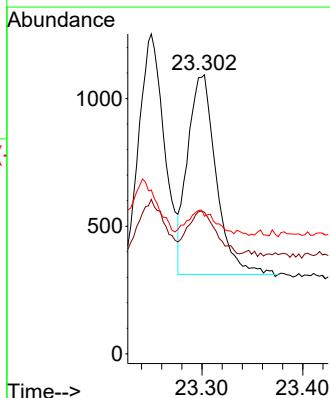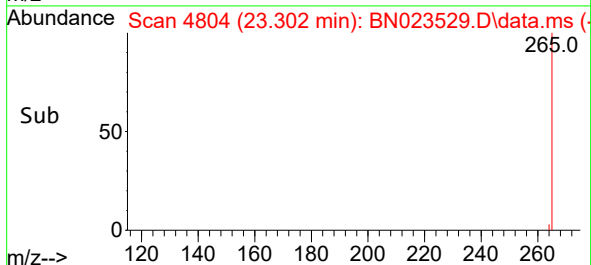



#26

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.887 min Scan# 5004

Delta R.T. 0.006 min

Lab File: BN023529.D

Acq: 30 Dec 2022 12:10

Instrument :

BN023529.D

ClientSampleId :





MDL-WATER-QT4-2022-07

Tgt Ion:	252	Resp:	141
Ion Ratio	Lower	Upper	
252	100		
253	63.4	21.4	32.2
125	79.6	16.2	24.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

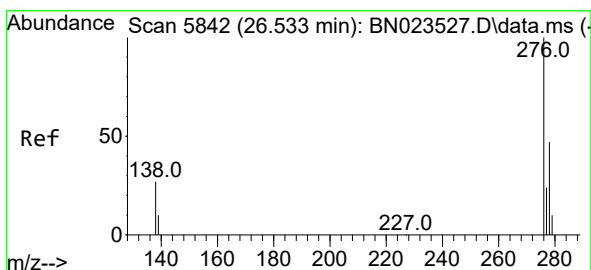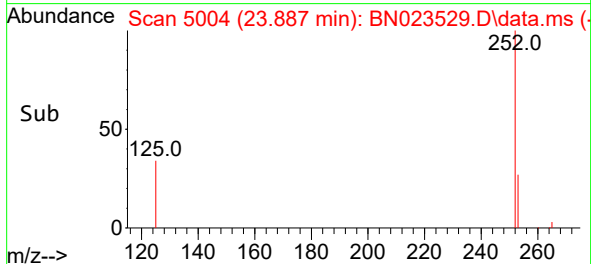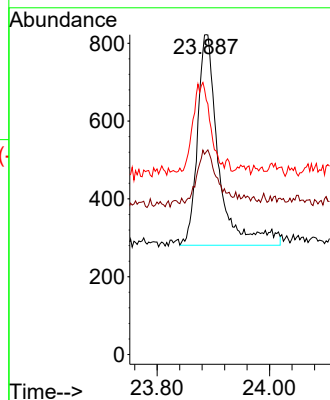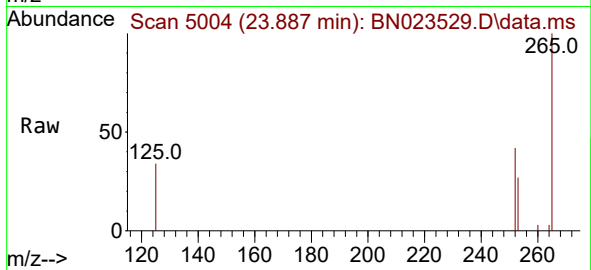

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.066 ng/ul




RT: 26.543 min Scan# 5845


Delta R.T. 0.010 min

Lab File: BN023529.D

Acq: 30 Dec 2022 12:10


Tgt Ion:	276	Resp:	1601
Ion Ratio	Lower	Upper	
276	100		
138	32.5	23.4	35.2
227	0.4	0.0	0.0

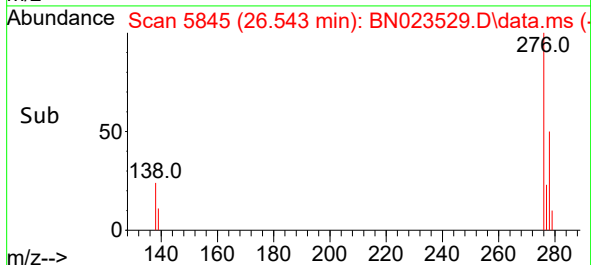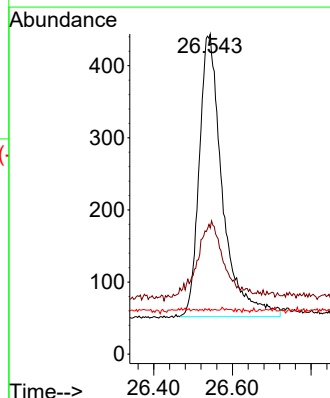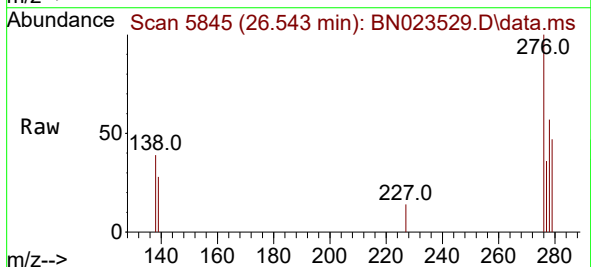

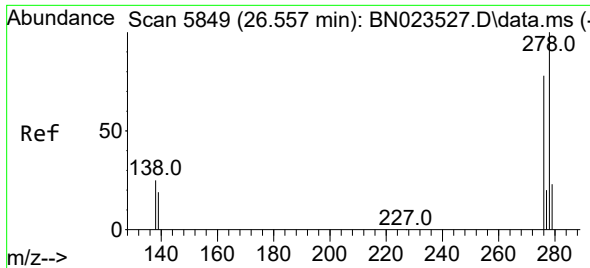

#28
Dibenzo(a,h)anthracene
Concen: 0.059 ng/ul
RT: 26.560 min Scan# 5849
Delta R.T. 0.003 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-QT4-2022-07

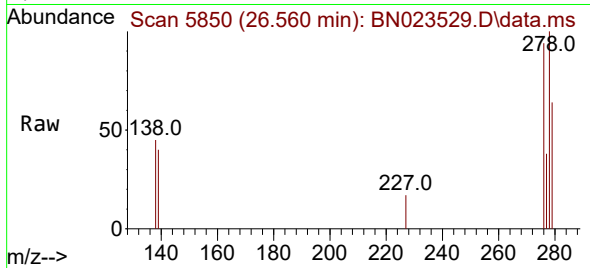

Tgt Ion:278 Resp: 1108
Ion Ratio Lower Upper
278 100
139 39.6 16.6 24.8#
279 64.1 21.3 31.9#

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/03/2023
Supervised By :Yogesh Patel 01/03/2023

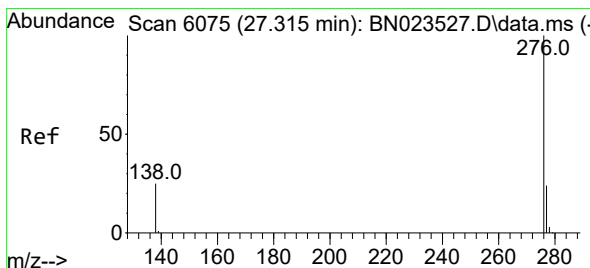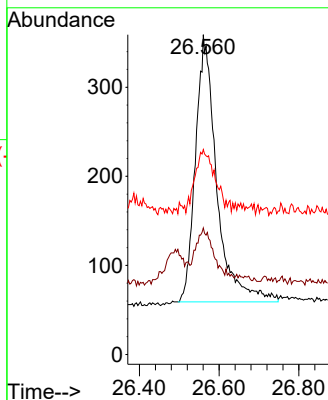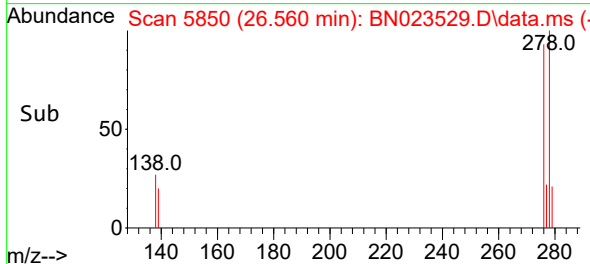

#29
Benzo(g,h,i)perylene
Concen: 0.080 ng/ul
RT: 27.322 min Scan# 6077
Delta R.T. 0.007 min
Lab File: BN023529.D
Acq: 30 Dec 2022 12:10

Tgt Ion:276 Resp: 1577
Ion Ratio Lower Upper
276 100
138 39.7 20.3 30.5#
277 35.6 19.7 29.5#

