

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN123119\
 Data File : BN009282.D
 Acq On : 31 Dec 2019 15:36
 Operator : JU
 Sample : K6308-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 31 16:58:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 11:02:23 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	2505	0.40	ng/ul	0.00
2) Naphthalene-d8	10.26	136	9034	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.13	164	4705	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.88
16) Chrysene-d12	21.09	240	6925	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	7349	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.86	152	3250	0.20	ng/ul	0.00
14) Fluoranthene-d10	18.92	212	6878	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.28	202	967	0.027	ng/ul#	1
23) Benzo(a)pyrene	23.08	252	1731	0.058	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN123119\
Data File : BN009282.D
Acq On : 31 Dec 2019 15:36
Operator : JU
Sample : K6308-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 31 16:58:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 11:02:23 2019
Response via : Initial Calibration

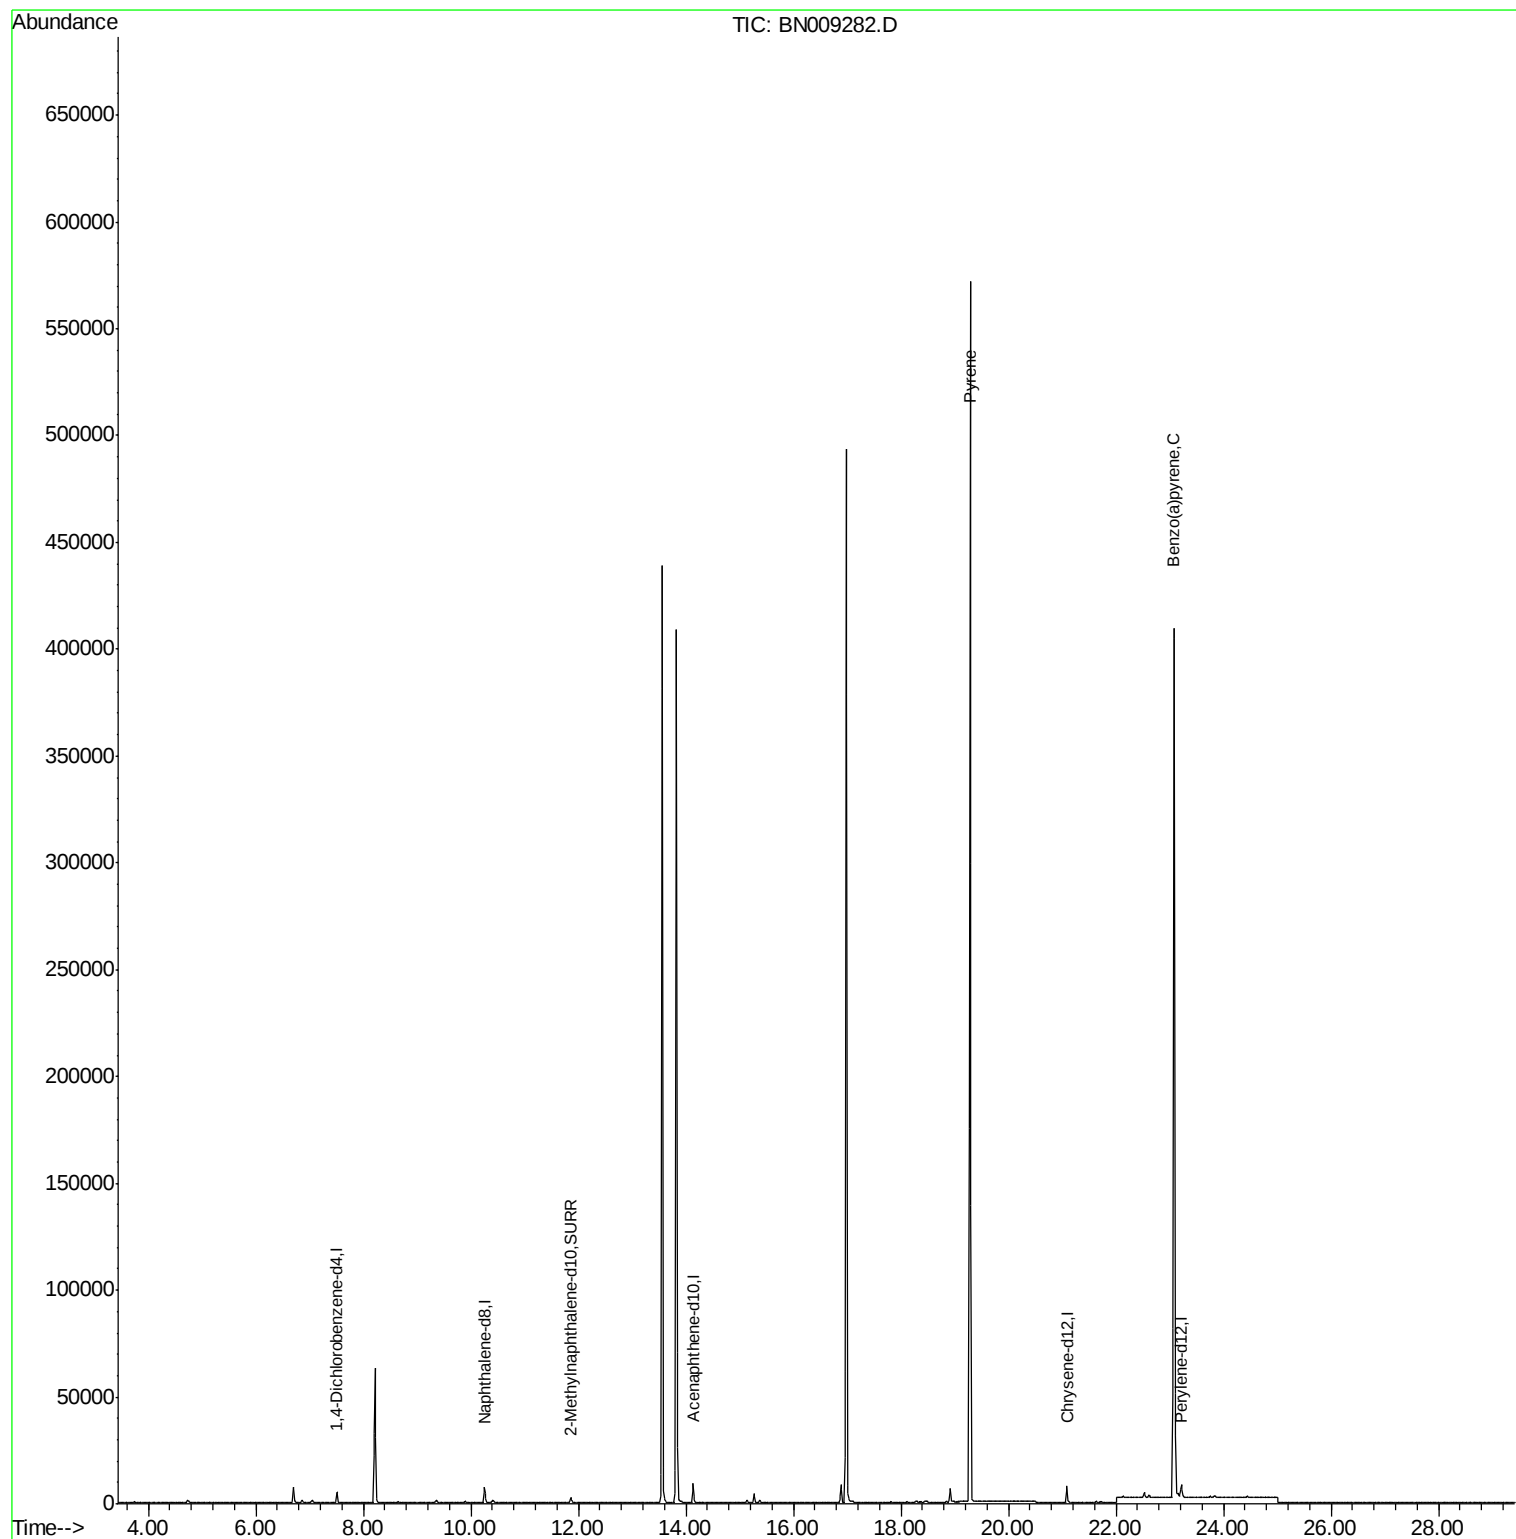

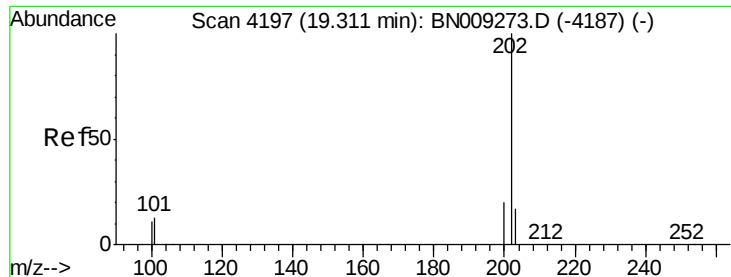

#17

Pvrene

Concen: 0.027 ng/ul

RT: 19.28 min Scan# 4191

Delta R.T. -0.03 min

Lab File: BN009282.D

Acq: 31 Dec 2019 15:36

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 967

Ion Ratio Lower Upper

202 100

101 170.3 10.9 16.3#




100 1105.9 9.0 13.6#

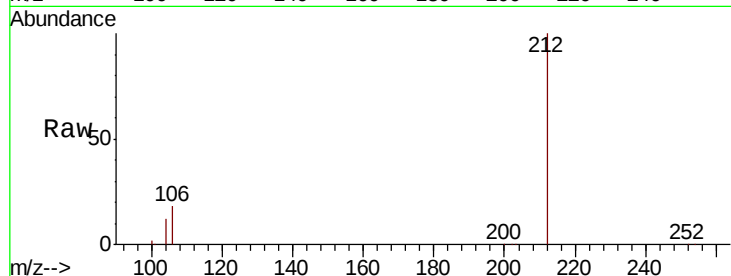

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

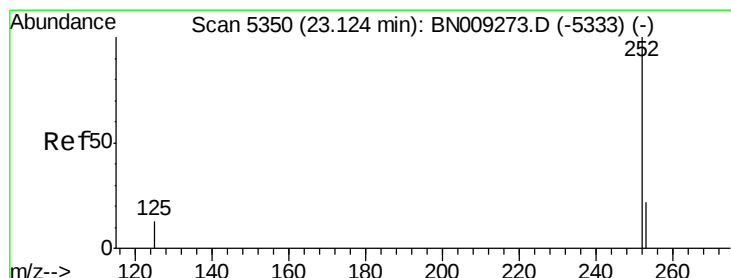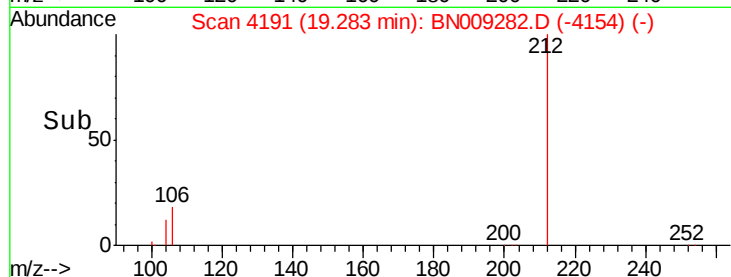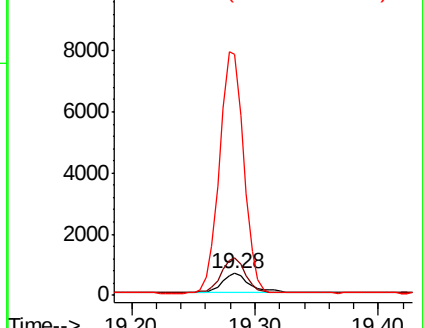

#23

Benzo(a)pyrene

Concen: 0.058 ng/ul

RT: 23.08 min Scan# 5335

Delta R.T. -0.04 min

Lab File: BN009282.D

Acq: 31 Dec 2019 15:36


Tgt Ion:252 Resp: 1731

Ion Ratio Lower Upper

252 100

253 51.2 20.2 30.4#

125 53.9 13.2 19.8#

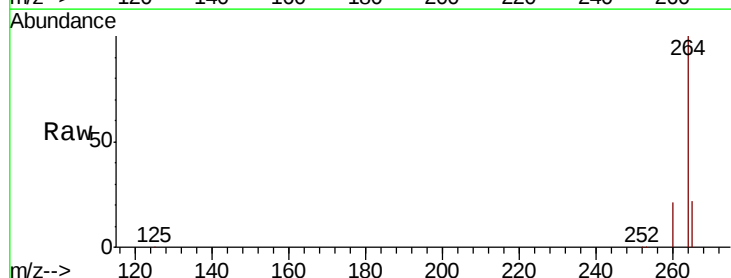

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

