


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN123119\
Data File : BN009275.D
Acq On : 31 Dec 2019 11:24
Operator : JU
Sample : PB125795BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK95

Manual Integrations
APPROVED

mohammad
1/1/2020 8:16:52 AM

Quant Time: Dec 31 12:31:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 11:02:23 2019
Response via : Initial Calibration

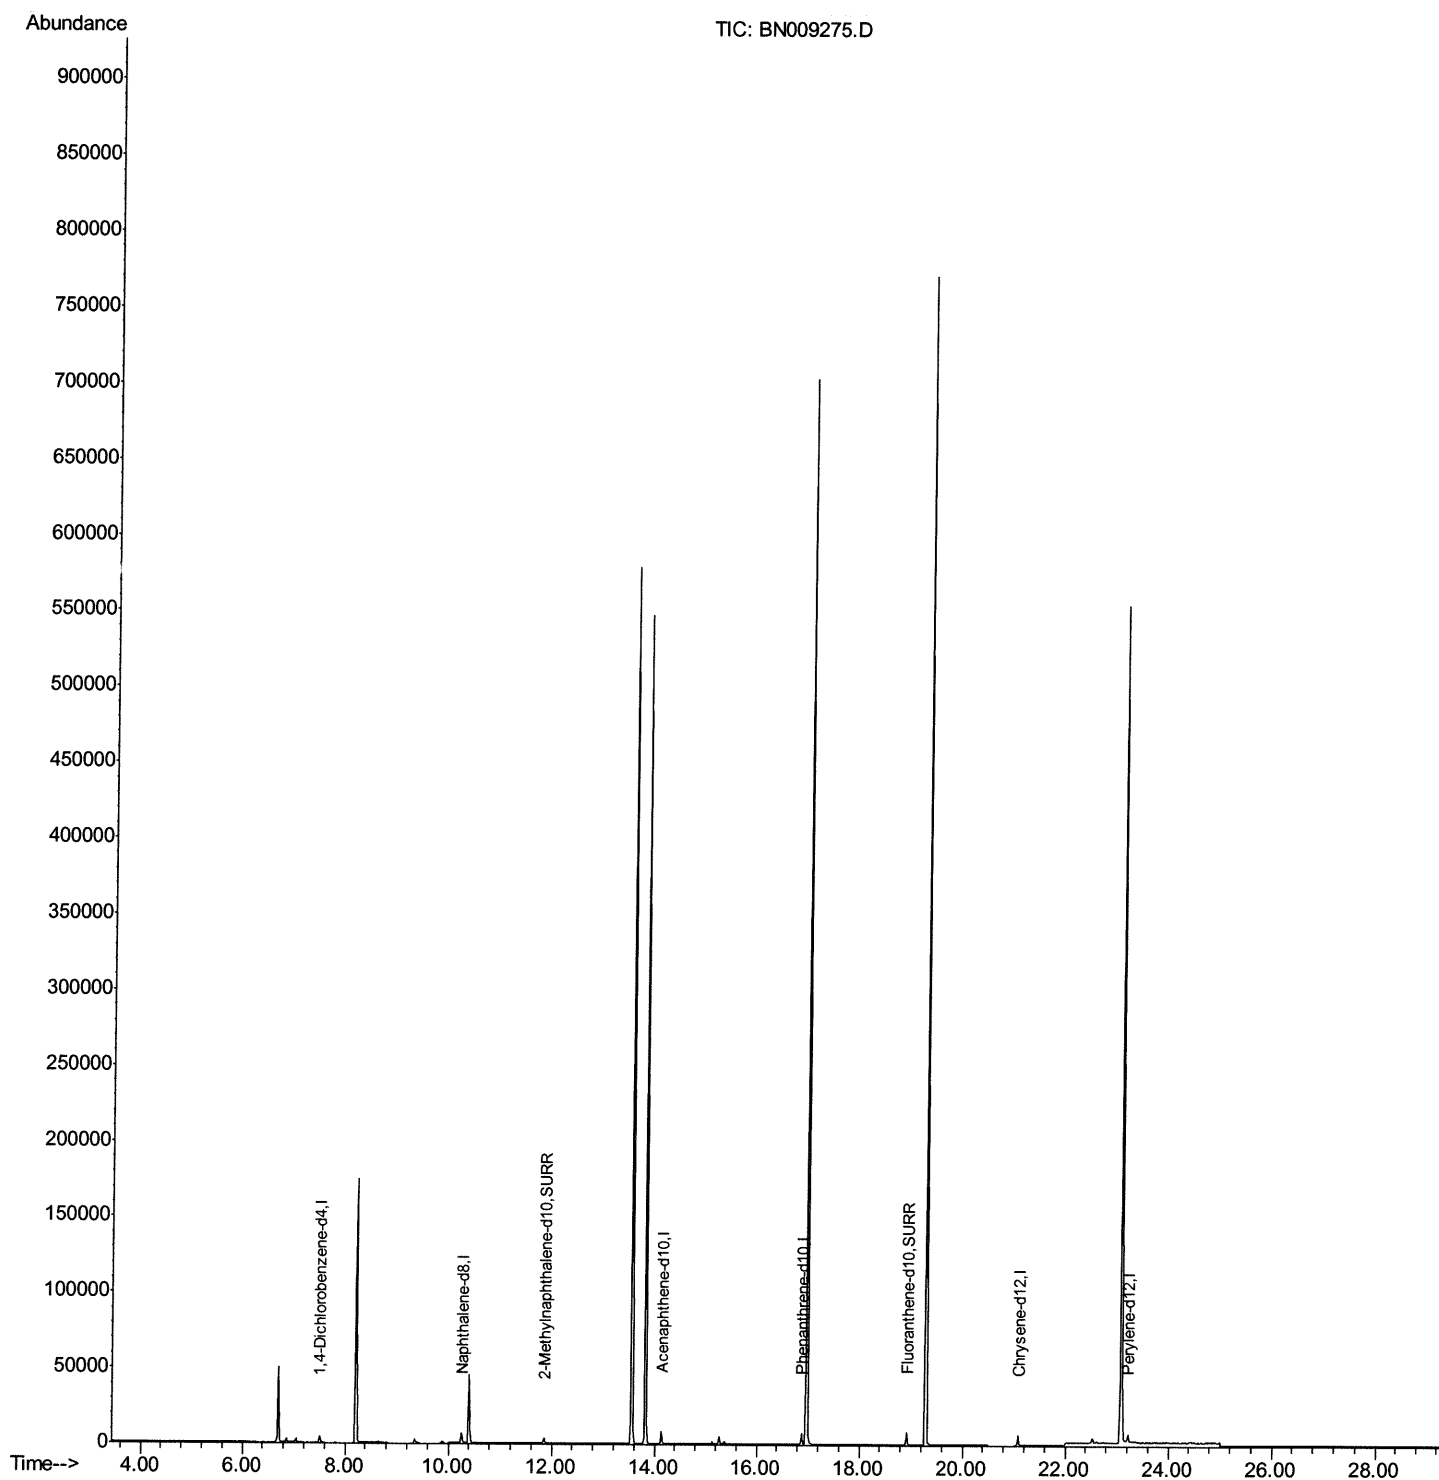

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN123119\
 Data File : BN009275.D
 Acq On : 31 Dec 2019 11:24
 Operator : JU
 Sample : PB125795BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK95

Manual Integrations
 APPROVED

mohammad
 1/1/2020 8:16:52 AM

Quant Time: Dec 31 12:30:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 11:02:23 2019
 Response via : Initial Calibration

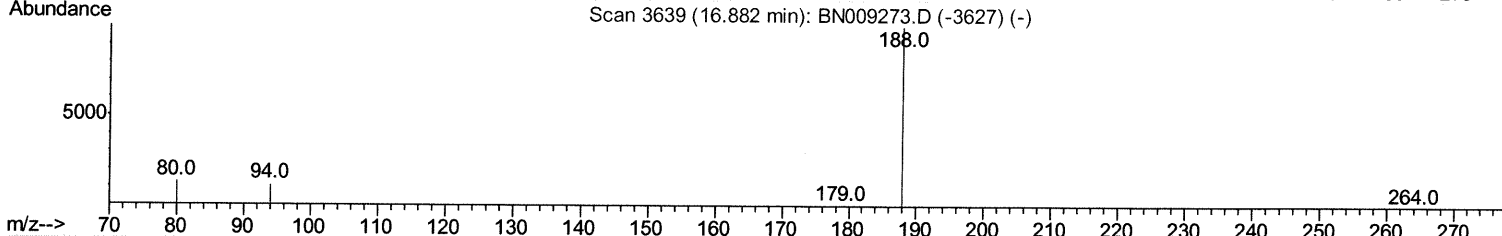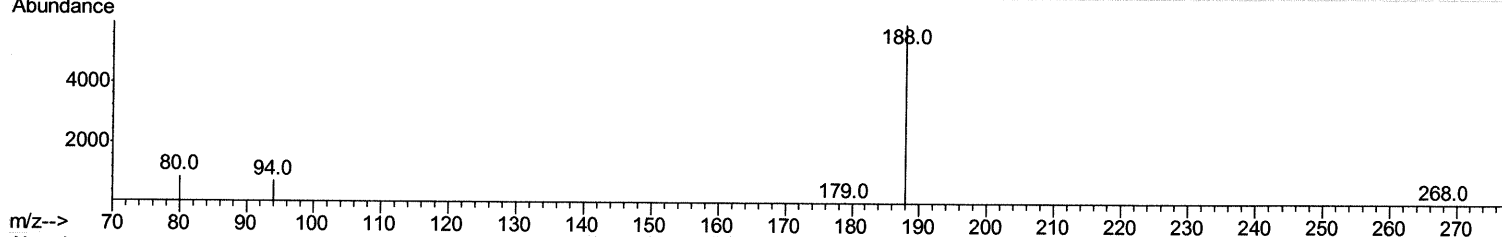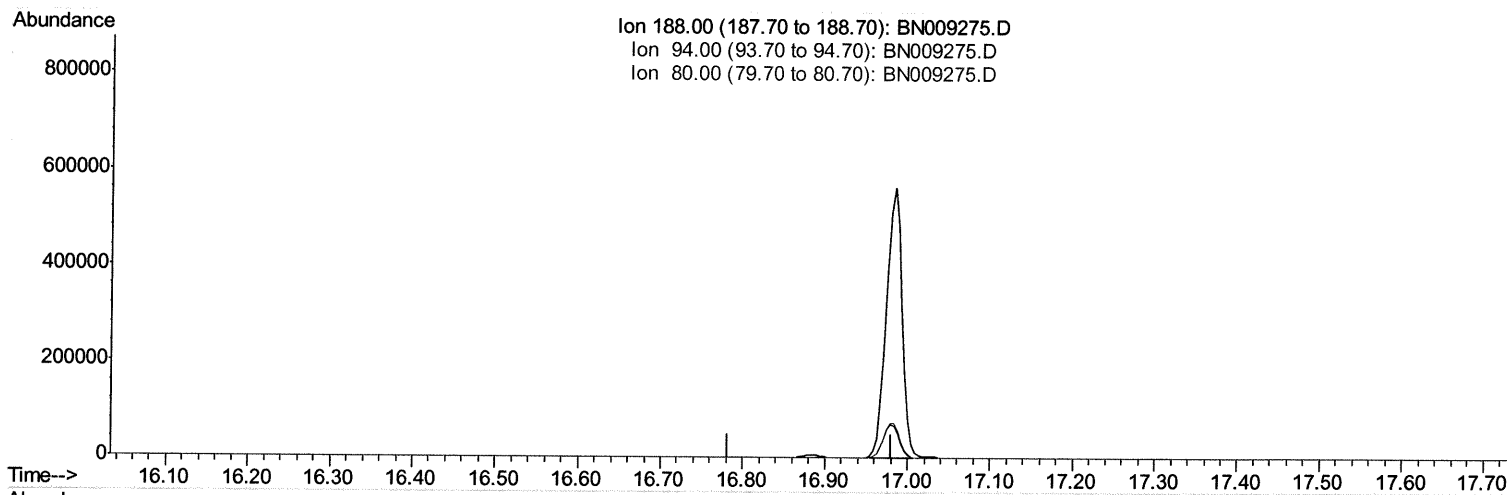

TIC: BN009275.D

(10) Phenanthrene-d10 (I)

16.882min (-16.882) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN123119\
 Data File : BN009275.D
 Acq On : 31 Dec 2019 11:24
 Operator : JU
 Sample : PB125795BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK95

Manual Integrations
 APPROVED

mohammad
 1/1/2020 8:16:52 AM

Quant Time: Dec 31 12:30:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 11:02:23 2019
 Response via : Initial Calibration

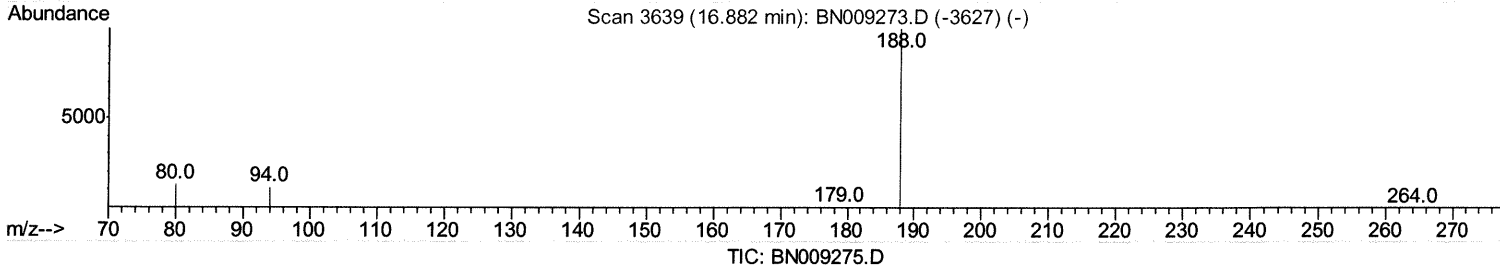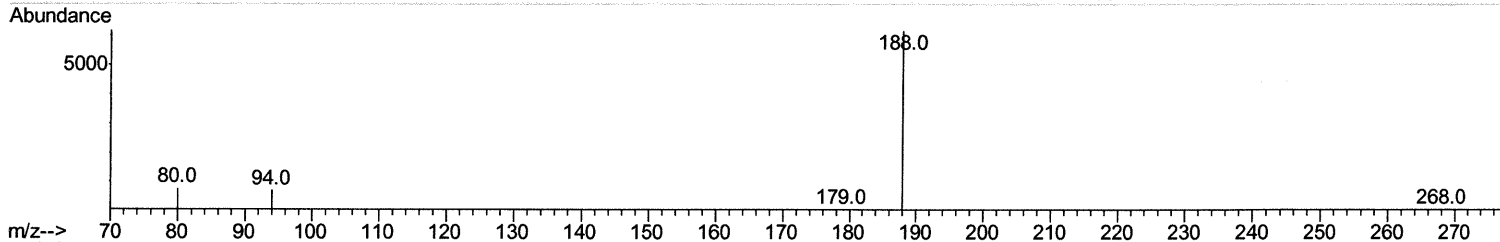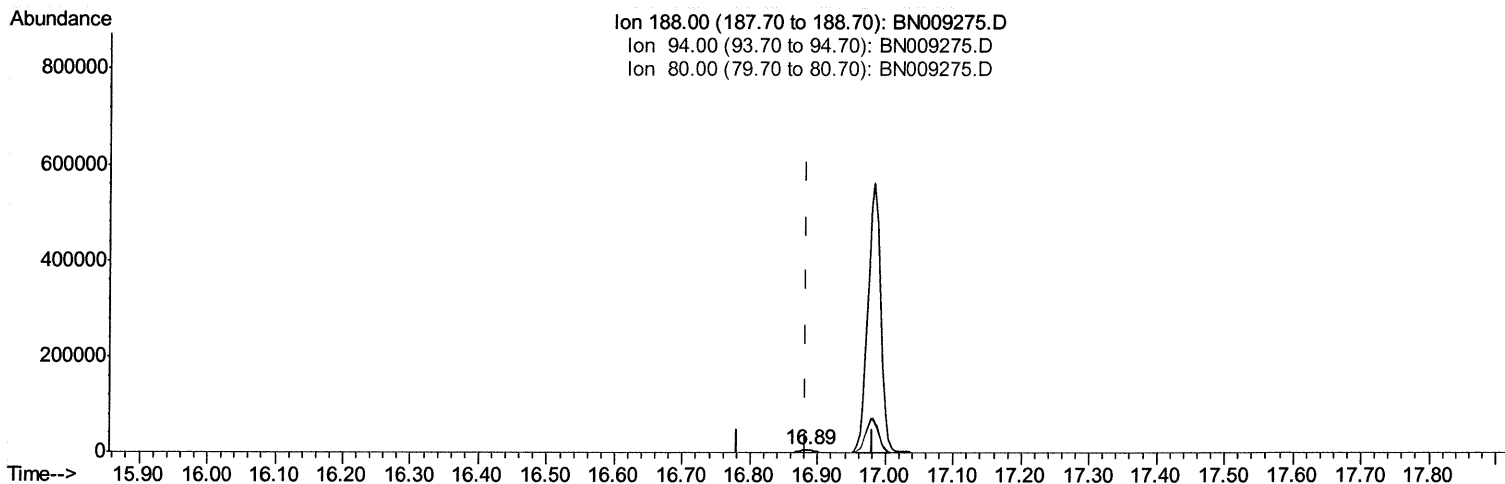

(10) Phenanthrene-d10 (I)

16.886min (+0.004) 0.40ng/ul m JU 1/2/20

response 8802

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.34
80.00	13.70	12.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN123119\
Data File : BN009275.D
Acq On : 31 Dec 2019 11:24
Operator : JU
Sample : PB125795BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK95

Manual Integrations
APPROVED

mohammad
1/1/2020 8:16:52 AM

Quant Time: Dec 31 12:31:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 11:02:23 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	2319	0.40	ng/ul	0.00
2) Naphthalene-d8	10.26	136	8366	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.13	164	4481	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.89	188	8802m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.09	240	6471	0.40	ng/ul	0.00
20) Perylene-d12	23.22	264	6820	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.86	152	4717	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.92	212	8677	0.33	ng/ul	0.00

Ju 1/2/20

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed