


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN123119\
Data File : BN009276.D
Acq On : 31 Dec 2019 12:00
Operator : JU
Sample : PB125569BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK69

Manual Integrations
APPROVED

mohammad
1/1/2020 8:16:54 AM

Quant Time: Dec 31 13:32:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 11:02:23 2019
Response via : Initial Calibration

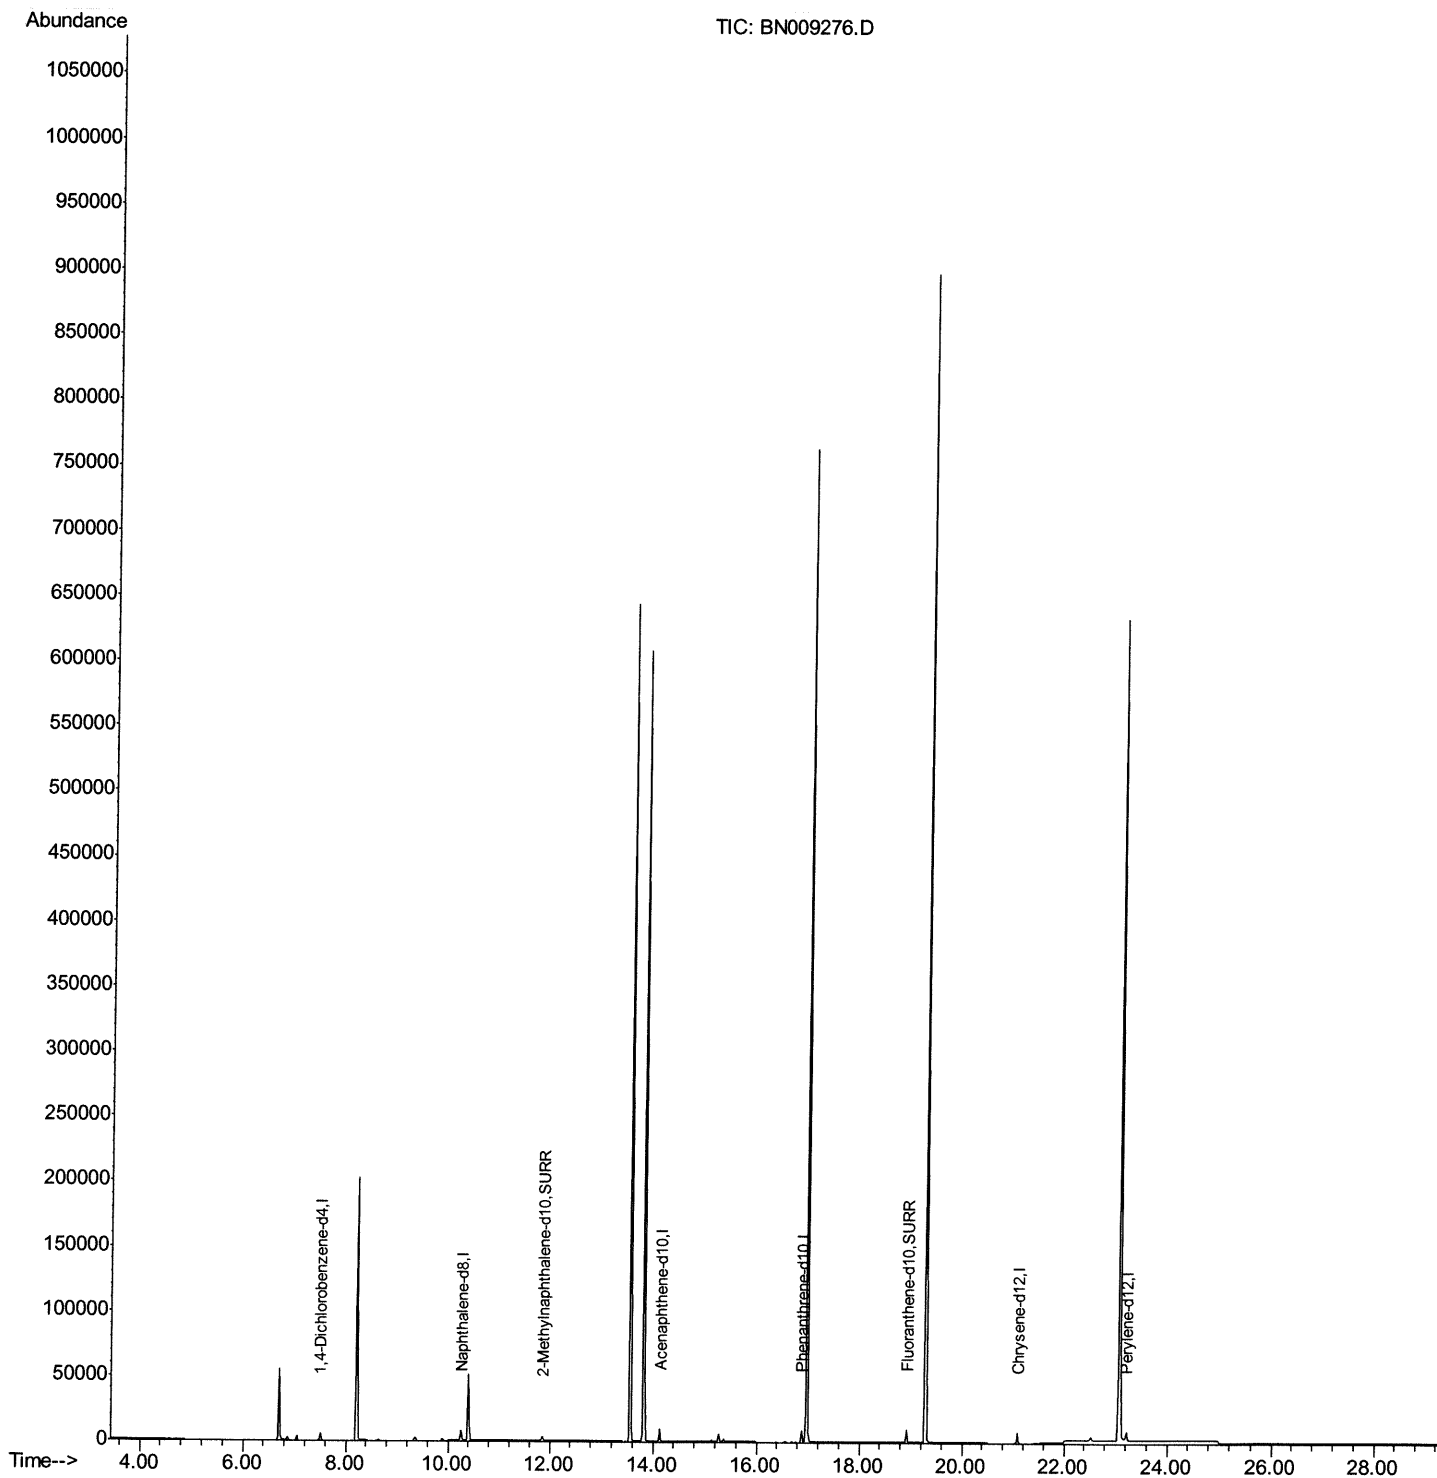

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN123119\
 Data File : BN009276.D
 Acq On : 31 Dec 2019 12:00
 Operator : JU
 Sample : PB125569BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK69

Manual Integrations
 APPROVED

mohammad
 1/1/2020 8:16:54 AM

Quant Time: Dec 31 13:31:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 11:02:23 2019
 Response via : Initial Calibration

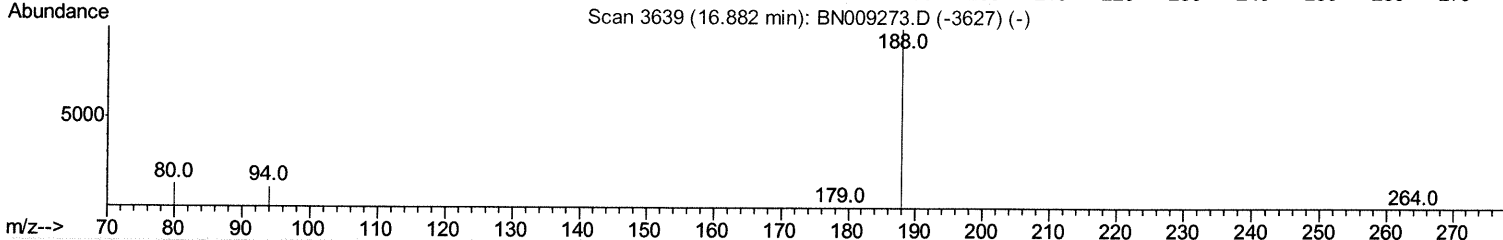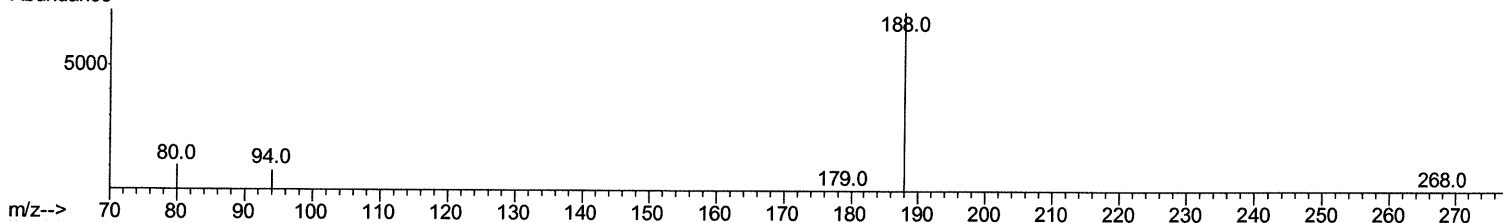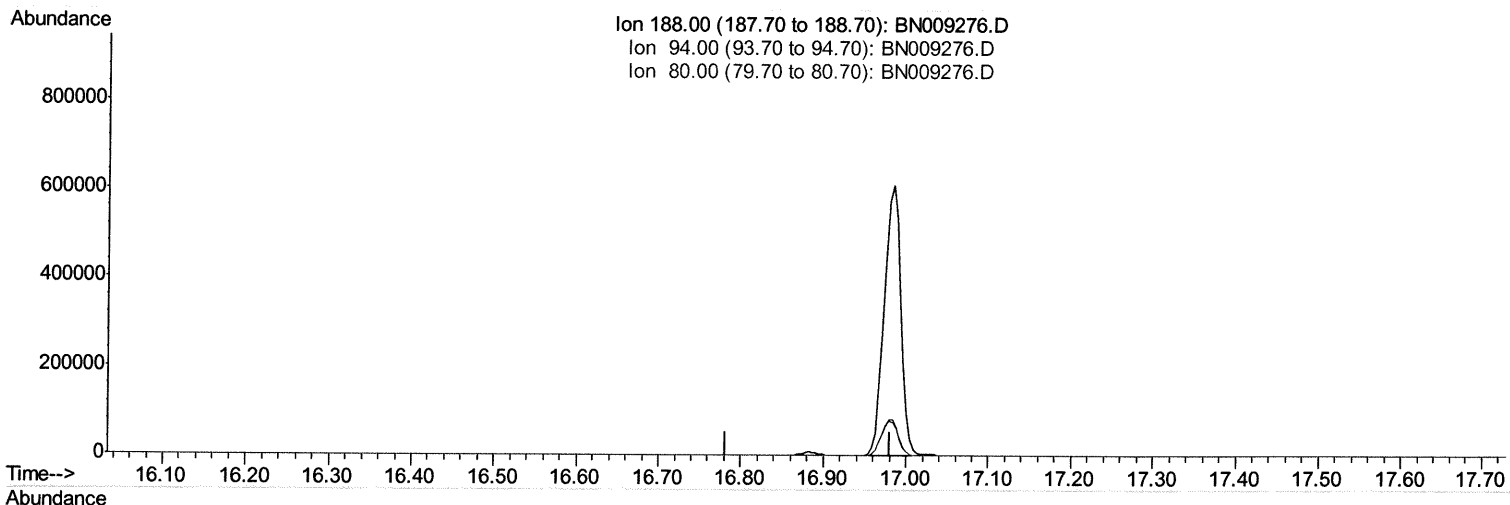

TIC: BN009276.D

(10) Phenanthrene-d10 (I)

16.882min (-16.882) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN123119\
 Data File : BN009276.D
 Acq On : 31 Dec 2019 12:00
 Operator : JU
 Sample : PB125569BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK69

Manual Integrations
 APPROVED

mohammad
 1/1/2020 8:16:54 AM

Quant Time: Dec 31 13:31:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 11:02:23 2019
 Response via : Initial Calibration

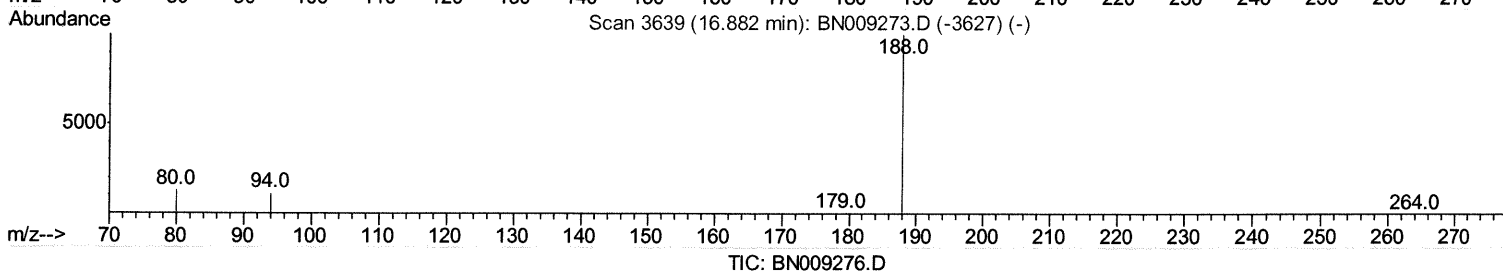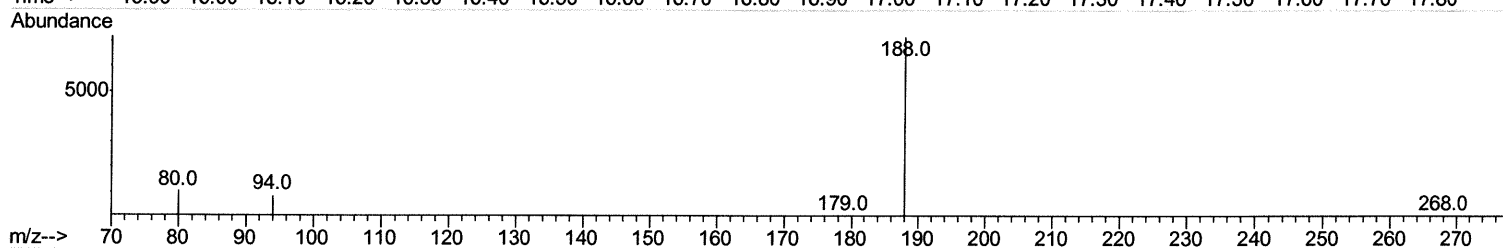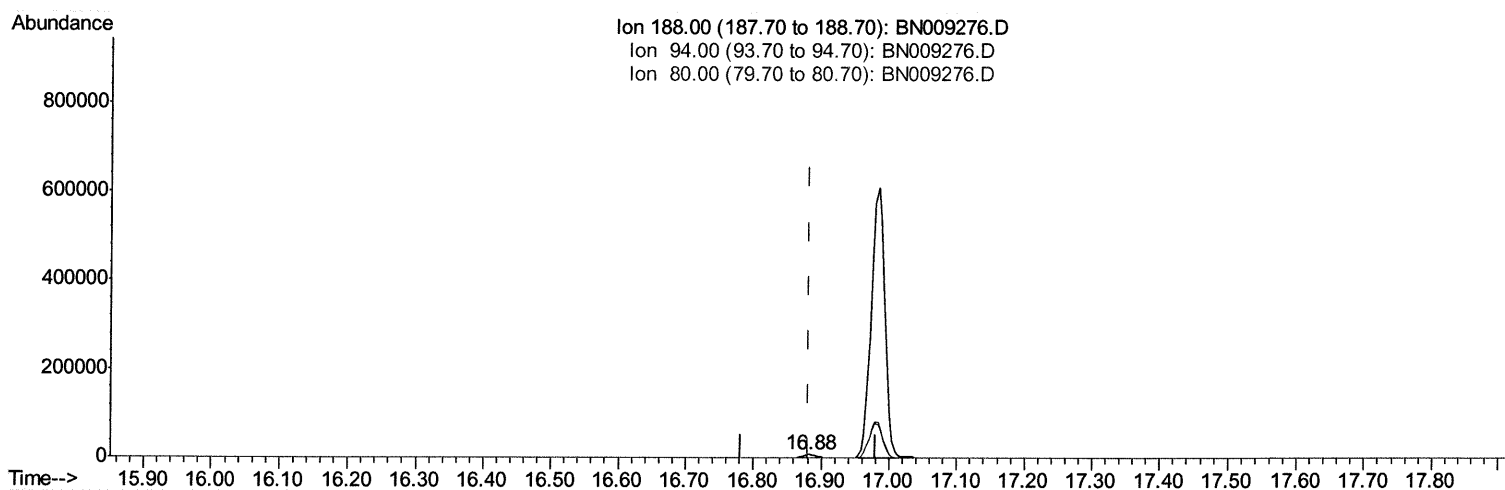

(10) Phenanthrene-d10 (I)

16.882min (-0.000) 0.40ng/ul m *JU 1/2/20*

response 10217

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.71
80.00	13.70	14.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN123119\
 Data File : BN009276.D
 Acq On : 31 Dec 2019 12:00
 Operator : JU
 Sample : PB125569BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK69

Manual Integrations
 APPROVED

mohammad
 1/1/2020 8:16:54 AM

Quant Time: Dec 31 13:32:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 11:02:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QI	on	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152		2596	0.40	ng/ul	0.00
2) Naphthalene-d8	10.26	136		9372	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.13	164		5129	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.88	188		10217m	0.40	ng/ul	0.00
16) Chrysene-d12	21.09	240		7701	0.40	ng/ul	0.00
20) Perylene-d12	23.22	264		8111	0.40	ng/ul	0.00

JU 1/2/20

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.86	152		5315	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.92	212		10241	0.34	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed