


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN123119\
Data File : BN009282.D
Acq On : 31 Dec 2019 15:36
Operator : JU
Sample : K6308-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C82

Manual Integrations
APPROVED

mohammad
1/1/2020 8:17:08 AM

Quant Time: Dec 31 17:05:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 11:02:23 2019
Response via : Initial Calibration

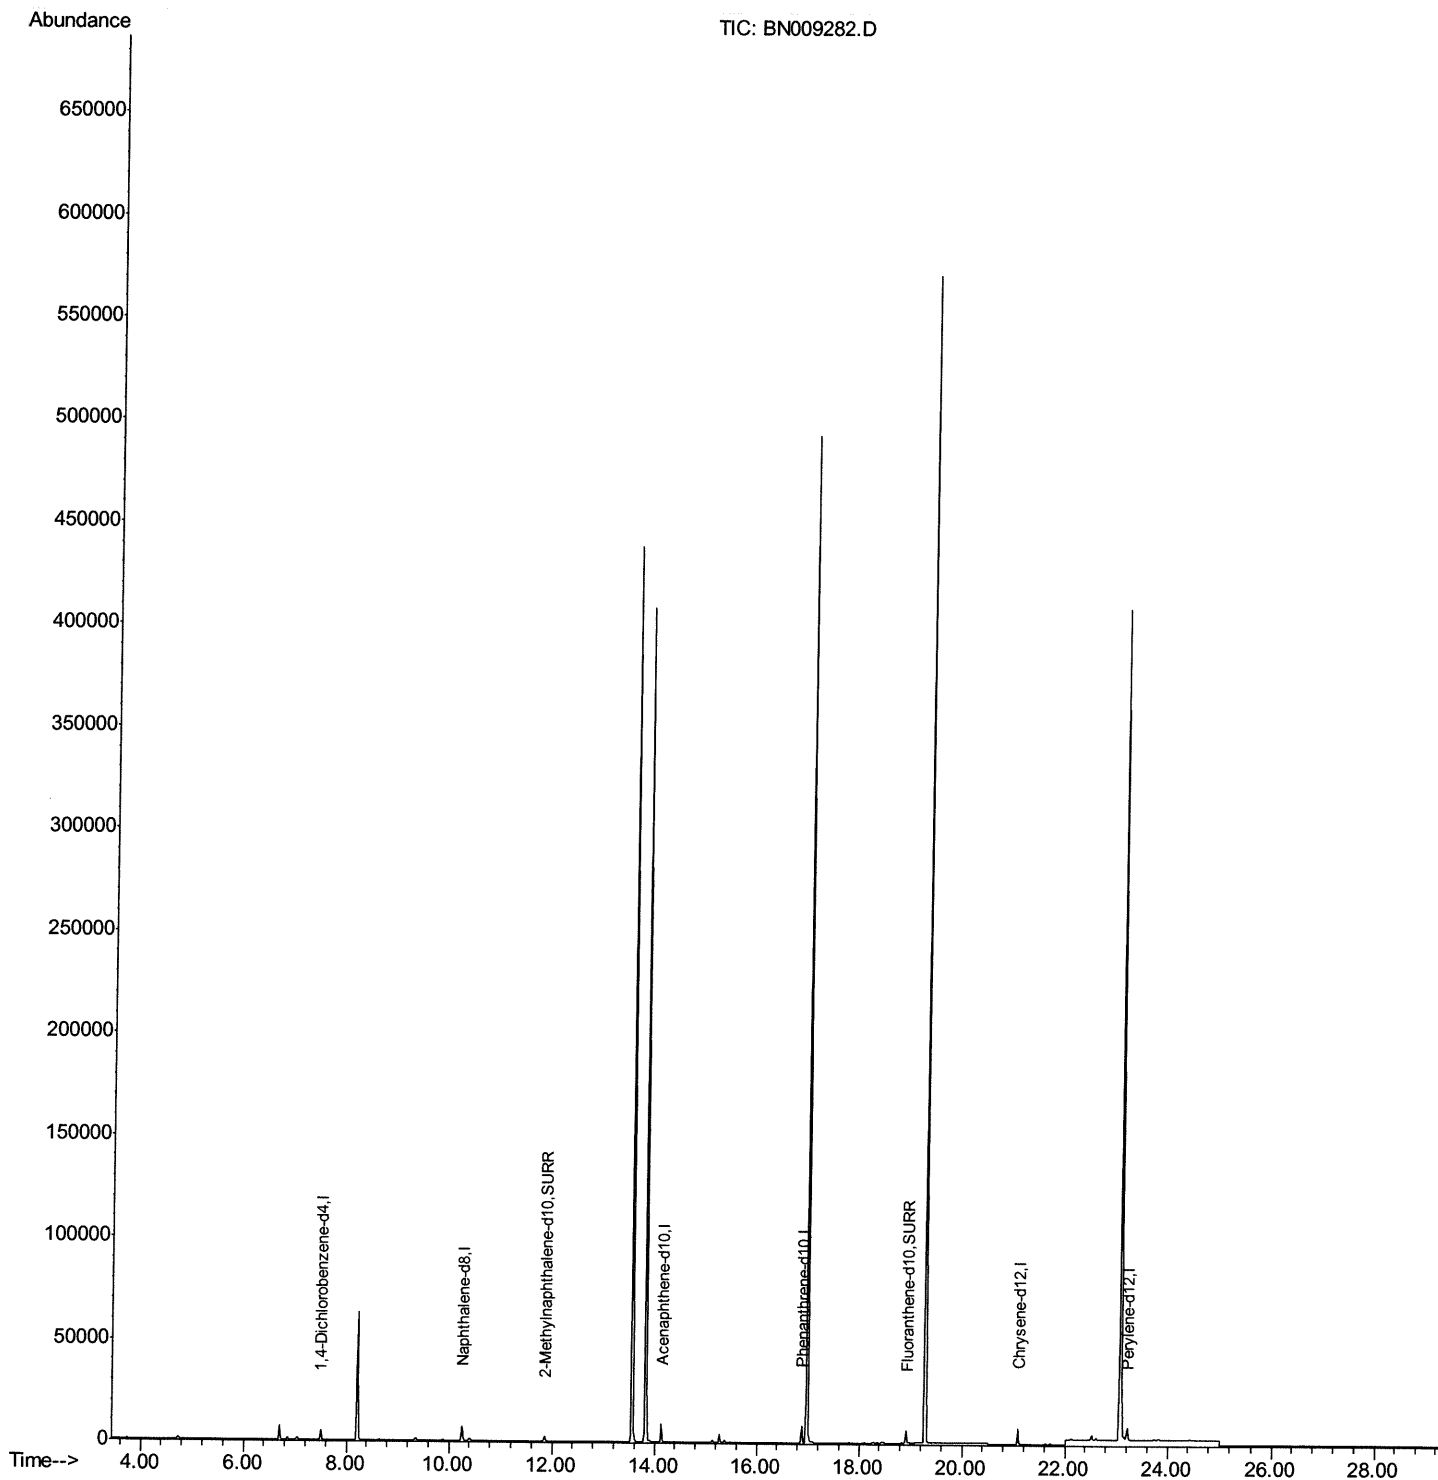

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN123119\
 Data File : BN009282.D
 Acq On : 31 Dec 2019 15:36
 Operator : JU
 Sample : K6308-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C82

Manual Integrations
 APPROVED

mohammad
 1/1/2020 8:17:08 AM

Quant Time: Dec 31 16:58:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 11:02:23 2019
 Response via : Initial Calibration

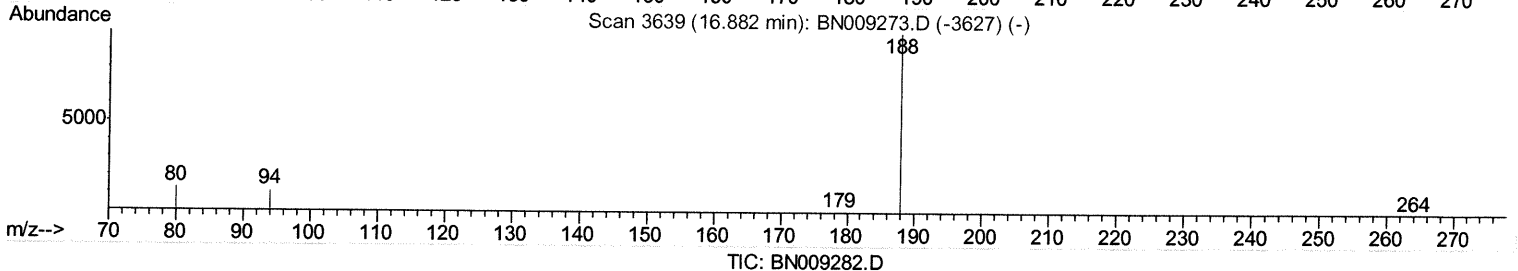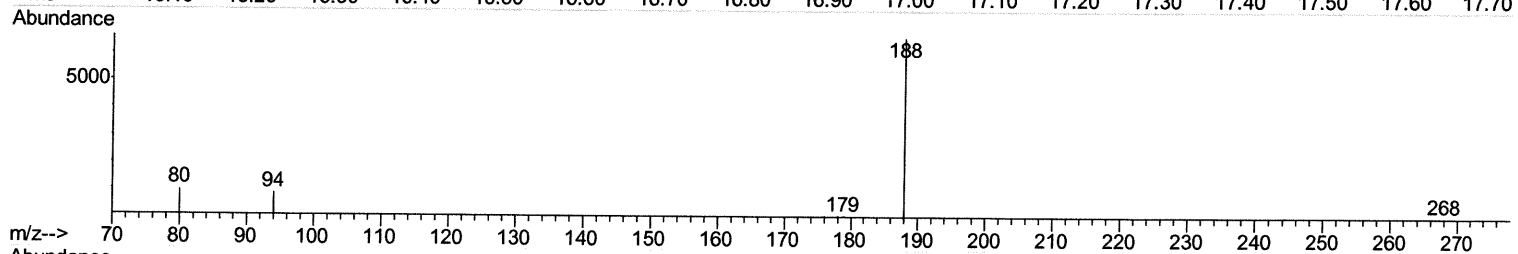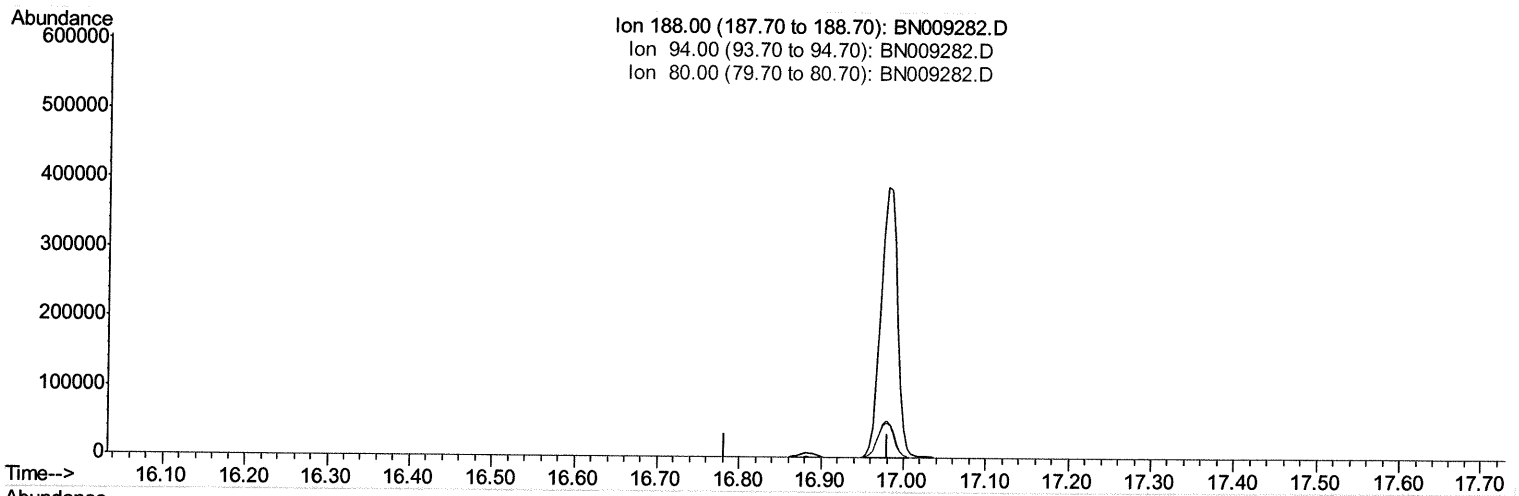

(10) Phenanthrene-d10 (I)

16.882min (-16.882) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN123119\
Data File : BN009282.D
Acq On : 31 Dec 2019 15:36
Operator : JU
Sample : K6308-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C82

Manual Integrations
APPROVED

mohammad
1/1/2020 8:17:08 AM

Quant Time: Dec 31 16:58:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 11:02:23 2019
Response via : Initial Calibration

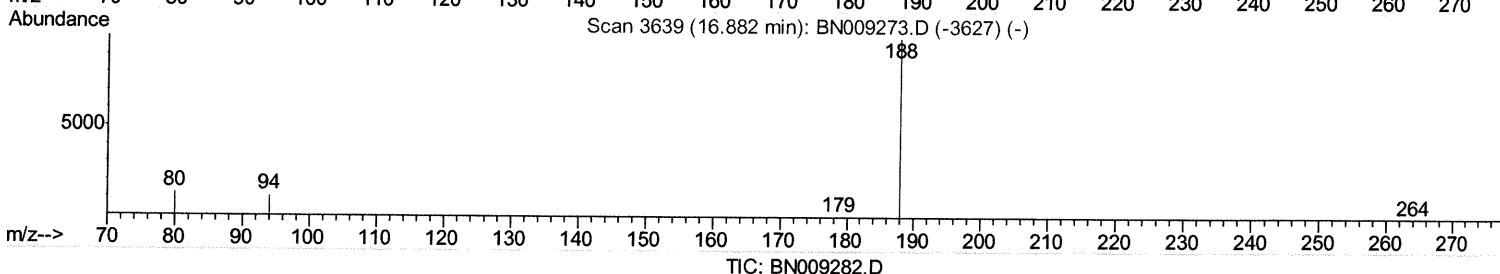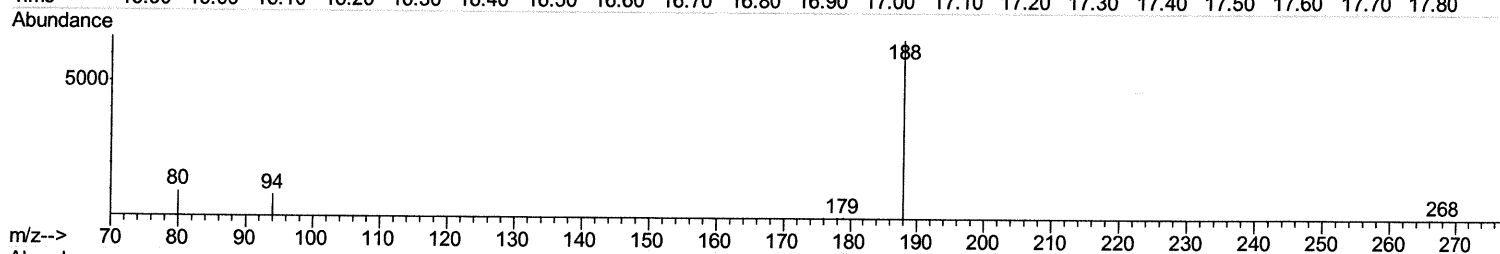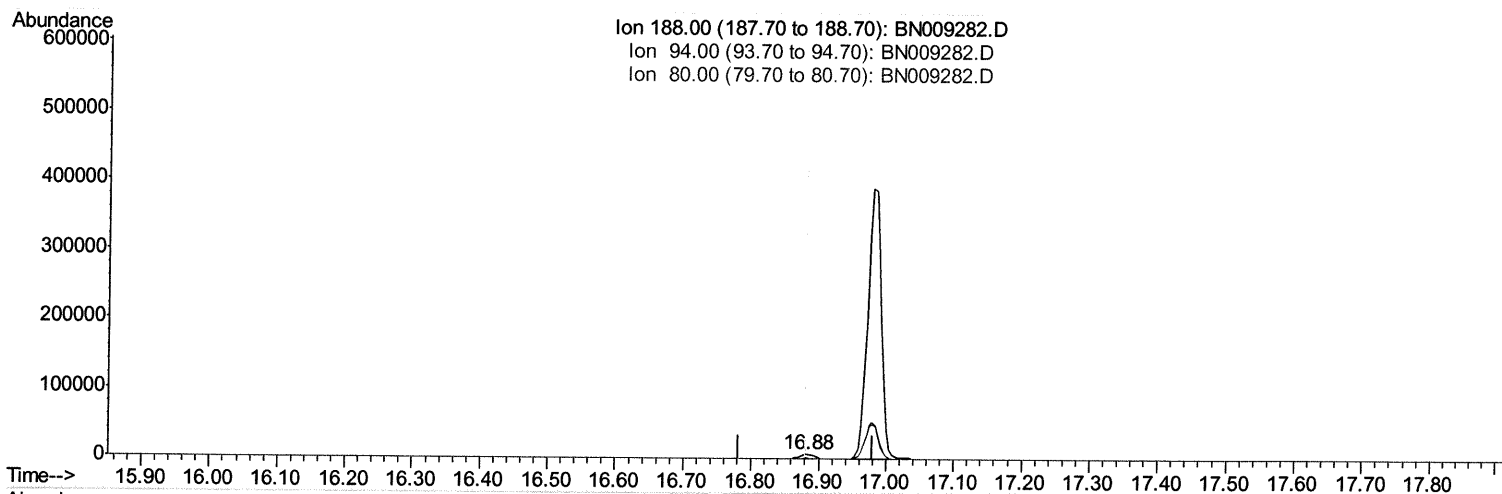

(10) Phenanthrene-d10 (I)

16.882min (+0.000) 0.40ng/ul m JU 1/2/20

response 9363

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	12.62
80.00	13.70	14.49
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN123119\
 Data File : BN009282.D
 Acq On : 31 Dec 2019 15:36
 Operator : JU
 Sample : K6308-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C82

Manual Integrations
 APPROVED

mohammad
 1/1/2020 8:17:08 AM

Quant Time: Dec 31 17:05:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 11:02:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	2505	0.40	ng/ul	0.00
2) Naphthalene-d8	10.26	136	9034	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.13	164	4705	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.88	188	9363m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.09	240	6925	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	7349	0.40	ng/ul	0.00

JU 1/2/20

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.86	152	3250	0.20	ng/ul	0.00
14) Fluoranthene-d10	18.92	212	6878	0.25	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed