

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR022019\
 Data File : VR026349.D
 Acq On : 20 Feb 2019 12:54
 Operator : SY/MD
 Sample : K1488-06
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 ESXD2

Quant Time: Feb 21 07:54:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR021919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 21 07:38:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	628900	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	540307	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	152430	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.16	65	240542	4.84	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.80%
7) Chloroethane-d5	2.62	69	226836	5.23	ug/L	0.00
Spiked Amount	7.000	Range	65 - 130	Recovery	=	74.71%
11) 1,1-Dichloroethene-d2	3.61	63	492346	3.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.60%
20) 2-Butanone-d5	6.58	46	186455	49.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.66%
24) Chloroform-d	7.20	84	440185	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
26) 1,2-Dichloroethane-d4	7.89	65	169698	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
32) Benzene-d6	7.85	84	838371	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
36) 1,2-Dichloropropane-d6	8.89	67	216531	4.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.40%
41) Toluene-d8	9.97	98	774823	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
43) trans-1,3-Dichloropropene-	10.23	79	49916	4.23	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.60%
46) 2-Hexanone-d5	10.59	63	152624	51.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.28%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	80787	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	140336	5.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.20%


Target Compounds					Ovalue
13) Acetone	3.70	43	9085	2.285 ug/L	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR022019\
Data File : VR026349.D
Acq On : 20 Feb 2019 12:54
Operator : SY/MD
Sample : K1488-06
Misc : 25mL/MSVOA R/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
ESXD2

Quant Time: Feb 21 07:54:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR021919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Feb 21 07:38:25 2019
Response via : Initial Calibration

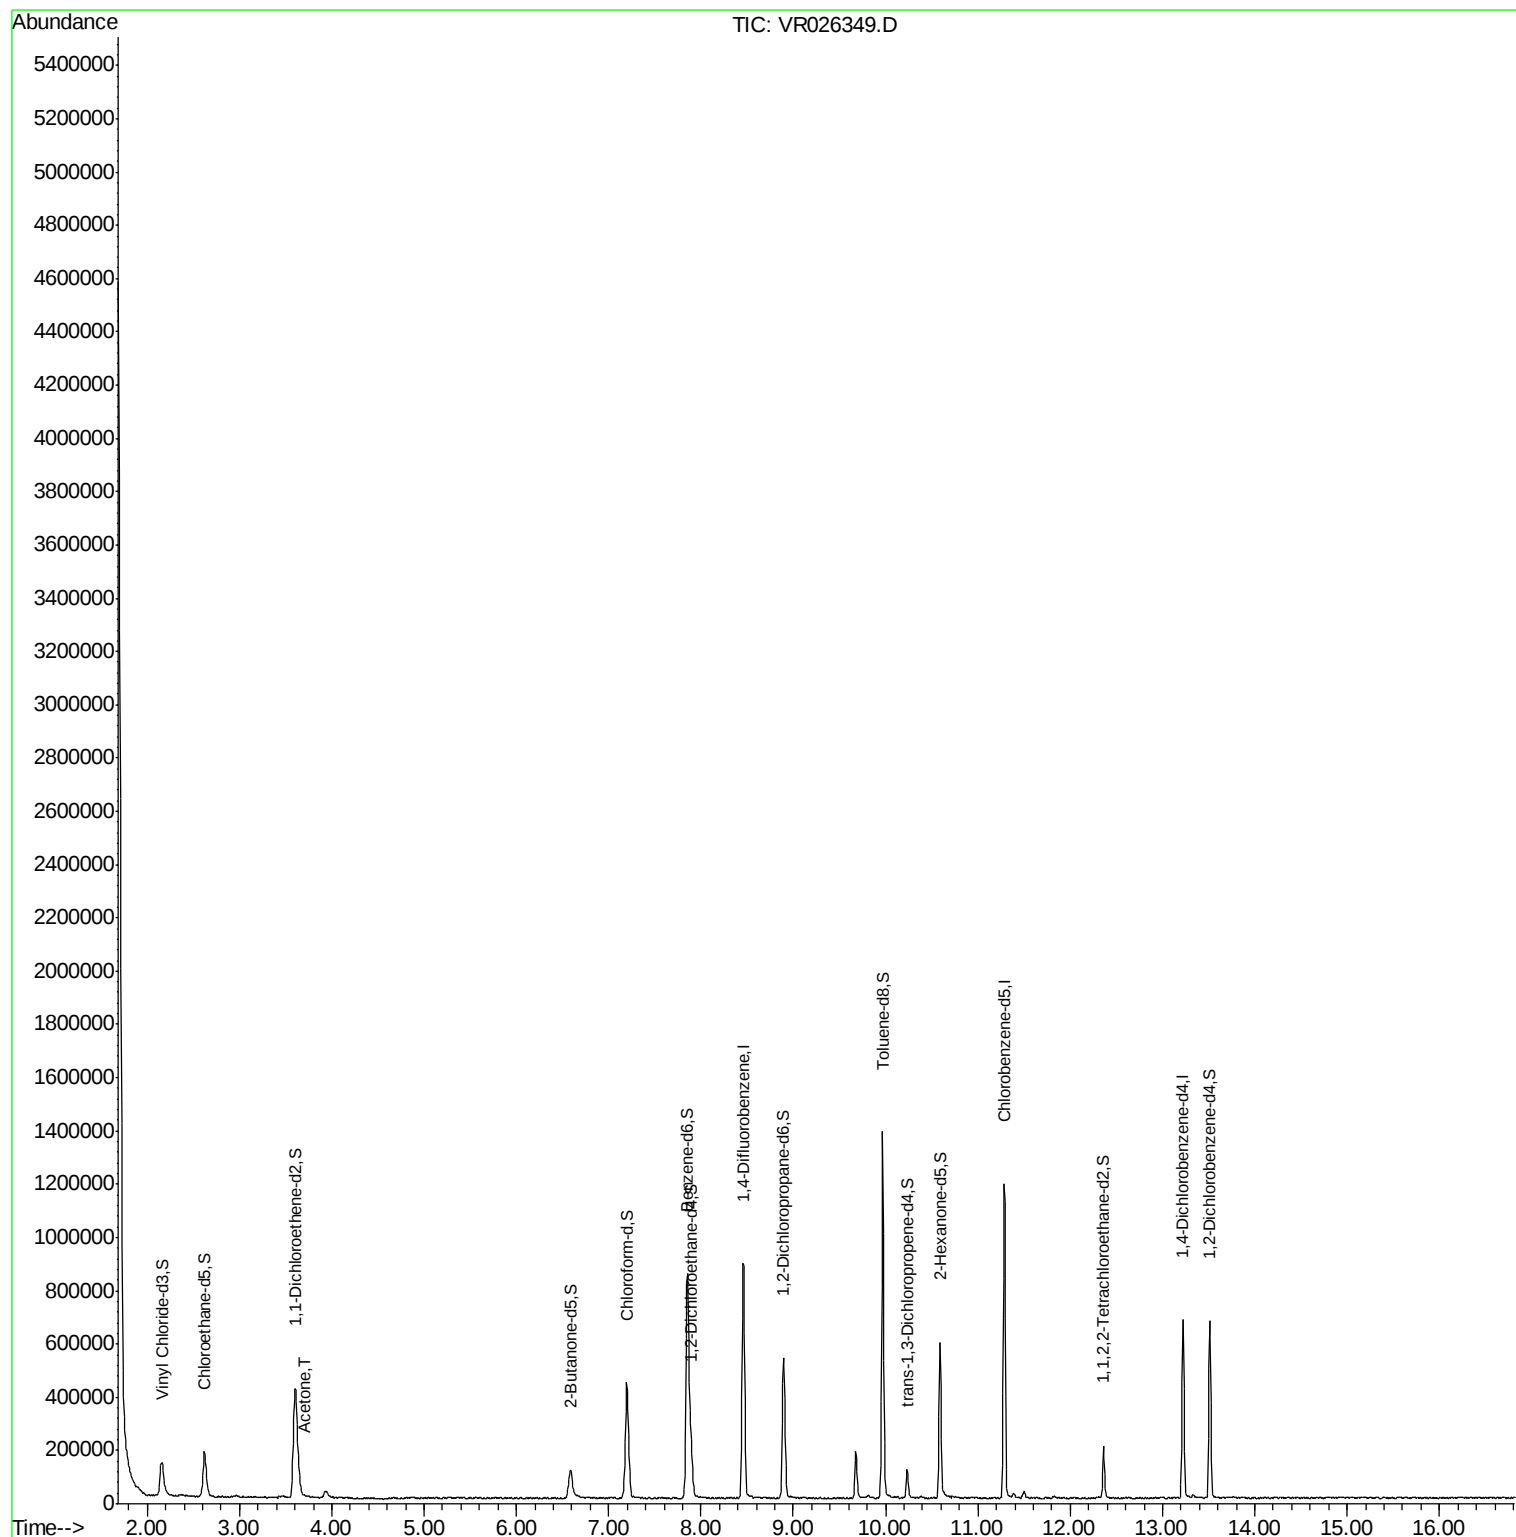

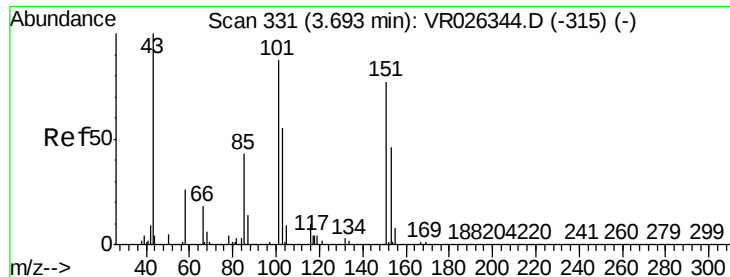

#13

Acetone

Concen: 2.285 ug/L

RT: 3.70 min Scan# 333

Delta R.T. 0.01 min

Lab File: VR026349.D

Acq: 20 Feb 2019 12:54

Instrument :
MSVOA_R
ClientSampleId :
ESXD2

Tot Ion: 43 Resp: 9085

Ion Ratio Lower Upper

43 100

58 11.8 0.0 58.0

