

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR022519\
 Data File : VR026372.D
 Acq On : 25 Feb 2019 13:14
 Operator : SY/MD
 Sample : K1589-08
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C09Q2

Quant Time: Feb 26 06:35:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR022219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Feb 26 06:18:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	528478	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.28	117	447389	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	143339	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.13	65	172875	3.34	ug/L	-0.02
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.80%
7) Chloroethane-d5	2.62	69	151816	3.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	71.60%
11) 1,1-Dichloroethene-d2	3.60	63	346244	2.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.00%#
20) 2-Butanone-d5	6.58	46	177295	46.99	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.98%
24) Chloroform-d	7.19	84	353914	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.00%
26) 1,2-Dichloroethane-d4	7.89	65	147615	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
32) Benzene-d6	7.85	84	633902	3.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.40%
36) 1,2-Dichloropropane-d6	8.89	67	173436	4.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	81.40%
41) Toluene-d8	9.96	98	546054	3.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.00%
43) trans-1,3-Dichloropropene-	10.24	79	39349	3.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.00%
46) 2-Hexanone-d5	10.59	63	155454	54.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.54%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	68041	4.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.20%
64) 1,2-Dichlorobenzene-d4	13.51	152	119178	4.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.20%


Target Compounds					Ovalue
13) Acetone	3.70	43	10170	2.996 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR022519\
Data File : VR026372.D
Acq On : 25 Feb 2019 13:14
Operator : SY/MD
Sample : K1589-08
Misc : 25mL/MSVOA R/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C09Q2

Quant Time: Feb 26 06:35:15 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR022219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Feb 26 06:18:07 2019
Response via : Initial Calibration

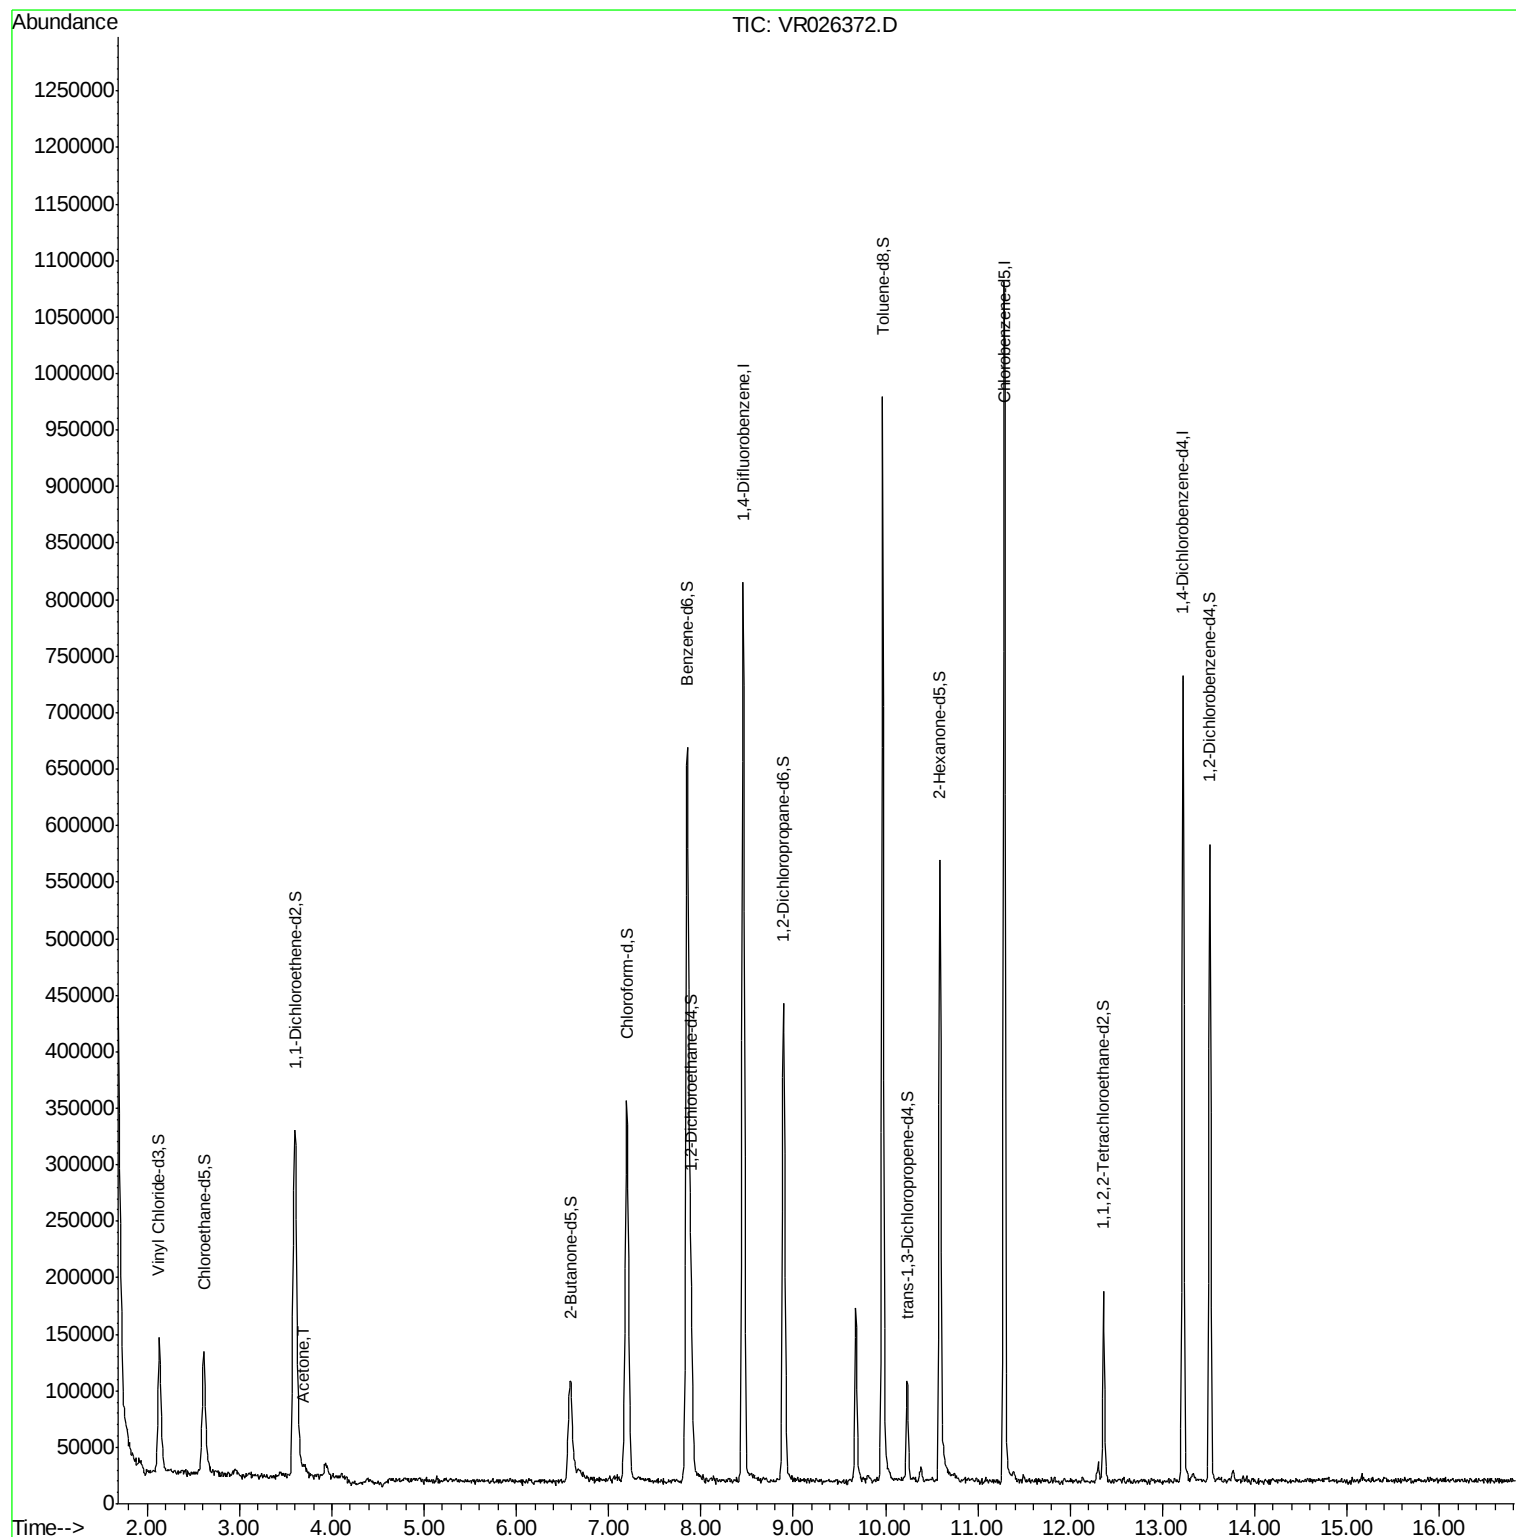

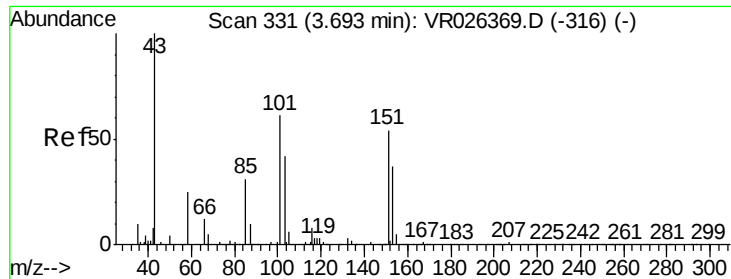

#13

Acetone

Concen: 2.996 ug/L

RT: 3.70 min Scan# 332

Delta R.T. 0.01 min

Lab File: VR026372.D

Acq: 25 Feb 2019 13:14

Instrument :
MSVOA_R
ClientSampleId :
C09Q2

Tot Ion: 43 Resp: 10170

Ion Ratio Lower Upper

43 100

58 23.9 0.0 52.2

