

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR040419\
 Data File : VR026450.D
 Acq On : 4 Apr 2019 17:00
 Operator : SY/MD
 Sample : K2271-11
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 DB7D2

Quant Time: Apr 05 07:53:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 05 07:16:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	469921	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.28	117	384843	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	113199	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	182839	5.12	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	102.40%
7) Chloroethane-d5	2.62	69	151741	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.00%
11) 1,1-Dichloroethene-d2	3.60	63	359190	3.89	ug/L	-0.02
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.80%
20) 2-Butanone-d5	6.58	46	168373	52.89	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.78%
24) Chloroform-d	7.20	84	332631	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	7.89	65	142930	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
32) Benzene-d6	7.85	84	606830	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	8.89	67	162387	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	9.97	98	533762	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
43) trans-1,3-Dichloropropene-	10.23	79	37882	4.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.60%
46) 2-Hexanone-d5	10.59	63	127523	56.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.58%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	59610	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	13.51	152	104556	6.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.00%#


Target Compounds				Ovalue
3) Chloromethane	2.00	50	14653	0.288 ug/L 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR040419\
Data File : VR026450.D
Acq On : 4 Apr 2019 17:00
Operator : SY/MD
Sample : K2271-11
Misc : 25mL/MSVOA R/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
DB7D2

Quant Time: Apr 05 07:53:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 05 07:16:54 2019
Response via : Initial Calibration

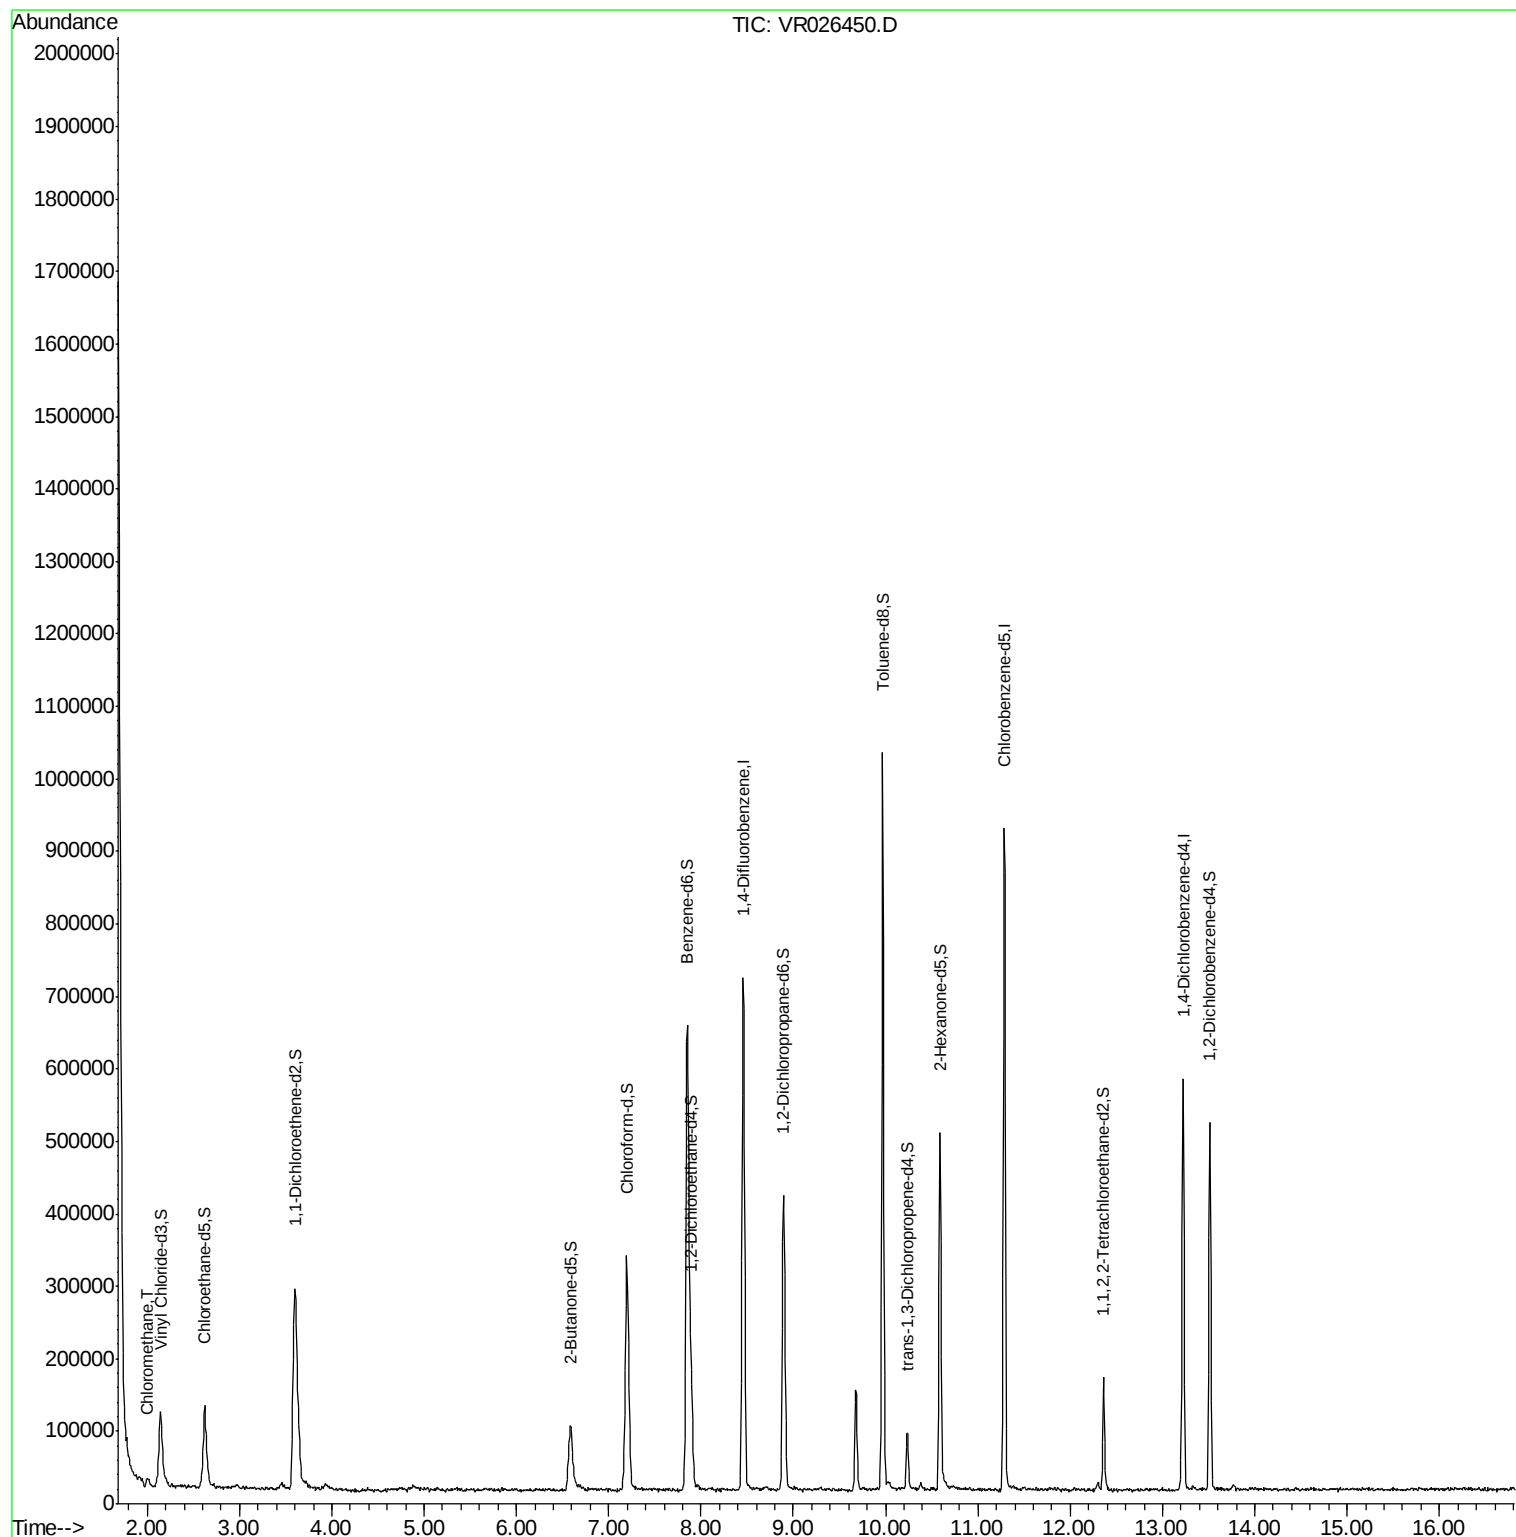

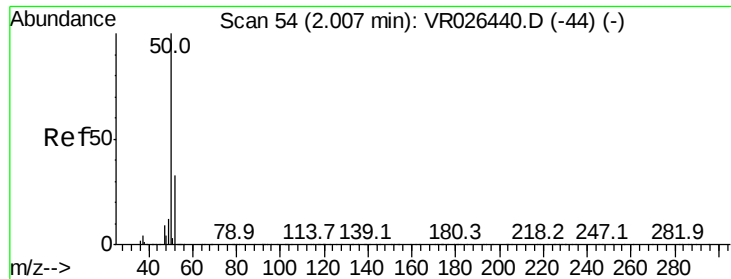

#3
 Chloromethane
 Concen: 0.288 ug/L
 RT: 2.00 min Scan# 53
 Delta R.T. -0.01 min
 Lab File: VR026450.D
 Acq: 4 Apr 2019 17:00

Instrument :
 MSVOA_R
 ClientSampleId :
 DB7D2

Tot Ion: 50 Resp: 14653
 Ion Ratio Lower Upper
 50 100
 52 24.1 22.5 41.9

