

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR040519\
 Data File : VR026463.D
 Acq On : 5 Apr 2019 14:47
 Operator : SY/MD
 Sample : K2271-19
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 DB7E0

Quant Time: Apr 06 06:45:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 06 05:54:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	517374	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	420356	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	122099	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	157512	4.01	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.20%
7) Chloroethane-d5	2.62	69	142518	4.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.00%
11) 1,1-Dichloroethene-d2	3.60	63	324608	3.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.80%
20) 2-Butanone-d5	6.58	46	152522	43.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.04%
24) Chloroform-d	7.20	84	304449	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.40%
26) 1,2-Dichloroethane-d4	7.89	65	130850	4.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.40%
32) Benzene-d6	7.85	84	547457	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
36) 1,2-Dichloropropane-d6	8.89	67	151211	4.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.00%
41) Toluene-d8	9.97	98	487803	4.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.00%
43) trans-1,3-Dichloropropene-	10.23	79	28984	3.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	62.80%
46) 2-Hexanone-d5	10.59	63	110854	44.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.58%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	52366	3.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.20%
64) 1,2-Dichlorobenzene-d4	13.51	152	88836	4.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.00%


Target Compounds					Ovalue
13) Acetone	3.69	43	7525	2.125 ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR040519\
Data File : VR026463.D
Acq On : 5 Apr 2019 14:47
Operator : SY/MD
Sample : K2271-19
Misc : 25mL/MSVOA R/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
DB7E0

Quant Time: Apr 06 06:45:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Apr 06 05:54:53 2019
Response via : Initial Calibration

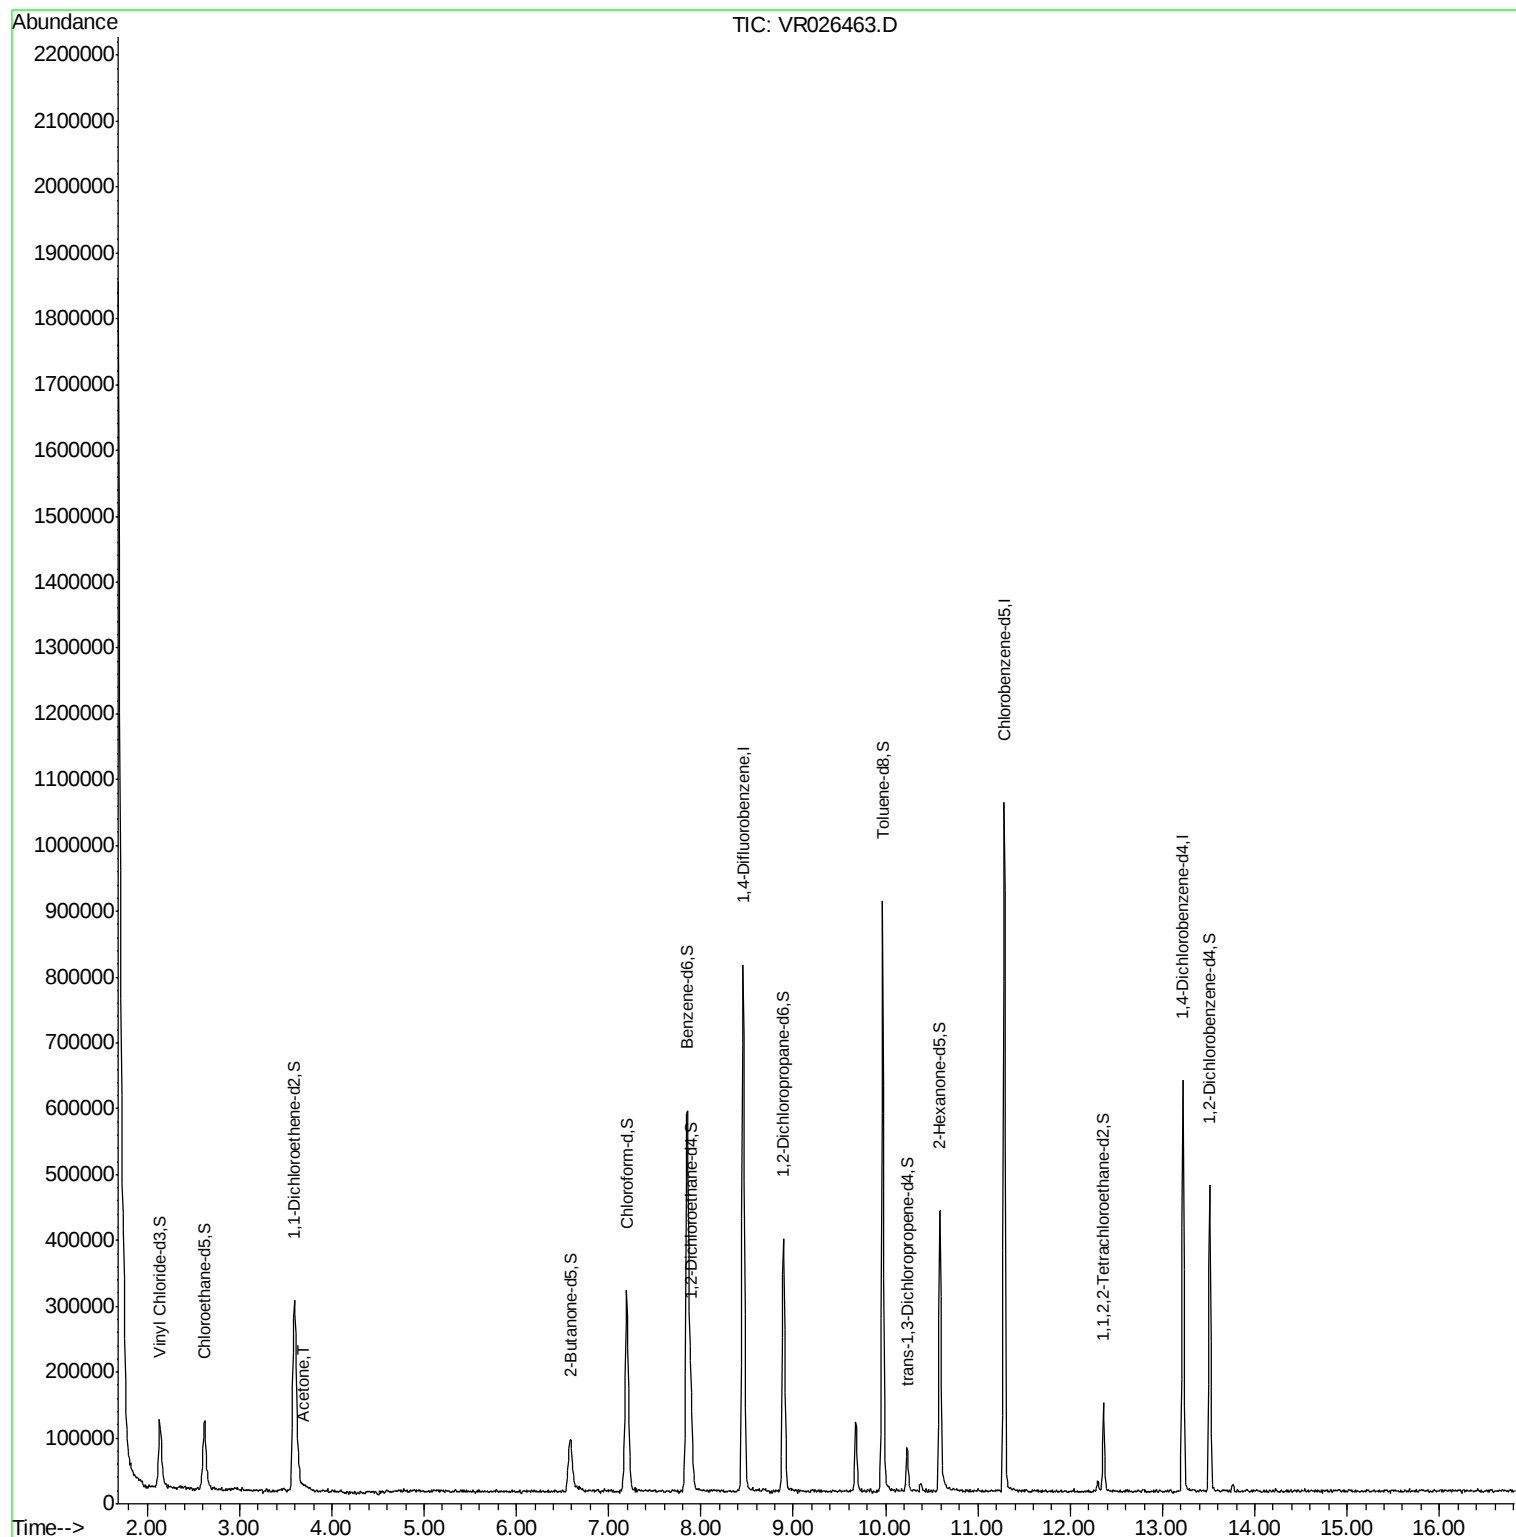

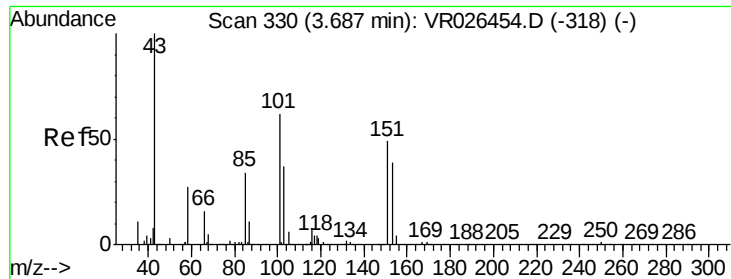

#13

Acetone

Concen: 2.125 ug/L

RT: 3.69 min Scan# 330

Delta R.T. 0.00 min

Lab File: VR026463.D

Acq: 5 Apr 2019 14:47

Instrument :
MSVOA_R
ClientSampleId :
DB7E0

Tot Ion: 43 Resp: 7525

Ion Ratio Lower Upper

43 100

58 14.5 0.0 53.8

