

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR040519\
 Data File : VR026464.D
 Acq On : 5 Apr 2019 15:19
 Operator : SY/MD
 Sample : K2282-01
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEYZ9

Quant Time: Apr 06 06:47:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 06 05:54:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	466321	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.28	117	382213	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	114369	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	157452	4.44	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.80%
7) Chloroethane-d5	2.62	69	140421	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.00%
11) 1,1-Dichloroethene-d2	3.60	63	320909	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	6.58	46	155820	49.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.66%
24) Chloroform-d	7.20	84	308035	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
26) 1,2-Dichloroethane-d4	7.89	65	134878	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
32) Benzene-d6	7.85	84	553436	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
36) 1,2-Dichloropropane-d6	8.89	67	153433	4.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.00%
41) Toluene-d8	9.97	98	493788	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
43) trans-1,3-Dichloropropene-	10.24	79	29542	3.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.40%
46) 2-Hexanone-d5	10.59	63	123233	54.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.54%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	58274	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.40%
64) 1,2-Dichlorobenzene-d4	13.51	152	97969	5.66	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.20%


Target Compounds					Ovalue
29) 1,1,1-Trichloroethane	7.43	97	12437	0.197 ug/L	94
34) Trichloroethene	8.71	95	95924	2.397 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR040519\
Data File : VR026464.D
Acq On : 5 Apr 2019 15:19
Operator : SY/MD
Sample : K2282-01
Misc : 25mL/MSVOA R/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEYZ9

Quant Time: Apr 06 06:47:31 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Apr 06 05:54:53 2019
Response via : Initial Calibration

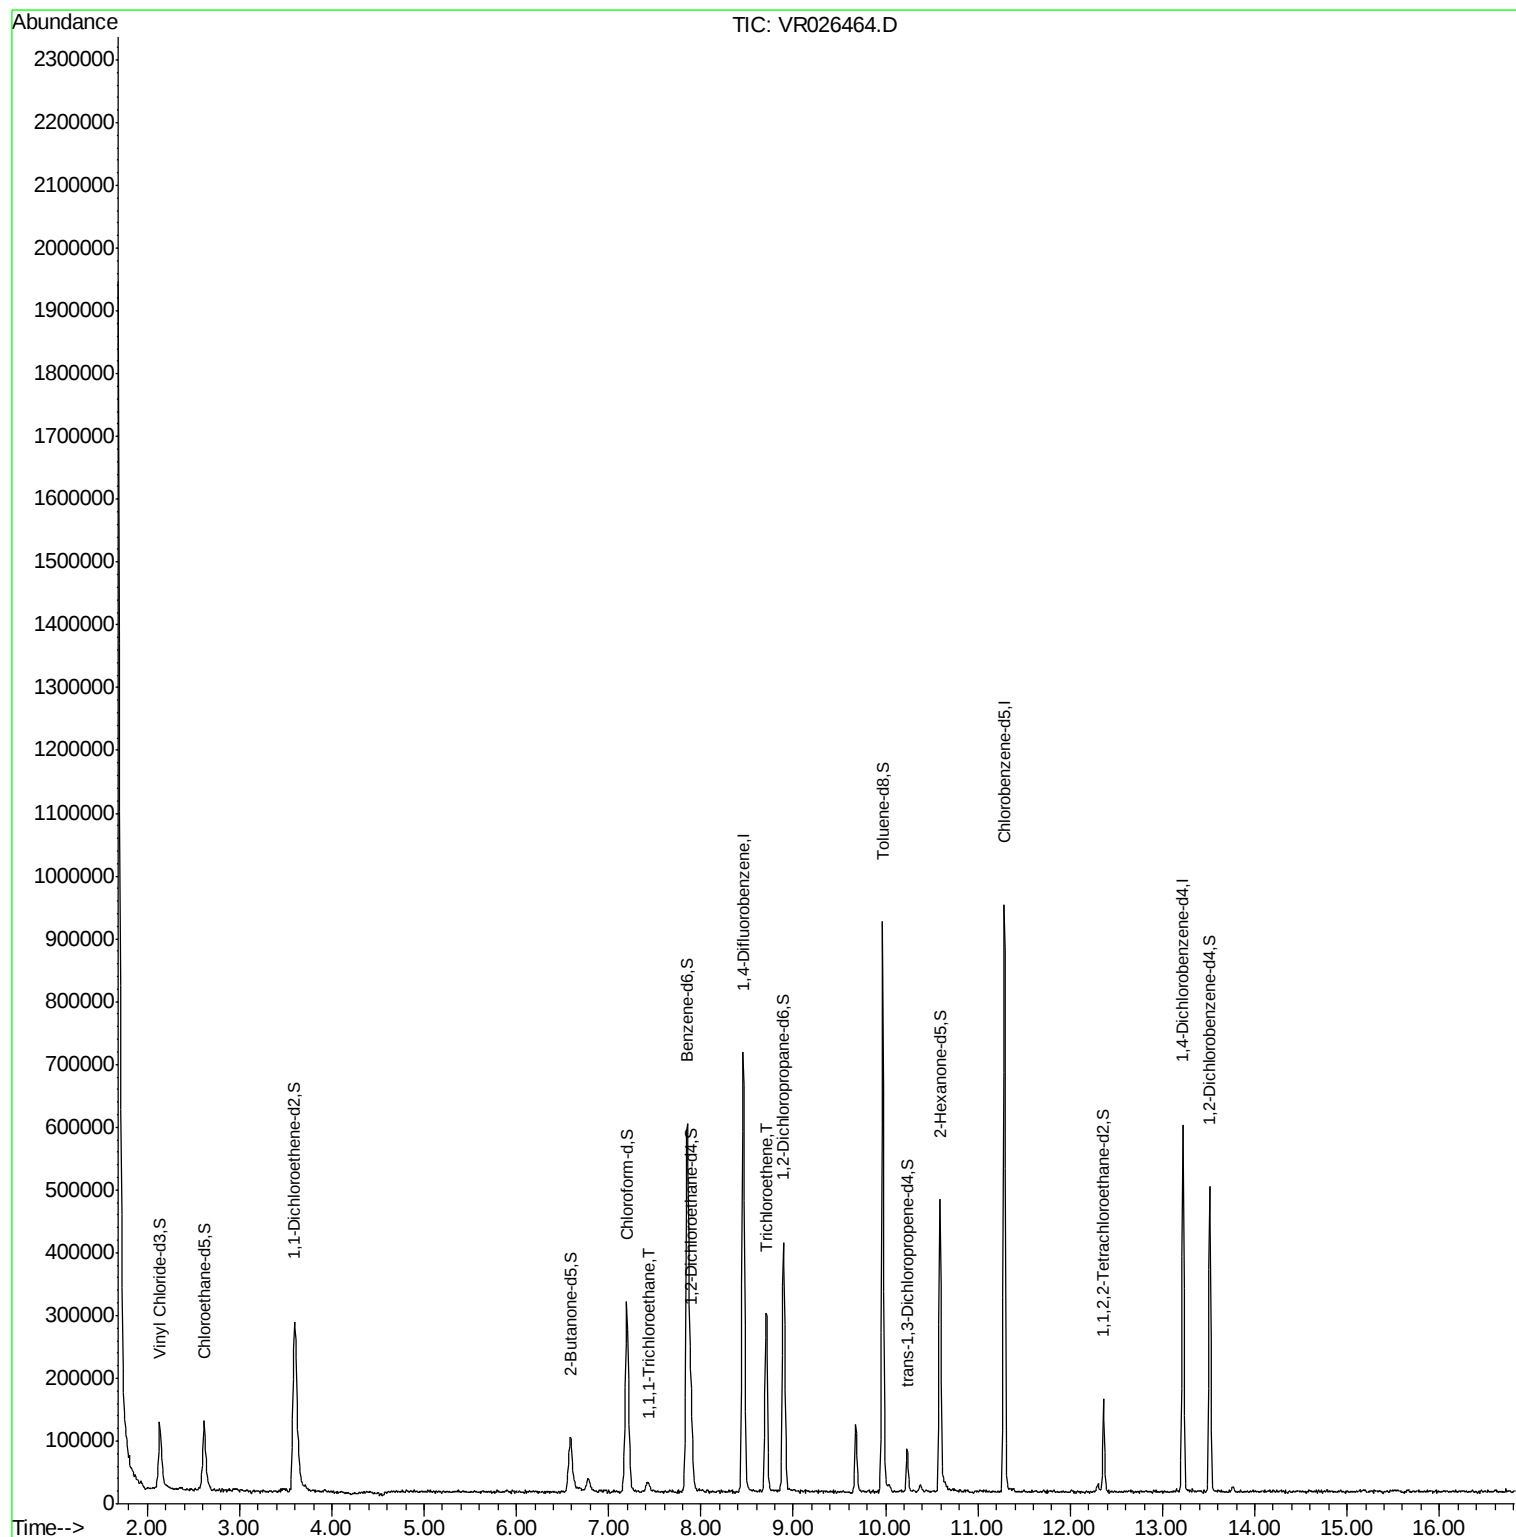

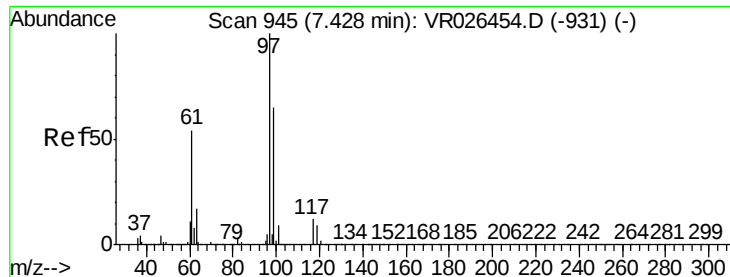

#29

1,1,1-Trichloroethane

Concen: 0.197 ug/L

RT: 7.43 min Scan# 945

Delta R.T. -0.00 min

Lab File: VR026464.D

Acq: 5 Apr 2019 15:19

Instrument :

MSVOA_R

ClientSampleId :

BEYZ9


Tot Ion: 97 Resp: 12437

Ion Ratio Lower Upper

97 100

99 68.8 49.6 74.4




61 54.8 41.8 62.6

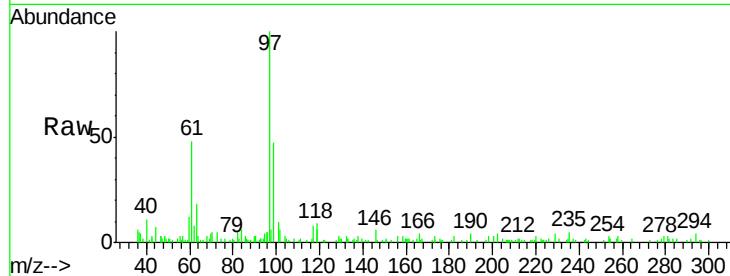

Abundance Ion 96.95 (96.65 to 97.65): VR0

Ion 99.05 (98.75 to 99.75): VR0

Ion 61.05 (60.75 to 61.75): VR0

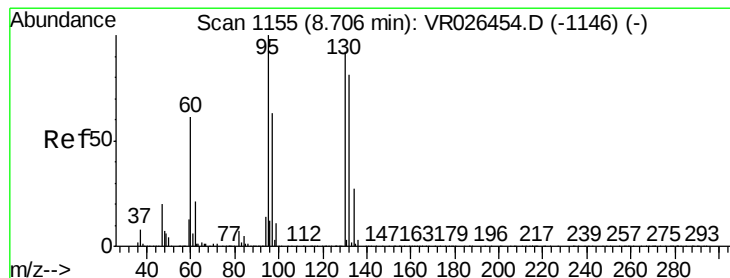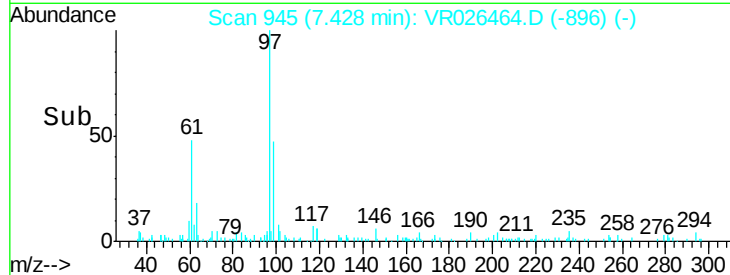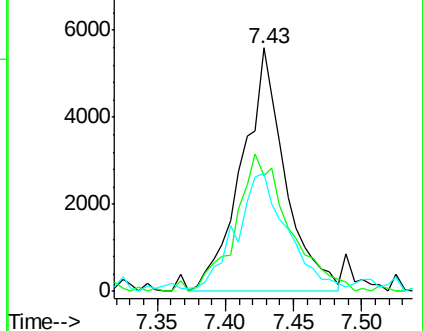

#34

Trichloroethene

Concen: 2.397 ug/L

RT: 8.71 min Scan# 1155

Delta R.T. -0.00 min

Lab File: VR026464.D

Acq: 5 Apr 2019 15:19

Tgt Ion: 95 Resp: 95924


Ion Ratio Lower Upper

95 100

97 59.4 43.8 81.3

132 79.9 57.2 106.2

130 82.4 59.7 110.9

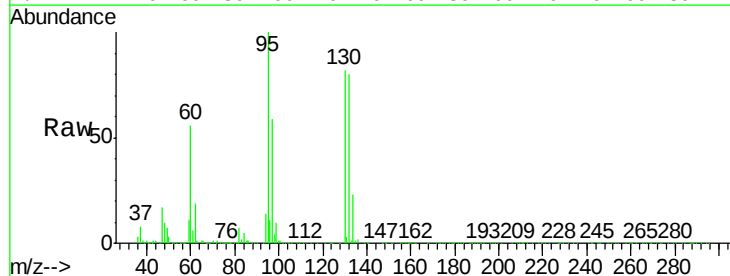

Abundance Ion 95.00 (94.70 to 95.70): VR0

Ion 96.95 (96.65 to 97.65): VR0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

