

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR040619\
 Data File : VR026484.D
 Acq On : 6 Apr 2019 20:20
 Operator : SY/MD
 Sample : K2282-06
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEZ04

Quant Time: Apr 07 00:14:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Apr 06 23:34:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	535028	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.28	117	442339	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	128035	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	148415	3.65	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.00%
7) Chloroethane-d5	2.62	69	132877	3.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.40%
11) 1,1-Dichloroethene-d2	3.60	63	307085	2.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.40%#
20) 2-Butanone-d5	6.59	46	162667	44.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.76%
24) Chloroform-d	7.20	84	318303	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
26) 1,2-Dichloroethane-d4	7.89	65	140309	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.40%
32) Benzene-d6	7.85	84	557210	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.60%
36) 1,2-Dichloropropane-d6	8.89	67	160421	4.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.60%
41) Toluene-d8	9.97	98	483009	3.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.40%
43) trans-1,3-Dichloropropene-	10.23	79	26948	2.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	55.60%
46) 2-Hexanone-d5	10.59	63	130301	50.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.08%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	61169	4.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.60%
64) 1,2-Dichlorobenzene-d4	13.51	152	97736	5.04	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.80%


Target Compounds					Ovalue
29) 1,1,1-Trichloroethane	7.43	97	14417	0.197 ug/L #	84
34) Trichloroethene	8.71	95	495982	10.711 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR040619\
Data File : VR026484.D
Acq On : 6 Apr 2019 20:20
Operator : SY/MD
Sample : K2282-06
Misc : 25mL/MSVOA R/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEZ04

Quant Time: Apr 07 00:14:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Apr 06 23:34:06 2019
Response via : Initial Calibration




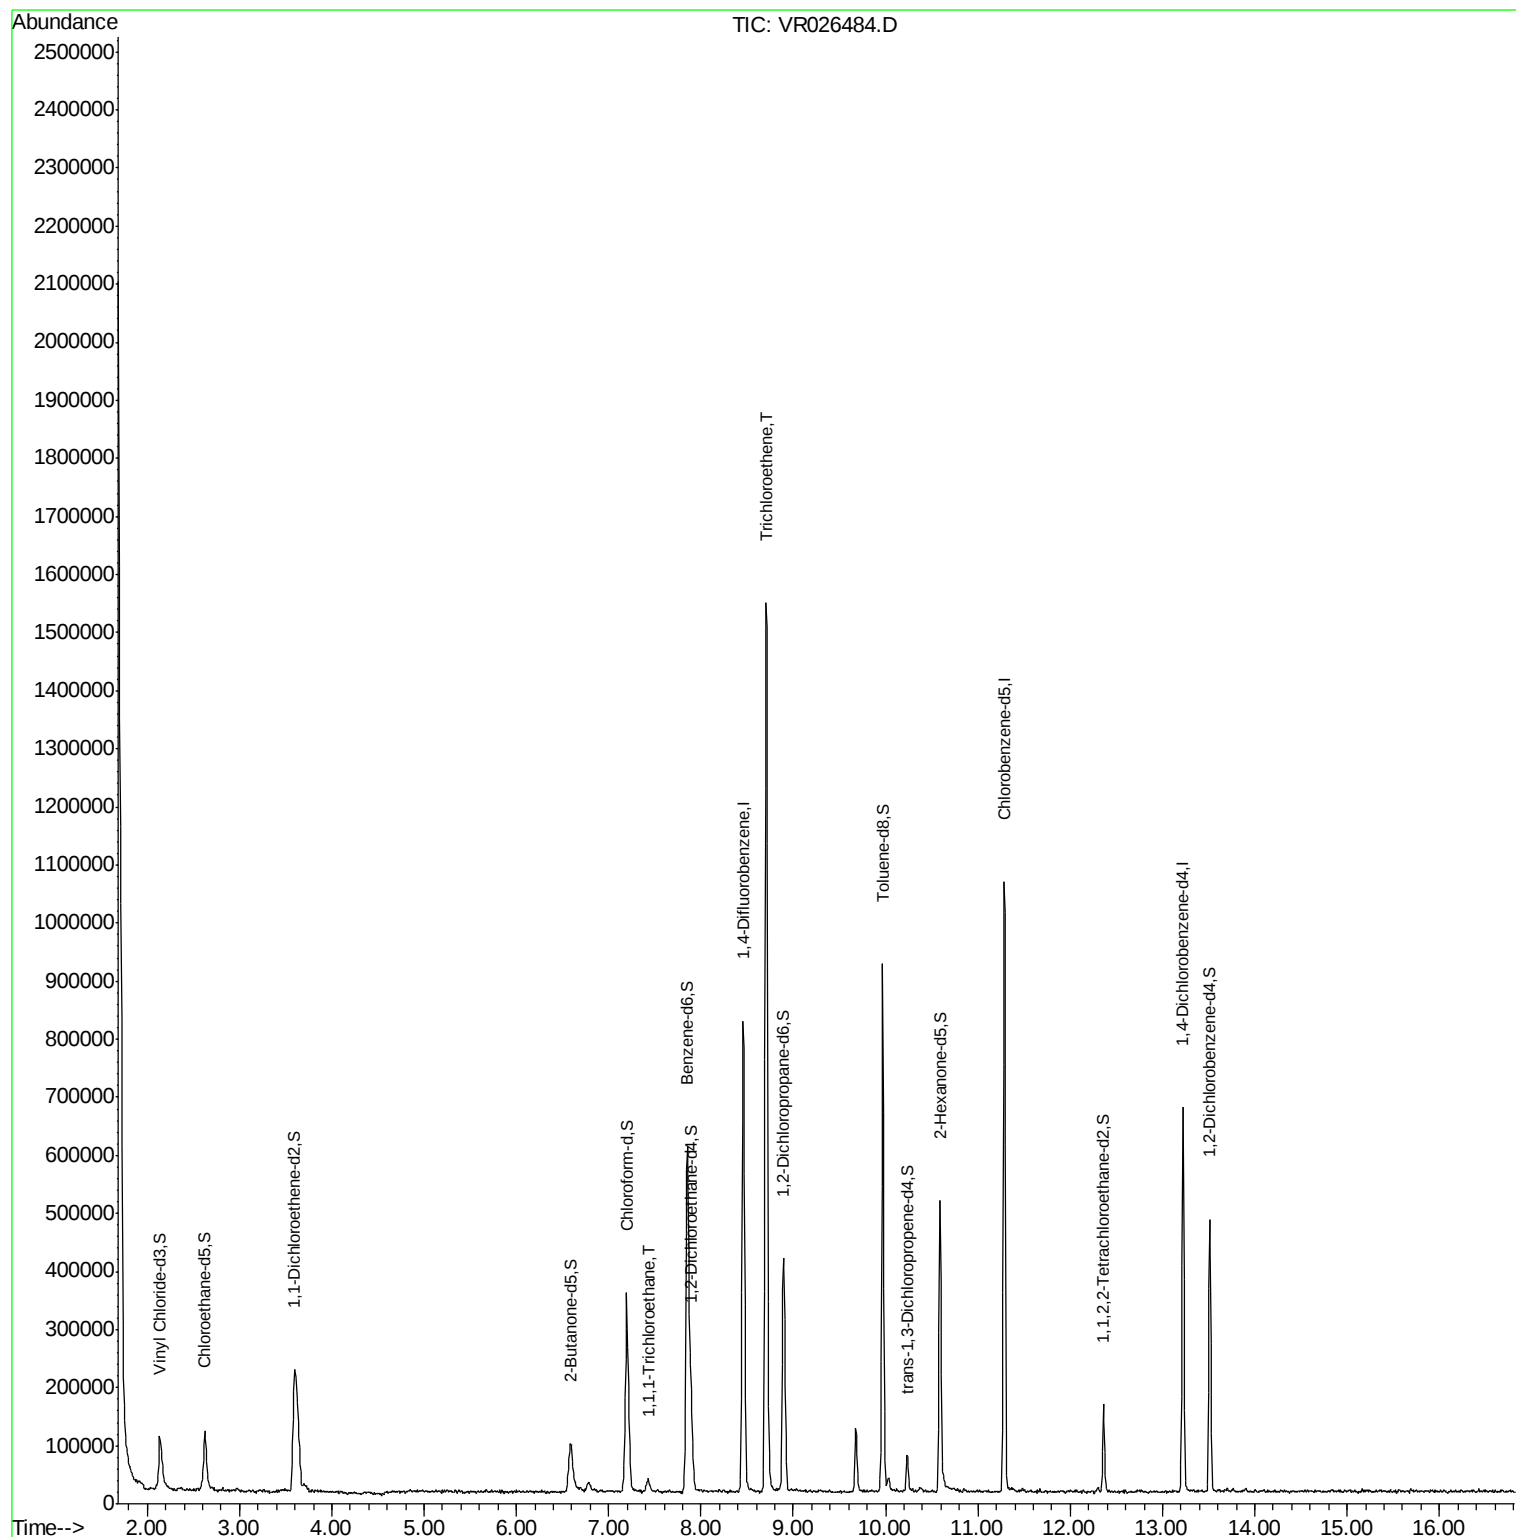


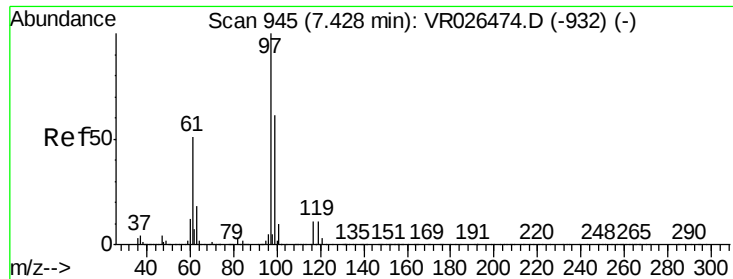

#29
1,1,1-Trichloroethane
Concen: 0.197 ug/L
RT: 7.43 min Scan# 945
Delta R.T. -0.00 min
Lab File: VR026484.D
Acq: 6 Apr 2019 20:20

Instrument :
MSVOA_R
ClientSampleId :
BEZ04

Tot Ion: 97 Resp: 14417
Ion Ratio Lower Upper
97 100
99 76.5 49.6 74.4#
61 61.3 41.8 62.6

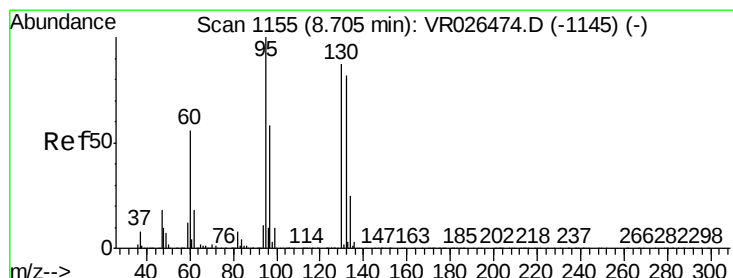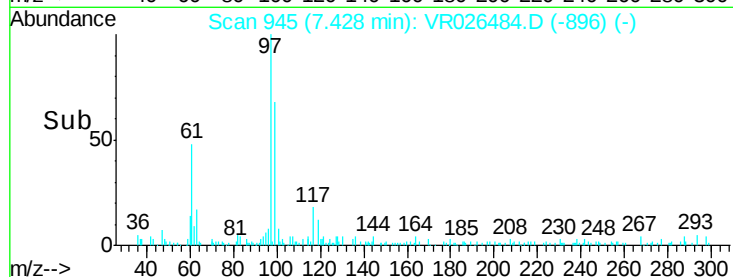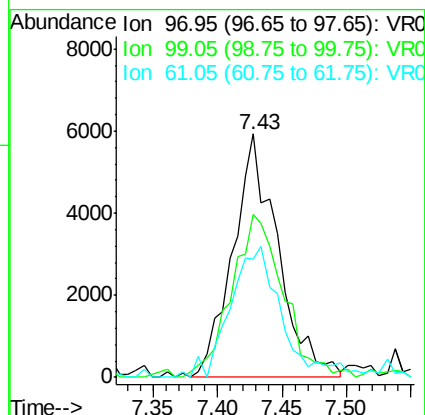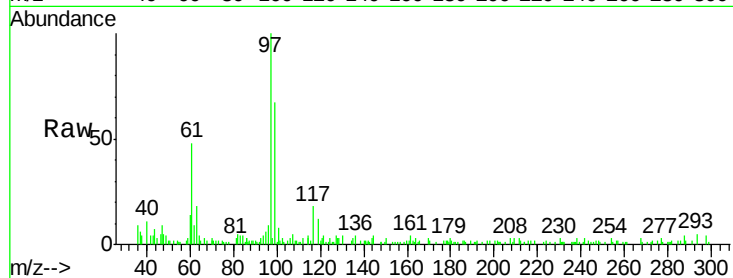

#34
Trichloroethene
Concen: 10.711 ug/L
RT: 8.71 min Scan# 1155
Delta R.T. -0.00 min
Lab File: VR026484.D
Acq: 6 Apr 2019 20:20

Tgt Ion: 95 Resp: 495982
Ion Ratio Lower Upper
95 100
97 61.2 43.8 81.3
132 83.9 57.2 106.2
130 89.8 59.7 110.9

