

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR040919\
 Data File : VR026525.D
 Acq On : 9 Apr 2019 20:22
 Operator : SY/MD
 Sample : K2285-09
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEZC7

Quant Time: Apr 10 06:58:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 05:42:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	612175	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	500316	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	148195	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	176806	3.80	ug/L	-0.02
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.00%
7) Chloroethane-d5	2.63	69	160521	4.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.80%
11) 1,1-Dichloroethene-d2	3.60	63	371225	3.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.80%
20) 2-Butanone-d5	6.59	46	172392	41.57	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.14%
24) Chloroform-d	7.20	84	359221	4.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.20%
26) 1,2-Dichloroethane-d4	7.89	65	152520	4.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.20%
32) Benzene-d6	7.85	84	646871	4.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.80%
36) 1,2-Dichloropropane-d6	8.89	67	175896	4.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.00%
41) Toluene-d8	9.97	98	580004	4.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.00%
43) trans-1,3-Dichloropropene-	10.23	79	30910	2.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	56.20%
46) 2-Hexanone-d5	10.59	63	137386	46.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.28%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	67645	4.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.80%
64) 1,2-Dichlorobenzene-d4	13.52	152	117774	5.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.00%


Target Compounds					Ovalue
14) Carbon disulfide	3.93	76	90877	0.577 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR040919\
Data File : VR026525.D
Acq On : 9 Apr 2019 20:22
Operator : SY/MD
Sample : K2285-09
Misc : 25mL/MSVOA R/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEZC7

Quant Time: Apr 10 06:58:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 05:42:05 2019
Response via : Initial Calibration

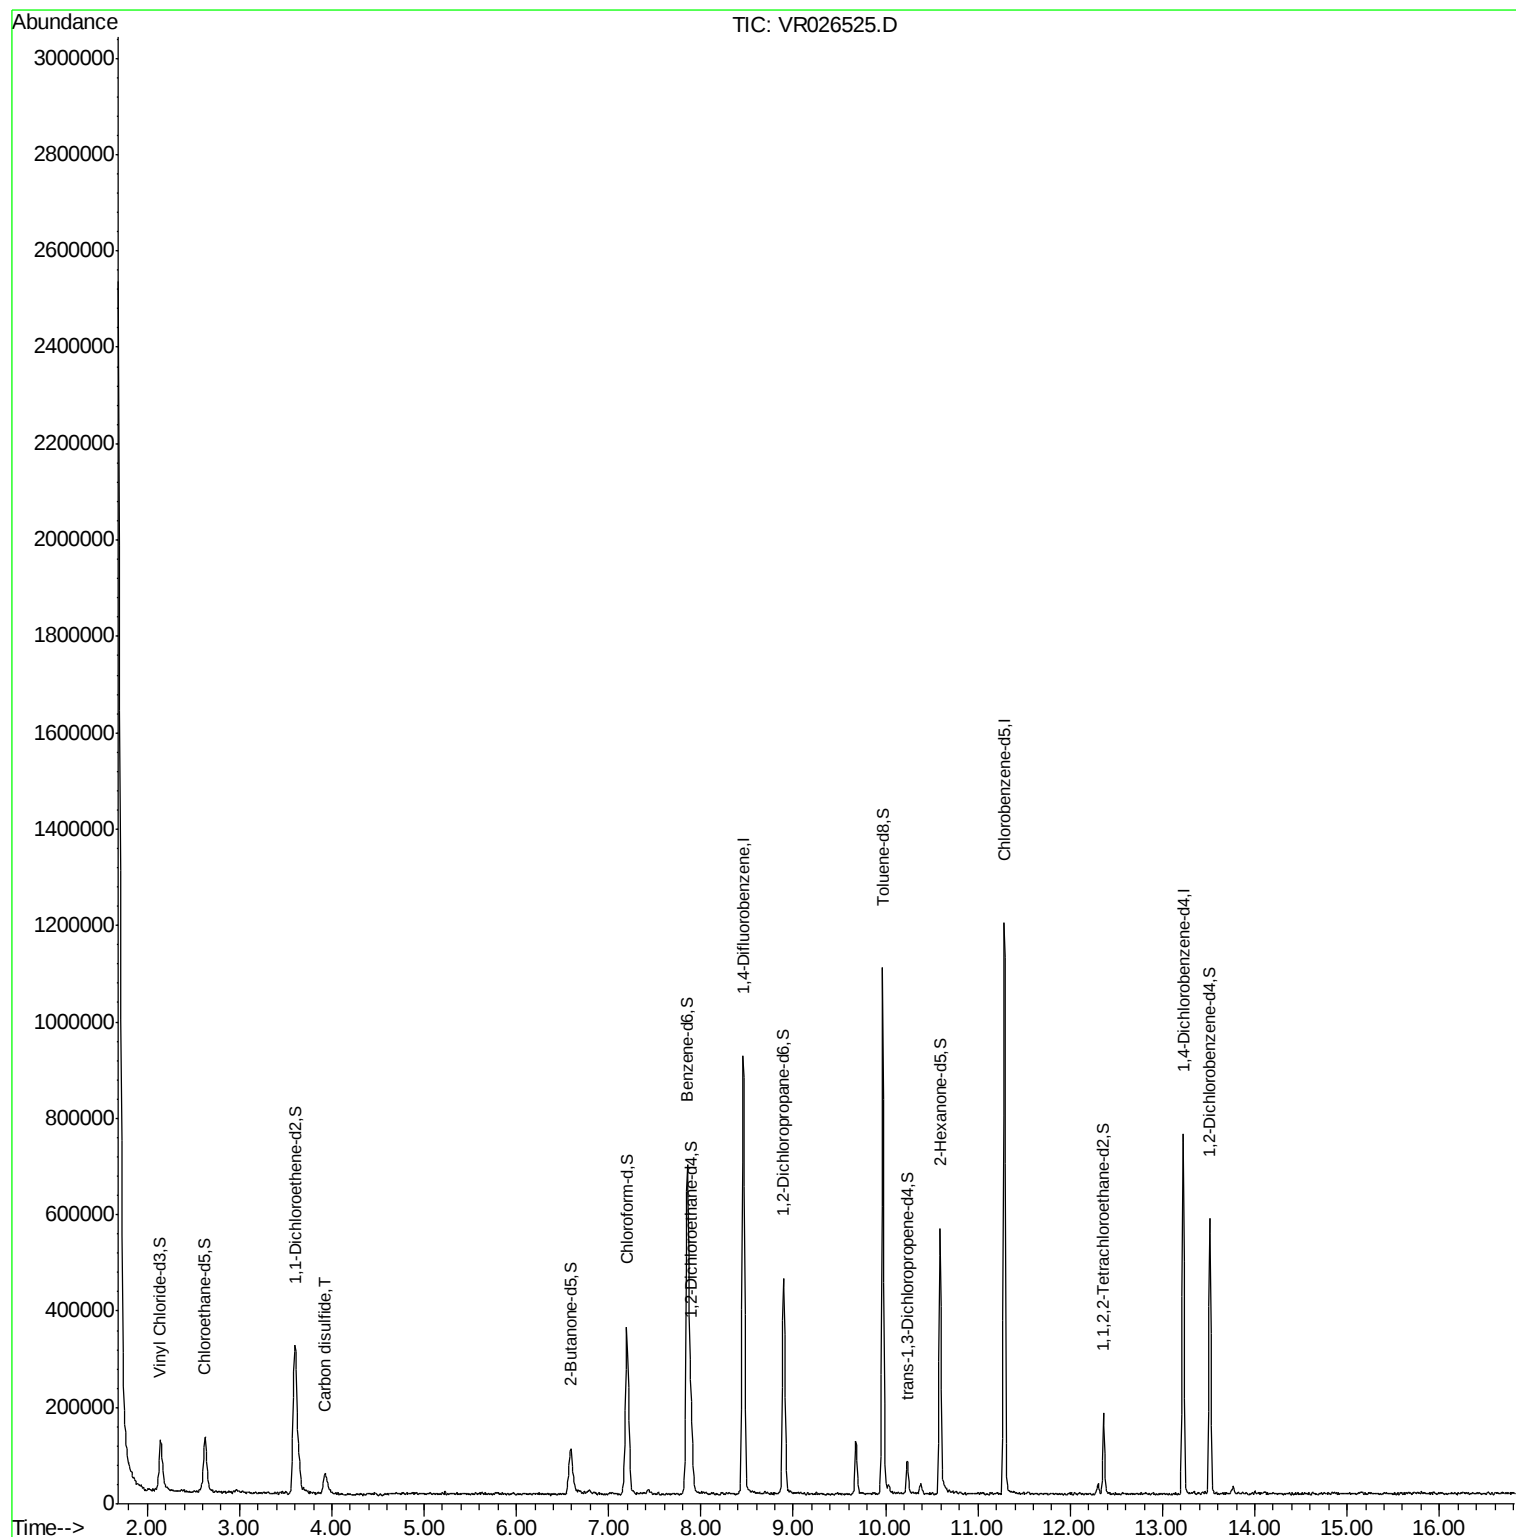

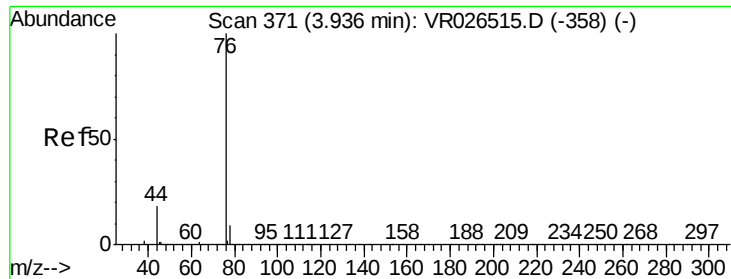

#14
 Carbon disulfide
 Concen: 0.577 ug/L
 RT: 3.93 min Scan# 370
 Delta R.T. -0.01 min
 Lab File: VR026525.D
 Acq: 9 Apr 2019 20:22

Instrument :
 MSVOA_R
 ClientSampleId :
 BEZC7

Tot Ion: 76 Resp: 90877
 Ion Ratio Lower Upper
 76 100
 78 8.6 7.7 11.5

