

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR040919\
 Data File : VR026534.D
 Acq On : 10 Apr 2019 2:14
 Operator : SY/MD
 Sample : K2285-16
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEZD4

Quant Time: Apr 10 07:44:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 07:28:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	543320	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	449657	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	125467	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	179246	4.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	2.63	69	160727	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.40%
11) 1,1-Dichloroethene-d2	3.61	63	363175	3.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.00%
20) 2-Butanone-d5	6.59	46	178364	48.46	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.92%
24) Chloroform-d	7.20	84	367415	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	7.89	65	159899	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	7.85	84	668249	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	8.89	67	172730	4.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.80%
41) Toluene-d8	9.97	98	588125	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	10.23	79	37702	3.82	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.40%
46) 2-Hexanone-d5	10.59	63	150695	56.93	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.86%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	71030	4.89	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.80%
64) 1,2-Dichlorobenzene-d4	13.52	152	119511	6.29	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	125.80%#


Target Compounds				Ovalue
13) Acetone	3.70	43	10769	2.895 ug/L 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR040919\
Data File : VR026534.D
Acq On : 10 Apr 2019 2:14
Operator : SY/MD
Sample : K2285-16
Misc : 25mL/MSVOA R/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEZD4

Quant Time: Apr 10 07:44:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 07:28:30 2019
Response via : Initial Calibration

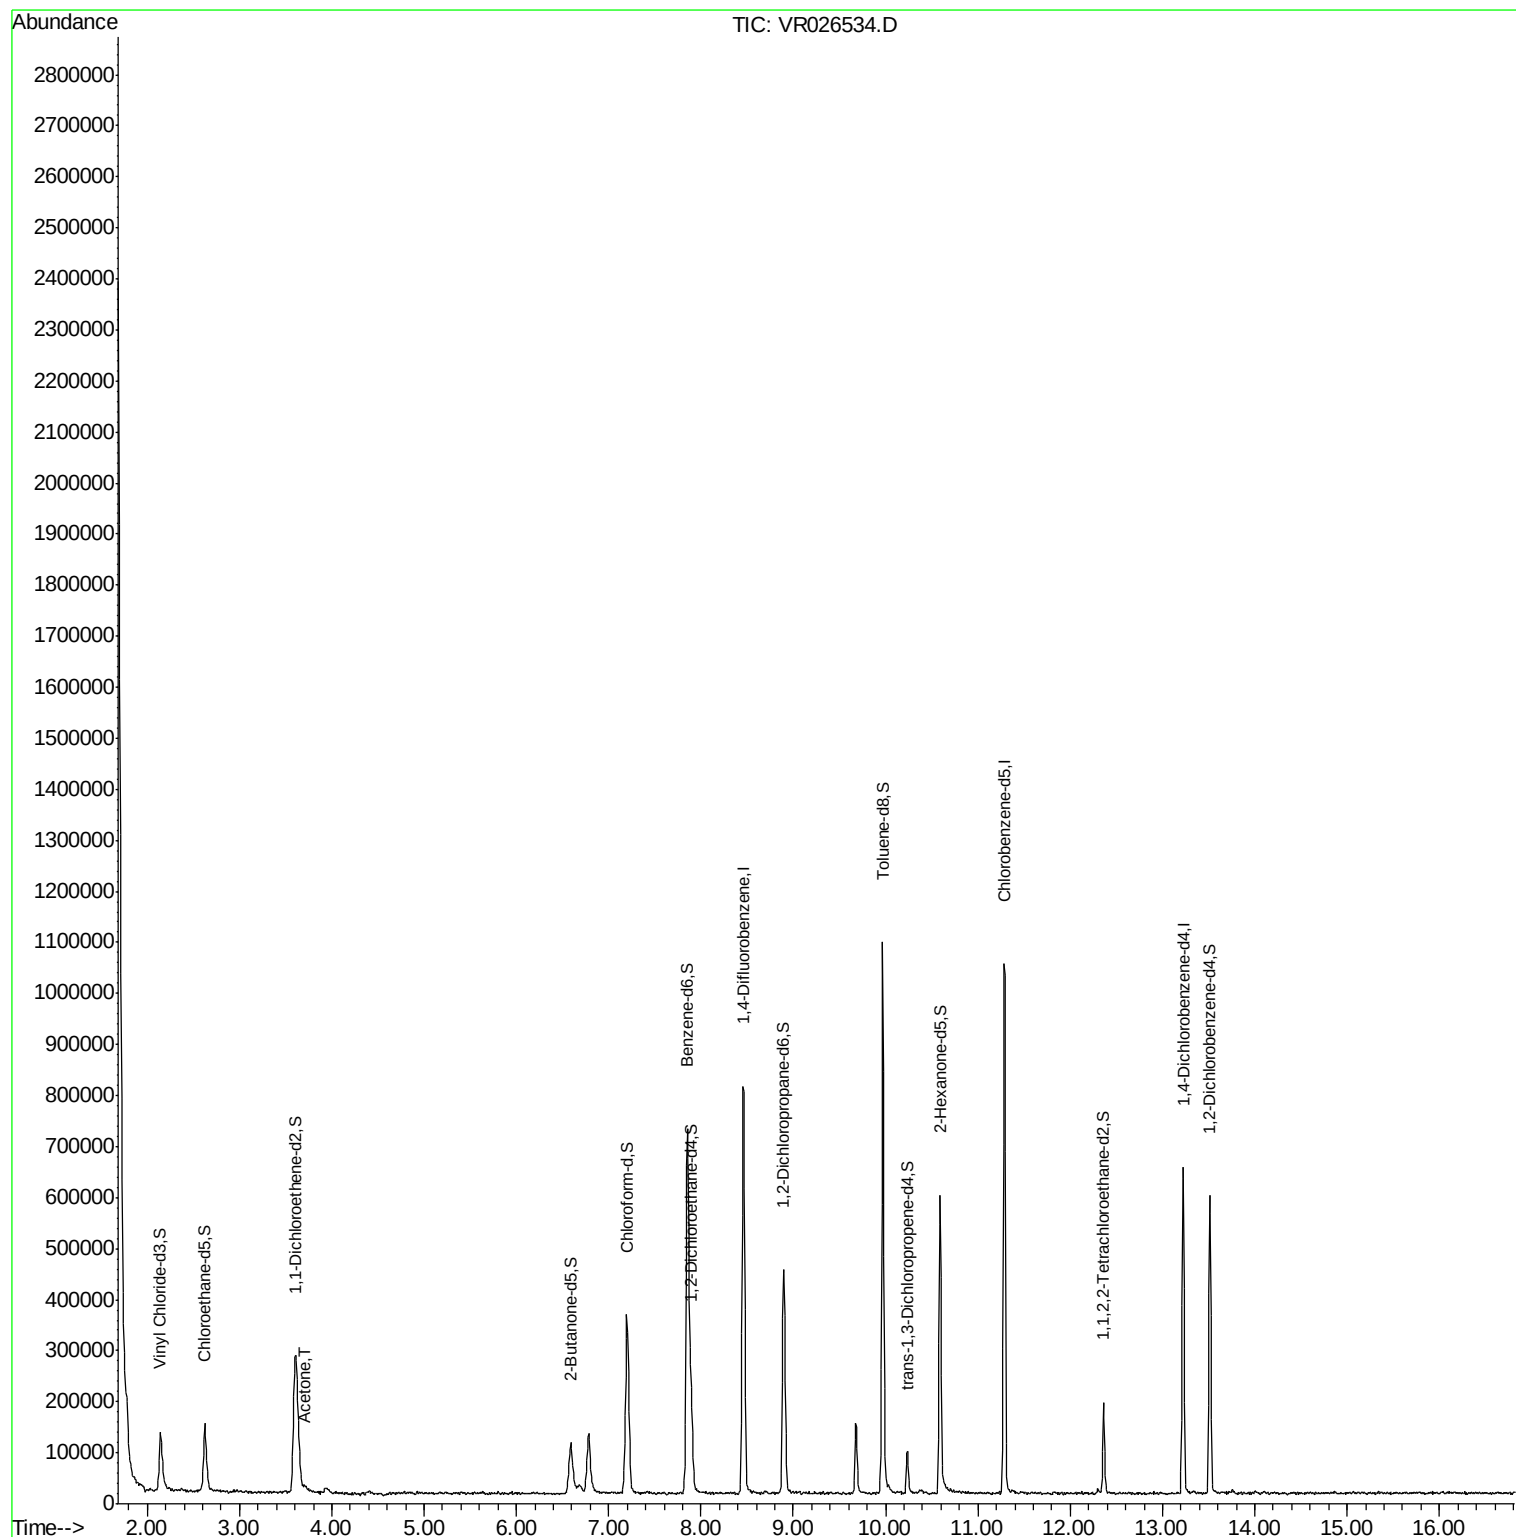

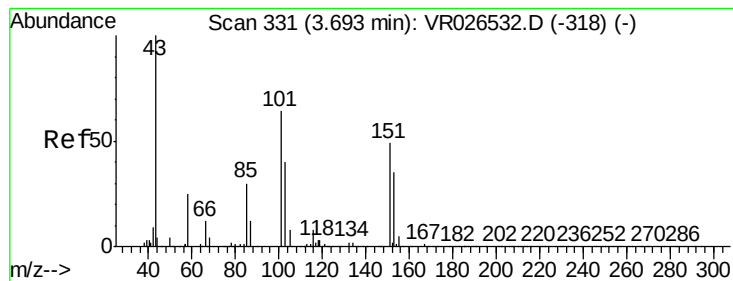

#13

Acetone

Concen: 2.895 ug/L

RT: 3.70 min Scan# 332

Delta R.T. 0.01 min

Lab File: VR026534.D

Acq: 10 Apr 2019 2:14

Instrument :
MSVOA_R
ClientSampleId :
BEZD4

Tot Ion: 43 Resp: 10769

Ion Ratio Lower Upper

43 100

58 32.8 0.0 53.8

