

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR040919\
 Data File : VR026537.D
 Acq On : 10 Apr 2019 3:50
 Operator : SY/MD
 Sample : K2285-19
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEZD7

Quant Time: Apr 10 08:00:44 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 07:28:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	474207	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	401725	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.23	152	119237	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	174434	4.84	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.80%
7) Chloroethane-d5	2.63	69	153554	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.20%
11) 1,1-Dichloroethene-d2	3.61	63	343816	3.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.80%
20) 2-Butanone-d5	6.59	46	174414	54.30	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.60%
24) Chloroform-d	7.20	84	354438	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
26) 1,2-Dichloroethane-d4	7.90	65	152478	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.00%
32) Benzene-d6	7.85	84	636264	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	8.90	67	173209	5.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.20%
41) Toluene-d8	9.97	98	571522	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
43) trans-1,3-Dichloropropene-	10.23	79	34774	3.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.80%
46) 2-Hexanone-d5	10.59	63	148195	62.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	125.32%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	71617	5.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.40%
64) 1,2-Dichlorobenzene-d4	13.52	152	122692	6.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	136.00%#


Target Compounds				Ovalue
13) Acetone	3.70	43	10240	3.154 ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR040919\
Data File : VR026537.D
Acq On : 10 Apr 2019 3:50
Operator : SY/MD
Sample : K2285-19
Misc : 25mL/MSVOA R/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEZD7

Quant Time: Apr 10 08:00:44 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR040319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 07:28:30 2019
Response via : Initial Calibration

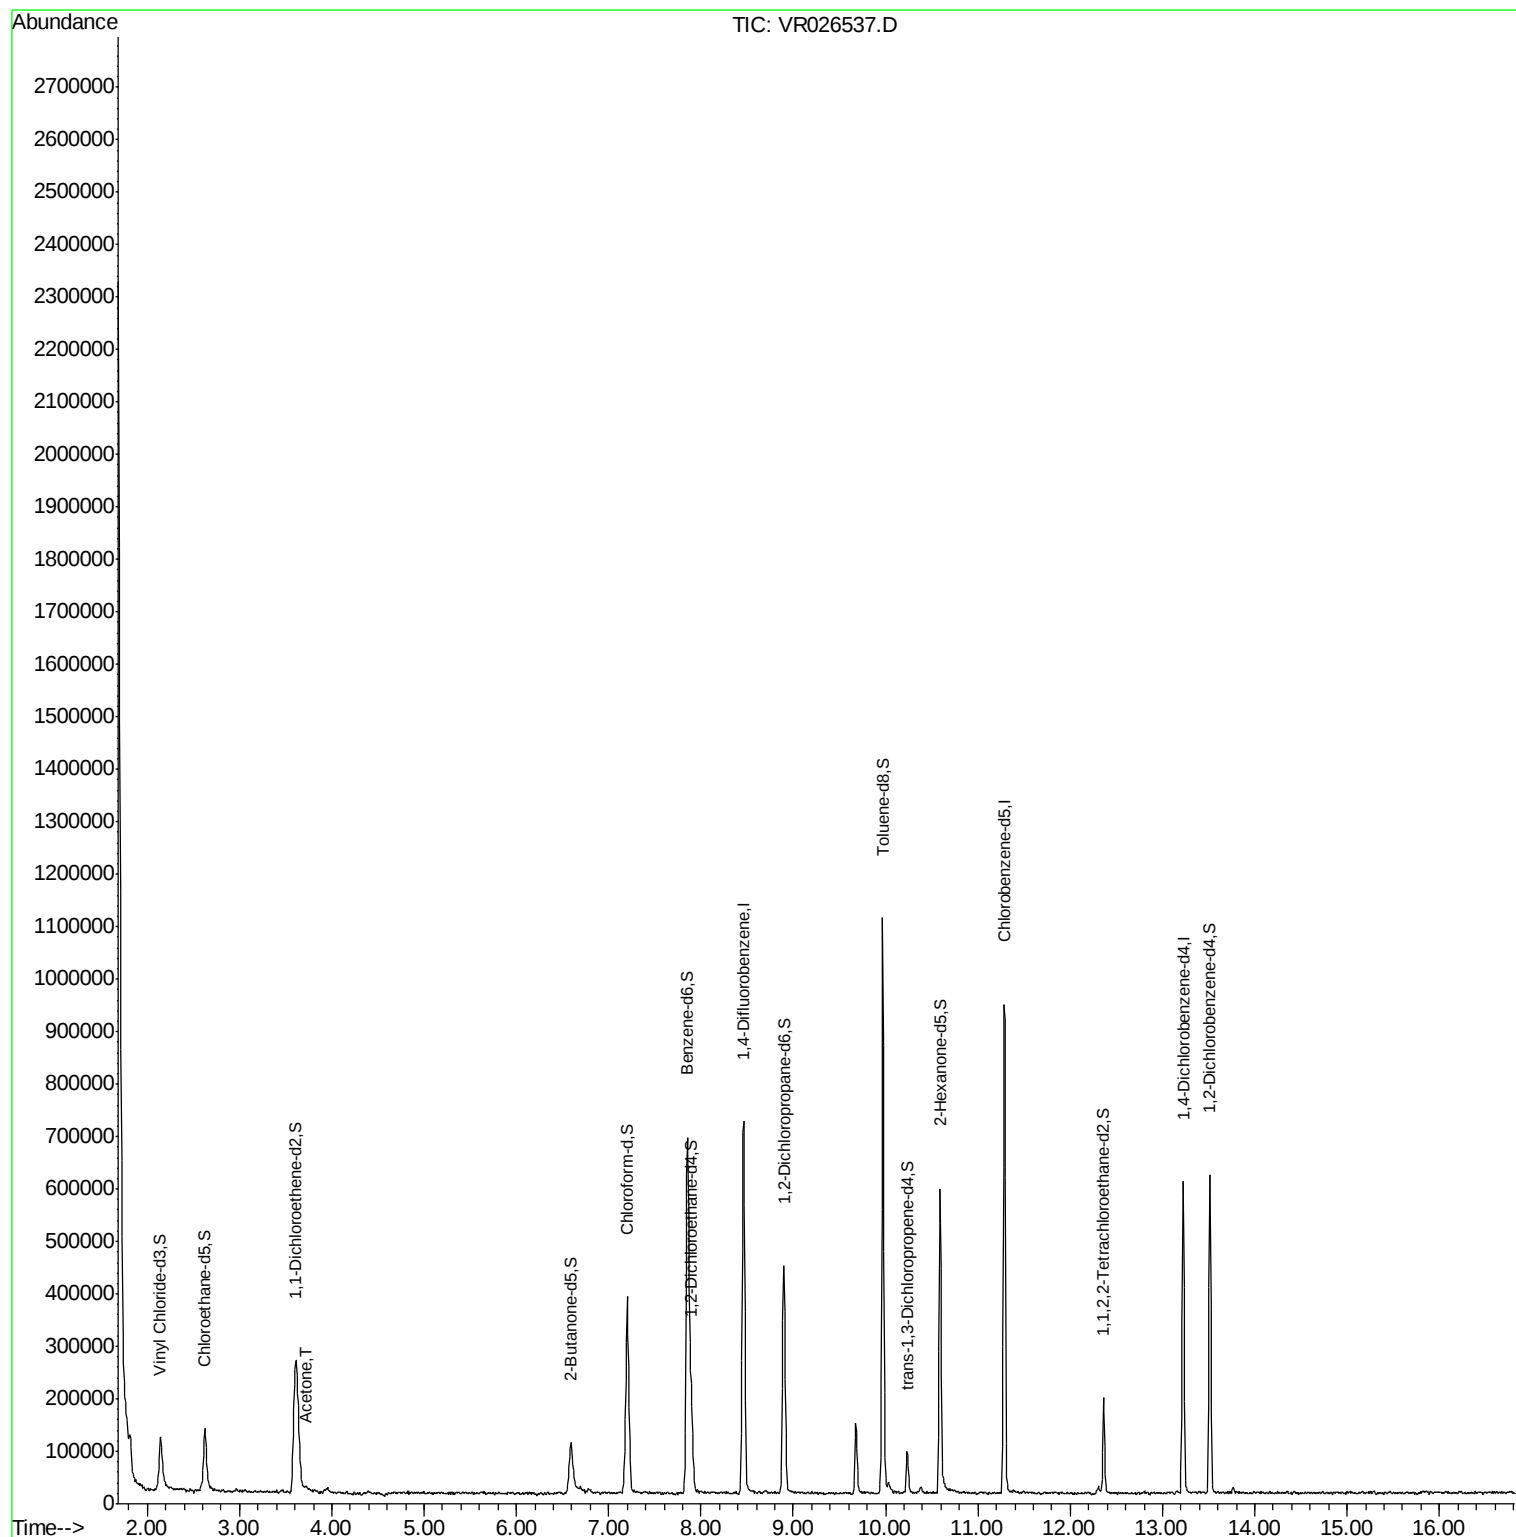

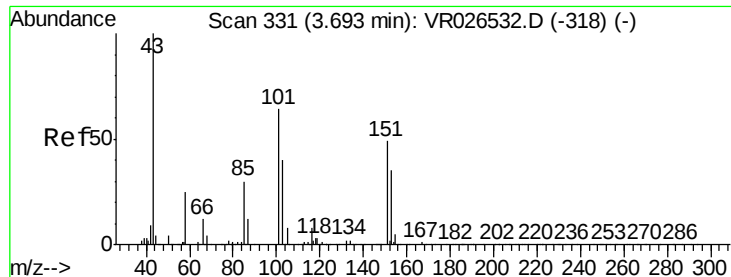

#13

Acetone

Concen: 3.154 ug/L

RT: 3.70 min Scan# 333

Delta R.T. 0.01 min

Lab File: VR026537.D

Acq: 10 Apr 2019 3:50

Instrument :
MSVOA_R
ClientSampleId :
BEZD7

Tot Ion: 43 Resp: 10240

Ion Ratio Lower Upper

43 100

58 27.5 0.0 53.8

