

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR041119\
 Data File : VR026582.D
 Acq On : 11 Apr 2019 22:56
 Operator : SY/MD
 Sample : K2297-03
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 E3YC4

Quant Time: Apr 12 02:47:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR041119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 12 02:06:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	527952	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	438444	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	145000	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	183412	4.63	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.60%
7) Chloroethane-d5	2.62	69	166156	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	3.60	63	370555	3.34	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.80%
20) 2-Butanone-d5	6.59	46	180478	47.94	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.88%
24) Chloroform-d	7.20	84	354294	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.80%
26) 1,2-Dichloroethane-d4	7.90	65	155165	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.40%
32) Benzene-d6	7.85	84	634377	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
36) 1,2-Dichloropropane-d6	8.89	67	169282	4.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.80%
41) Toluene-d8	9.97	98	572503	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.00%
43) trans-1,3-Dichloropropene-	10.23	79	33592	3.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.00%
46) 2-Hexanone-d5	10.59	63	140006	48.85	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.70%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	67709	4.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	119405	5.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.40%


Target Compounds					Ovalue
13) Acetone	3.69	43	20578	5.300 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR041119\
Data File : VR026582.D
Acq On : 11 Apr 2019 22:56
Operator : SY/MD
Sample : K2297-03
Misc : 25mL/MSVOA R/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
E3YC4

Quant Time: Apr 12 02:47:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR041119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 12 02:06:27 2019
Response via : Initial Calibration

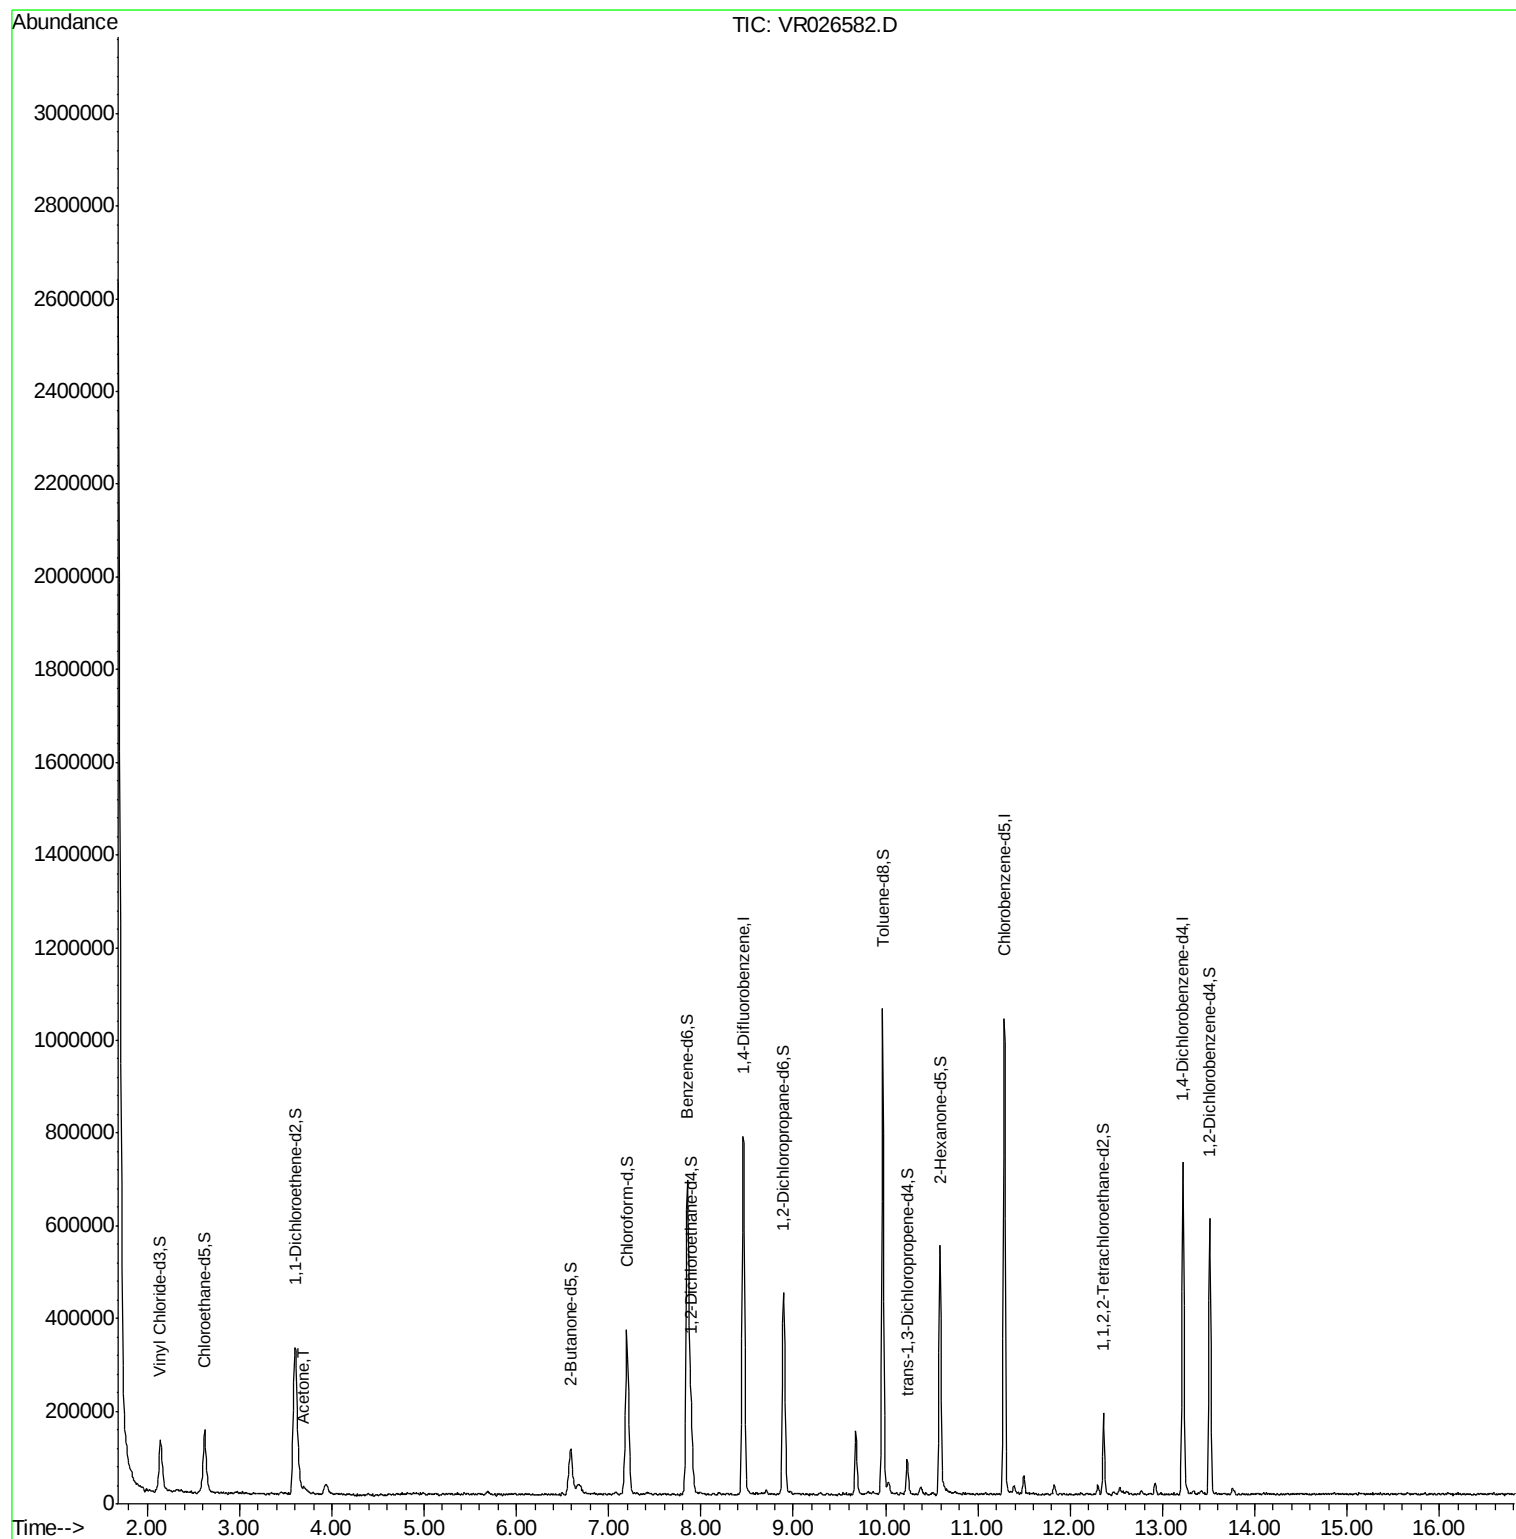

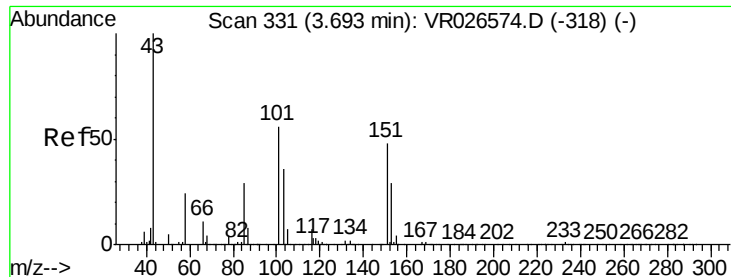

#13

Acetone

Concen: 5.300 ug/L

RT: 3.69 min Scan# 331

Delta R.T. 0.00 min

Lab File: VR026582.D

Acq: 11 Apr 2019 22:56

Instrument :
MSVOA_R
ClientSampleId :
E3YC4

Tot Ion: 43 Resp: 20578

Ion Ratio Lower Upper

43 100

58 27.3 0.0 49.4

