

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR061618\
 Data File : VR025335.D
 Acq On : 16 Jun 2018 21:21
 Operator : SY/MD
 Sample : J3550-05
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 ESWF7

Quant Time: Jun 18 03:42:19 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 02:40:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	498881	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	414385	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	123713	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	46705	2.75	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.00%
7) Chloroethane-d5	2.63	69	38232	3.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	61.20%#
11) 1,1-Dichloroethene-d2	3.63	63	80726	1.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	37.00%#
20) 2-Butanone-d5	6.59	46	116248	25.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	51.04%
24) Chloroform-d	7.20	84	159430	2.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	50.20%#
26) 1,2-Dichloroethane-d4	7.89	65	67436	2.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	55.60%#
32) Benzene-d6	7.86	84	322307	2.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	45.80%#
36) 1,2-Dichloropropane-d6	8.90	67	103129	2.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	51.60%#
41) Toluene-d8	9.97	98	250768	2.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	40.40%#
43) trans-1,3-Dichloropropene-	10.24	79	14247	1.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	26.80%#
46) 2-Hexanone-d5	10.59	63	92733	25.15	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	50.30%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	43238	2.78	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	55.60%#
64) 1,2-Dichlorobenzene-d4	13.51	152	58935	2.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	56.20%#


Target Compounds				Ovalue
13) Acetone	3.70	43	15641	7.604 ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR061618\
Data File : VR025335.D
Acq On : 16 Jun 2018 21:21
Operator : SY/MD
Sample : J3550-05
Misc : 25mL/MSVOA R/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
ESWF7

Quant Time: Jun 18 03:42:19 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 02:40:54 2018
Response via : Initial Calibration

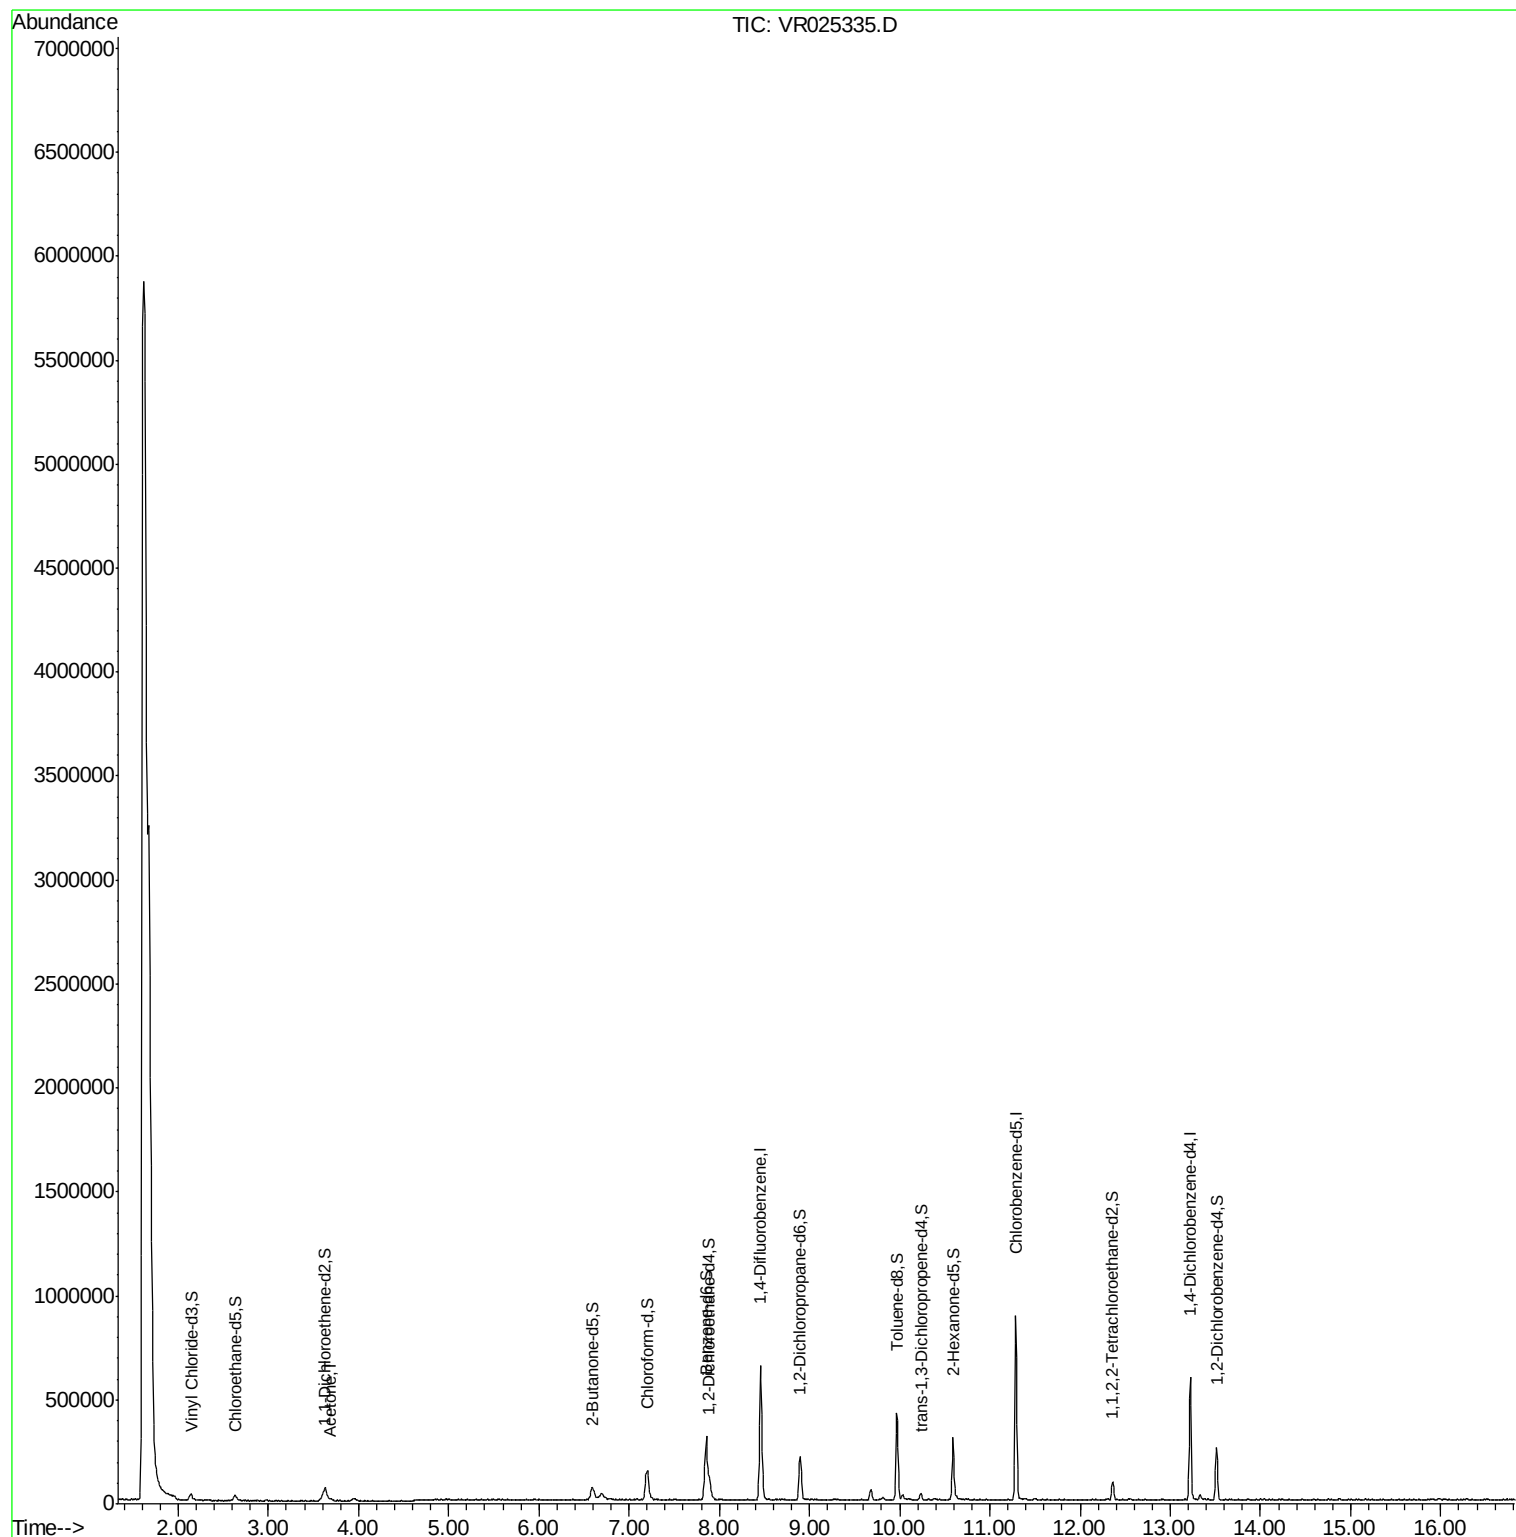

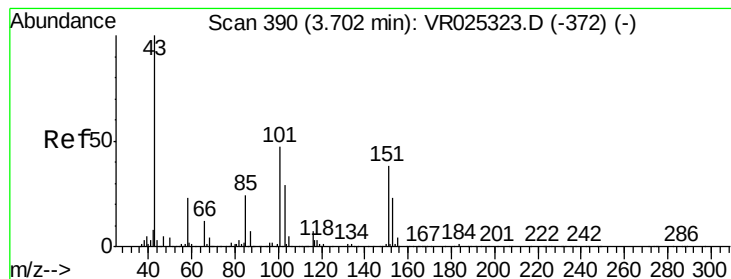

#13
 Acetone
 Concen: 7.604 ug/L
 RT: 3.70 min Scan# 389
 Delta R.T. -0.01 min
 Lab File: VR025335.D
 Acq: 16 Jun 2018 21:21

Instrument :
 MSVOA_R
 ClientSampleId :
 ESWF7

Tot Ion: 43 Resp: 15641
 Ion Ratio Lower Upper
 43 100
 58 24.3 0.0 41.6

