

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR061618\
 Data File : VR025348.D
 Acq On : 17 Jun 2018 6:07
 Operator : SY/MD
 Sample : J3513-08
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 COKE4

Quant Time: Jun 18 04:56:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 18 04:02:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	558172	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	468283	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	140661	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	73697	3.87	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.40%
7) Chloroethane-d5	2.64	69	60459	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.60%
11) 1,1-Dichloroethene-d2	3.63	63	137595	2.81	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.20%#
20) 2-Butanone-d5	6.59	46	265598	52.12	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.24%
24) Chloroform-d	7.20	84	286386	4.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.60%
26) 1,2-Dichloroethane-d4	7.89	65	117782	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.60%
32) Benzene-d6	7.86	84	586322	3.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.80%
36) 1,2-Dichloropropane-d6	8.90	67	192718	4.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.40%
41) Toluene-d8	9.97	98	467788	3.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.60%#
43) trans-1,3-Dichloropropene-	10.23	79	23743	1.98	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	39.60%#
46) 2-Hexanone-d5	10.59	63	209375	50.25	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.50%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	84758	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	13.51	152	107182	4.49	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.80%


Target Compounds					Ovalue
13) Acetone	3.70	43	9434	4.099 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR061618\
Data File : VR025348.D
Acq On : 17 Jun 2018 6:07
Operator : SY/MD
Sample : J3513-08
Misc : 25mL/MSVOA R/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0KE4

Quant Time: Jun 18 04:56:15 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 18 04:02:12 2018
Response via : Initial Calibration

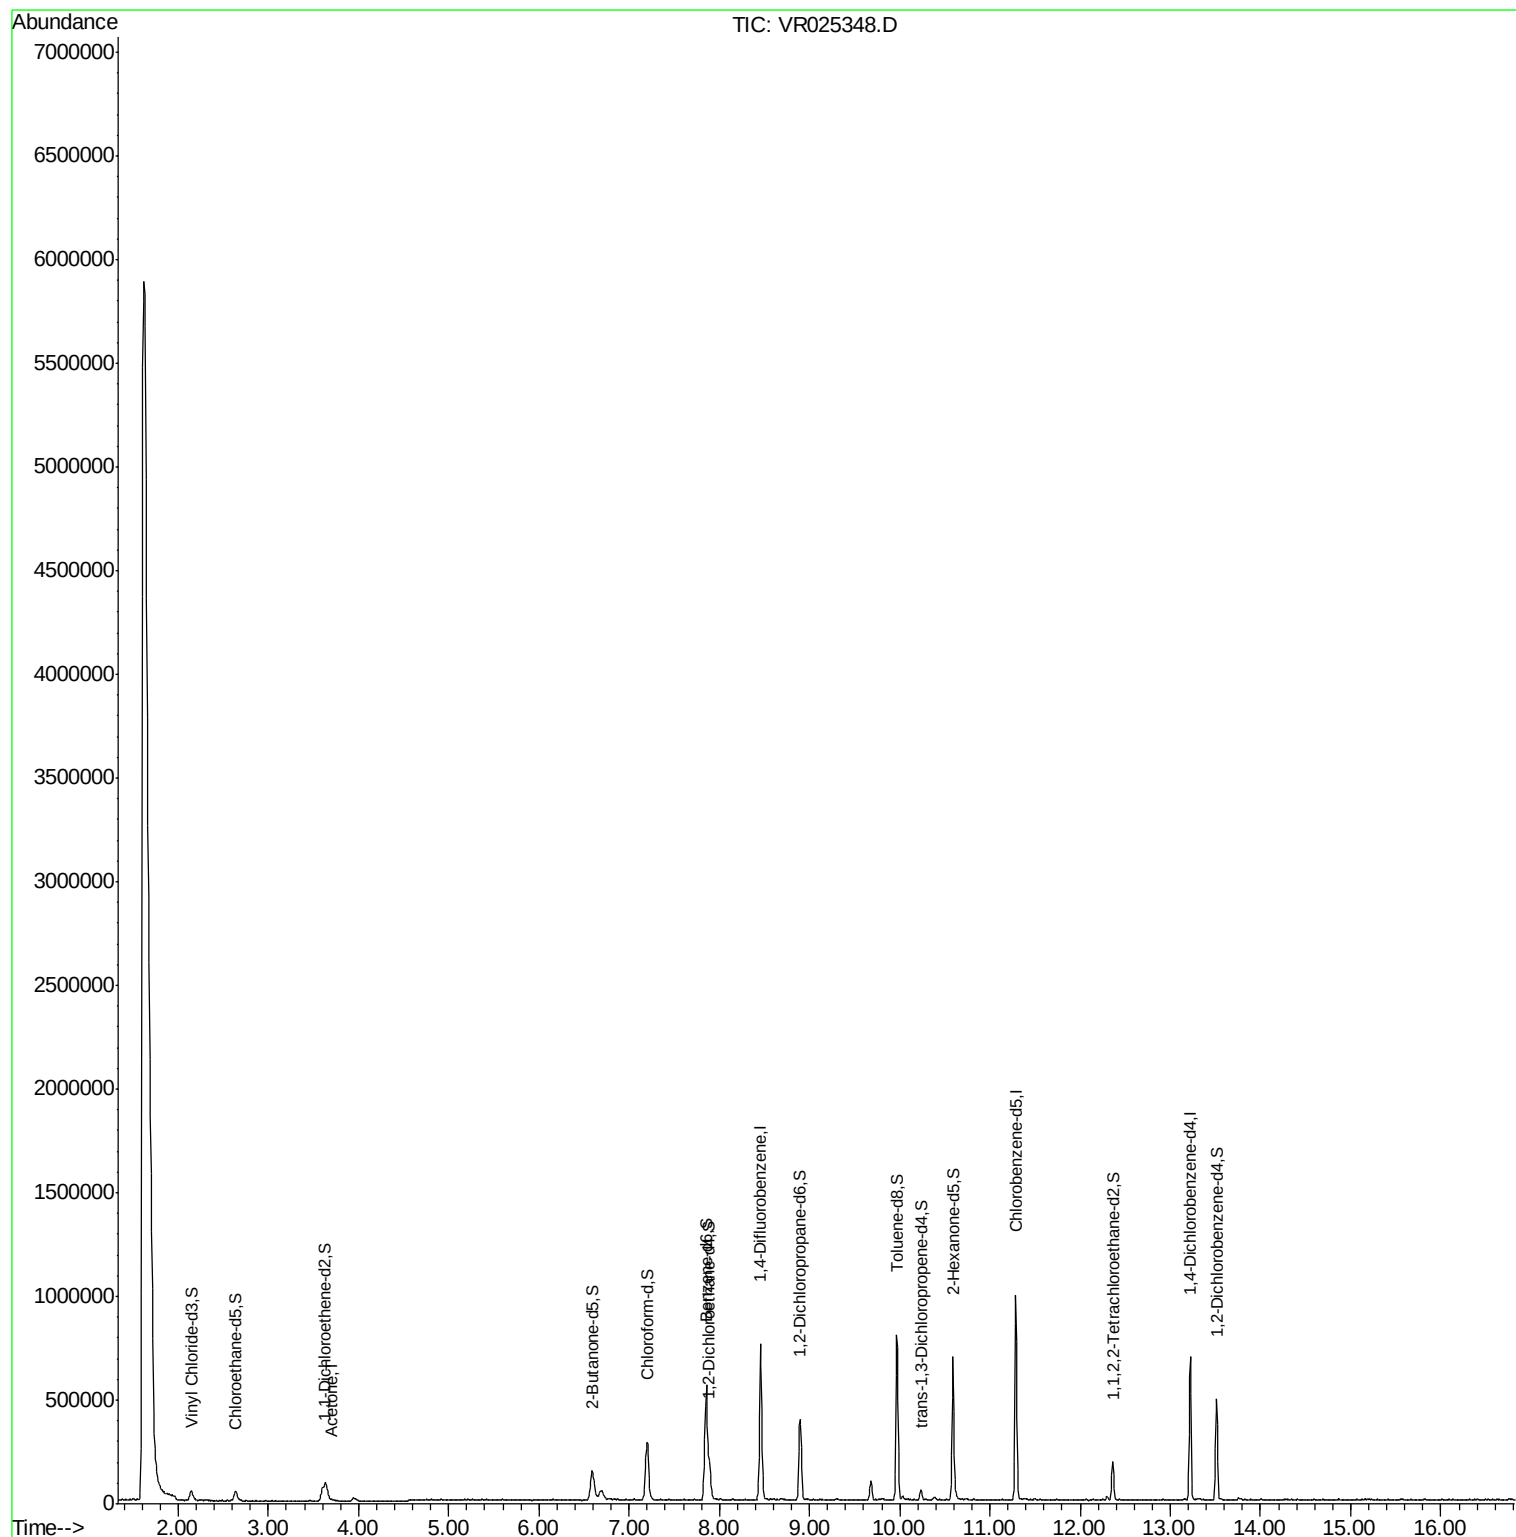

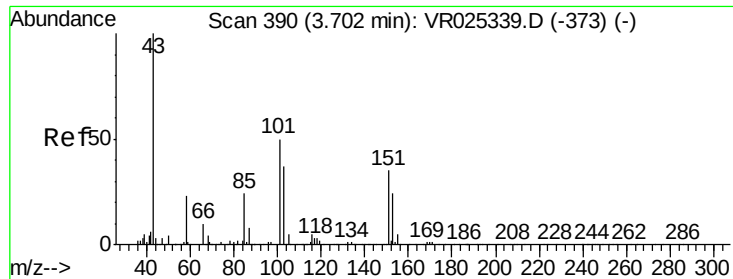

#13

Acetone

Concen: 4.099 ug/L

RT: 3.70 min Scan# 390

Delta R.T. -0.00 min

Lab File: VR025348.D

Acq: 17 Jun 2018 6:07

Instrument :

MSVOA_R

ClientSampleId :

COKE4

Tot Ion: 43 Resp: 9434

Ion Ratio Lower Upper

43 100

58 17.1 0.0 41.6

