

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR061918\
 Data File : VR025369.D
 Acq On : 19 Jun 2018 17:01
 Operator : SY/MD
 Sample : J3553-13
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0KK1

Quant Time: Jun 20 02:14:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 20 01:37:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	564565	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	485001	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	156472	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	74596	3.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.60%
7) Chloroethane-d5	2.64	69	57539	4.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.40%
11) 1,1-Dichloroethene-d2	3.65	63	161685	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	6.60	46	314091	60.94	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.88%
24) Chloroform-d	7.20	84	376300	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
26) 1,2-Dichloroethane-d4	7.90	65	157214	5.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.40%
32) Benzene-d6	7.86	84	814198	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	8.90	67	247242	5.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.80%
41) Toluene-d8	9.97	98	716206	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
43) trans-1,3-Dichloropropene-	10.24	79	46599	3.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.00%
46) 2-Hexanone-d5	10.59	63	267487	61.98	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.96%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	107975	5.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	118.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	159684	6.02	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	120.40%#


Target Compounds					Ovalue
13) Acetone	3.71	43	10154	4.36 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR061918\
Data File : VR025369.D
Acq On : 19 Jun 2018 17:01
Operator : SY/MD
Sample : J3553-13
Misc : 25mL/MSVOA R/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0KK1

Quant Time: Jun 20 02:14:00 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 20 01:37:06 2018
Response via : Initial Calibration

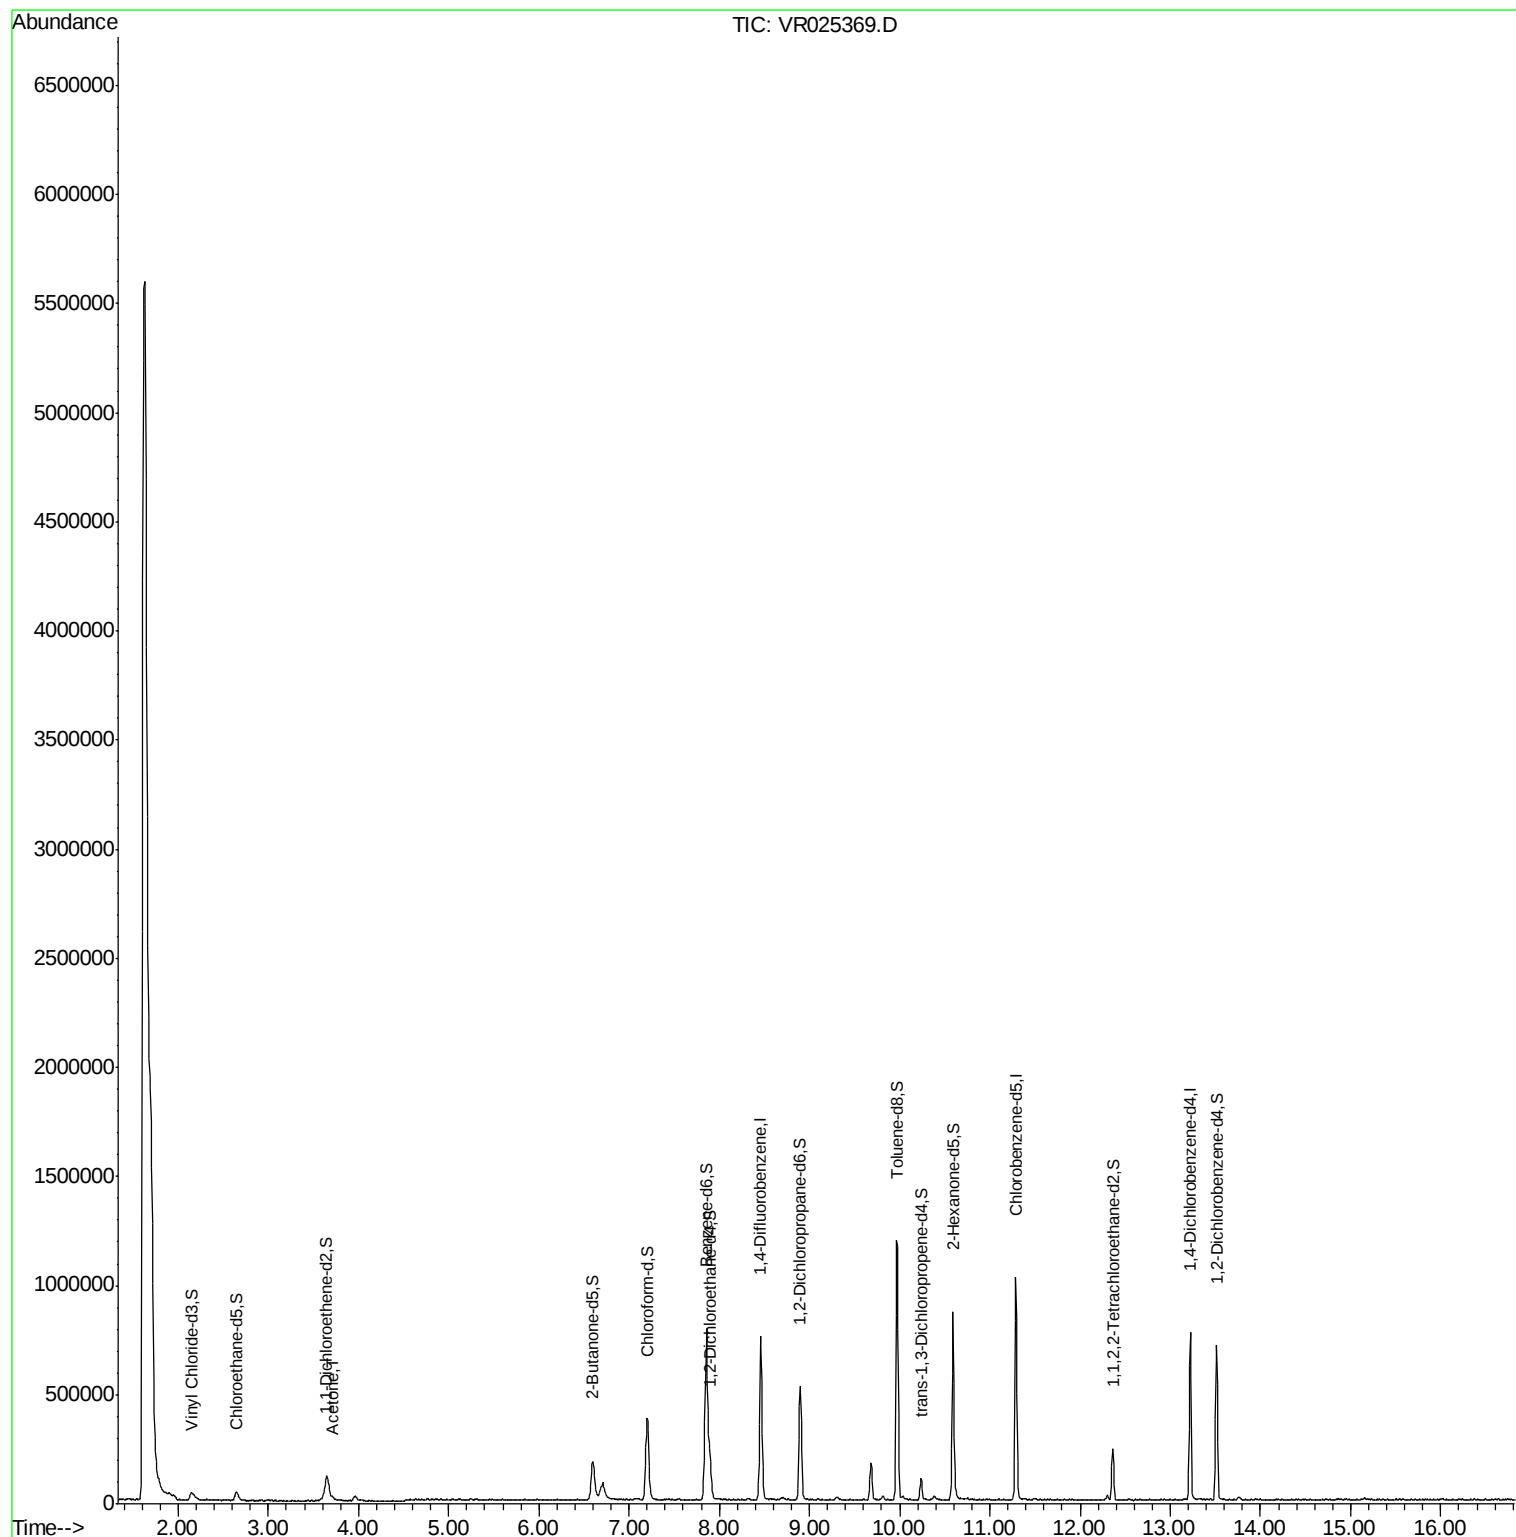

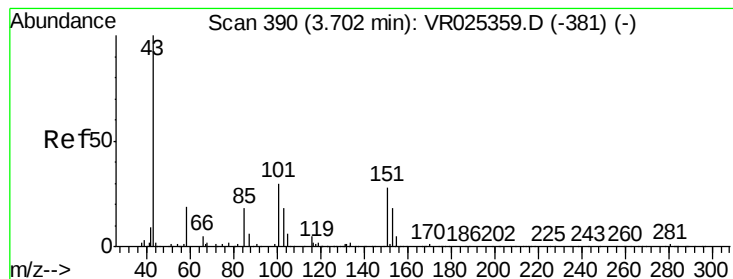

#13

Acetone

Concen: 4.36 ug/L

RT: 3.71 min Scan# 392

Delta R.T. 0.01 min

Lab File: VR025369.D

Acq: 19 Jun 2018 17:01

Instrument :
MSVOA_R
ClientSampleId :
C0KK1

Tot Ion: 43 Resp: 10154

Ion Ratio Lower Upper

43 100

58 18.9 0.0 41.6

