

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR061918\
 Data File : VR025372.D
 Acq On : 19 Jun 2018 18:40
 Operator : SY/MD
 Sample : J3553-17
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0KK5

Quant Time: Jun 20 02:18:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 20 01:37:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	496567	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	434031	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	149226	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	77442	4.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.60%
7) Chloroethane-d5	2.65	69	60261	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.00%
11) 1,1-Dichloroethene-d2	3.64	63	153999	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	6.60	46	282685	62.35	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.70%
24) Chloroform-d	7.20	84	334849	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.00%
26) 1,2-Dichloroethane-d4	7.90	65	138480	5.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.60%
32) Benzene-d6	7.86	84	703637	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	8.90	67	218769	5.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.60%
41) Toluene-d8	9.97	98	613473	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
43) trans-1,3-Dichloropropene-	10.24	79	37185	3.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.80%
46) 2-Hexanone-d5	10.59	63	238020	61.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.26%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	100212	6.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	123.20%#
64) 1,2-Dichlorobenzene-d4	13.51	152	150089	5.93	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.60%


Target Compounds					Ovalue
13) Acetone	3.71	43	13844	6.76 ug/L	97
34) Trichloroethene	8.71	95	9638	0.23 ug/L #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR061918\
Data File : VR025372.D
Acq On : 19 Jun 2018 18:40
Operator : SY/MD
Sample : J3553-17
Misc : 25mL/MSVOA R/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0KK5

Quant Time: Jun 20 02:18:17 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 20 01:37:06 2018
Response via : Initial Calibration

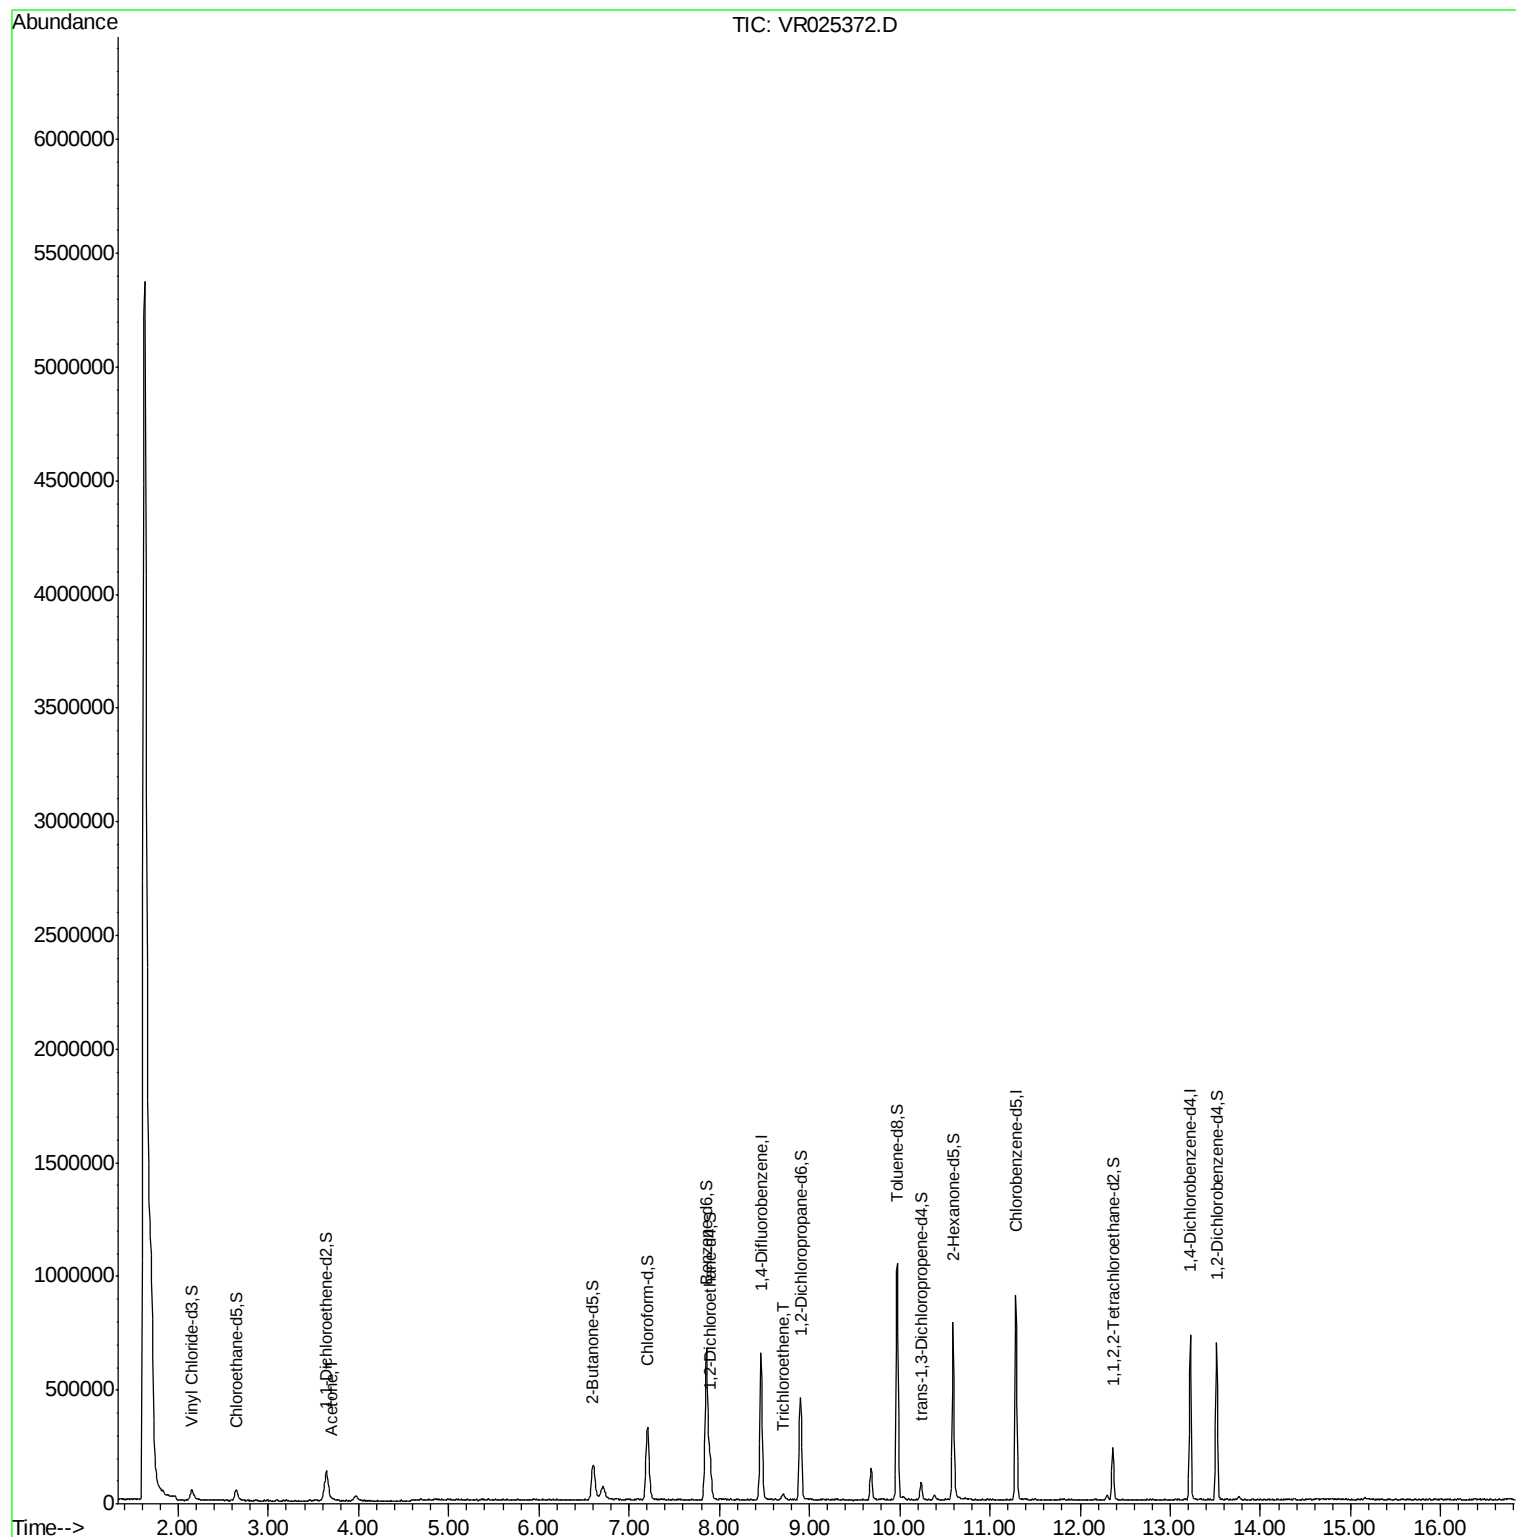

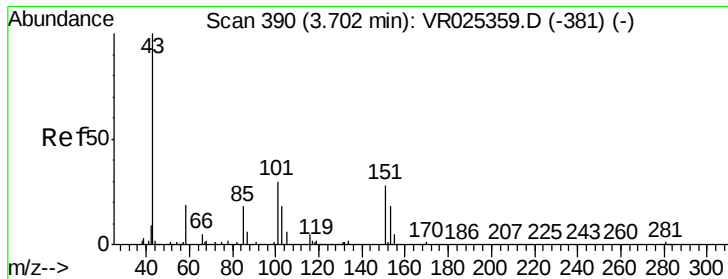

#13

Acetone

Concen: 6.76 ug/L

RT: 3.71 min Scan# 391

Delta R.T. 0.01 min

Lab File: VR025372.D

Acq: 19 Jun 2018 18:40

Instrument :

MSVOA_R

ClientSampled :


C0KK5

Tot Ion: 43 Resp: 13844

Ion Ratio Lower Upper




43 100

58 22.3 0.0 41.6

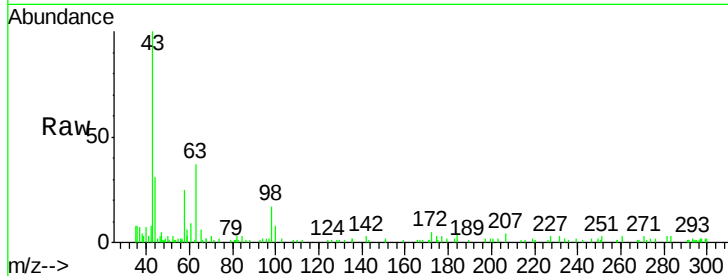

Abundance Ion 43.05 (42.75 to 43.75): VR0

Ion 58.05 (57.75 to 58.75): VR0

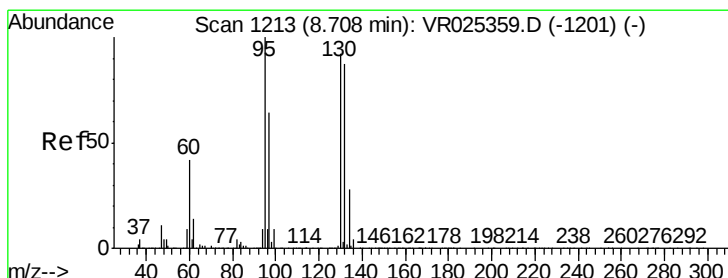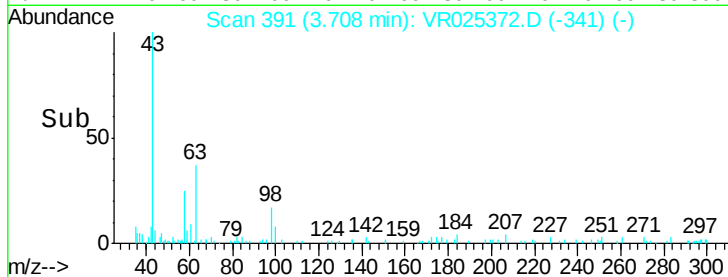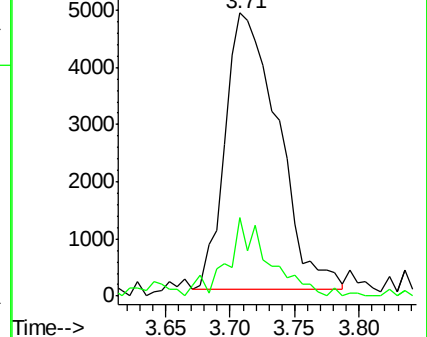

#34

Trichloroethene

Concen: 0.23 ug/L

RT: 8.71 min Scan# 1214

Delta R.T. 0.01 min

Lab File: VR025372.D

Acq: 19 Jun 2018 18:40

Tgt Ion: 95 Resp: 9638


Ion Ratio Lower Upper

95 100

97 65.1 45.6 84.6

132 117.2 60.9 113.1#

130 101.4 62.0 115.2

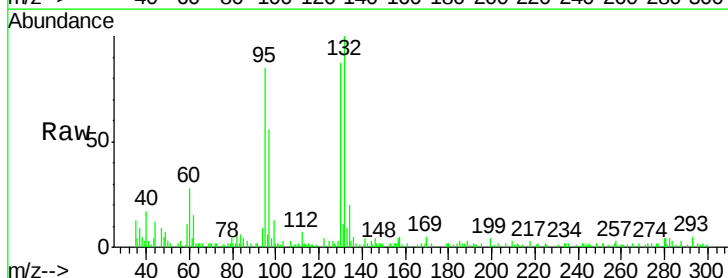

Abundance Ion 95.00 (94.70 to 95.70): VR0

Ion 96.95 (96.65 to 97.65): VR0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

