


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR062118\
Data File : VR025403.D
Acq On : 21 Jun 2018 18:15
Operator : SY/MD
Sample : J3615-06
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEXW3

Manual Integrations
APPROVED

MMDadoda
6/26/2018 12:01:58 PM

Quant Time: Jun 22 03:59:52 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 22 02:50:30 2018
Response via : Initial Calibration

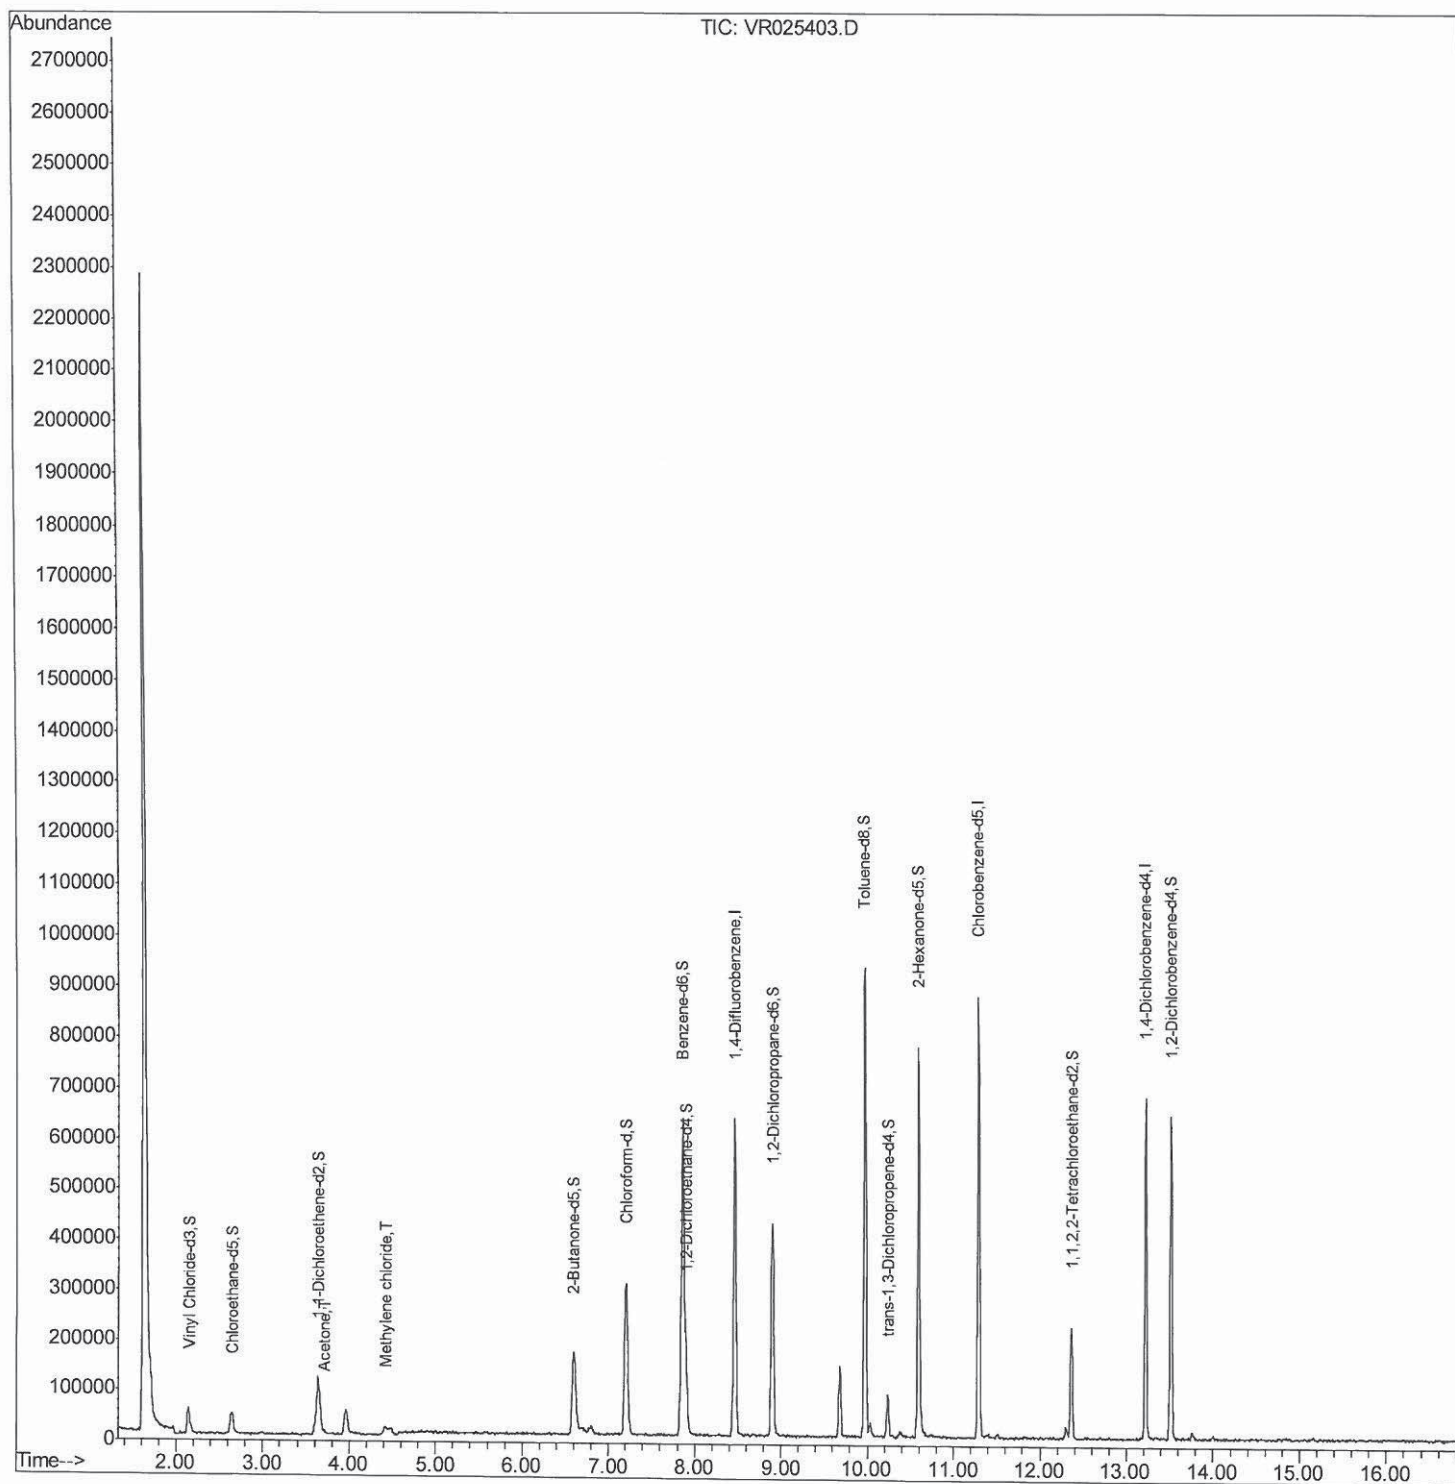




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR062118\
Data File : VR025403.D
Acq On : 21 Jun 2018 18:15
Operator : SY/MD
Sample : J3615-06
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEXW3

Manual Integrations
APPROVED

MMDadoda
6/26/2018 12:01:58 PM

Quant Time: Jun 22 02:54:04 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 22 02:50:30 2018
Response via : Initial Calibration

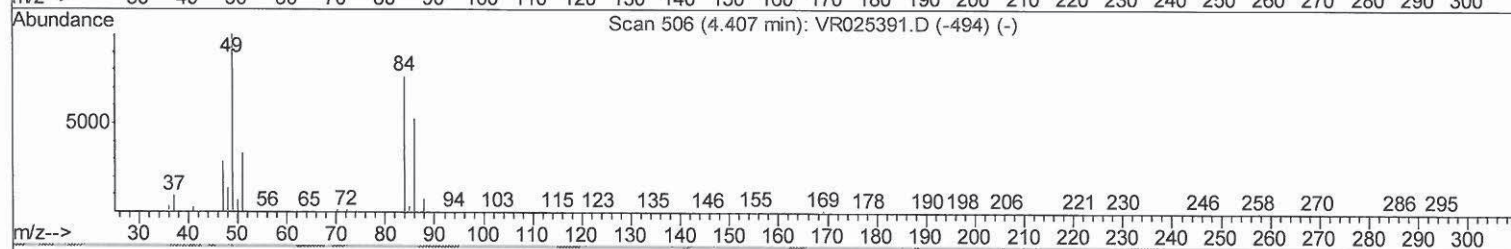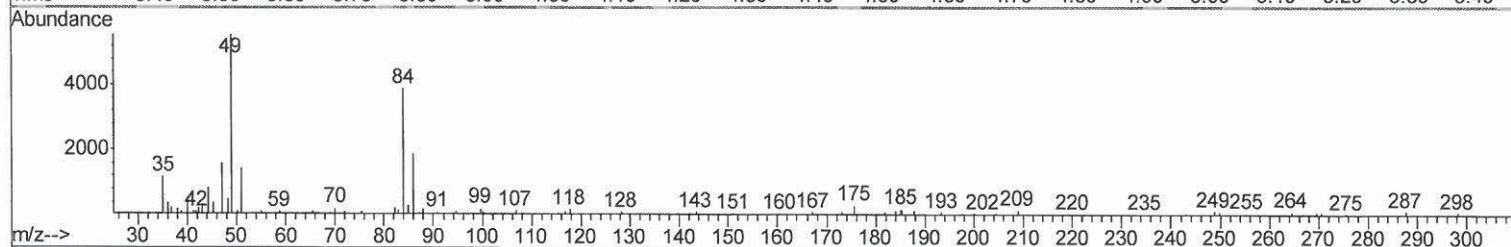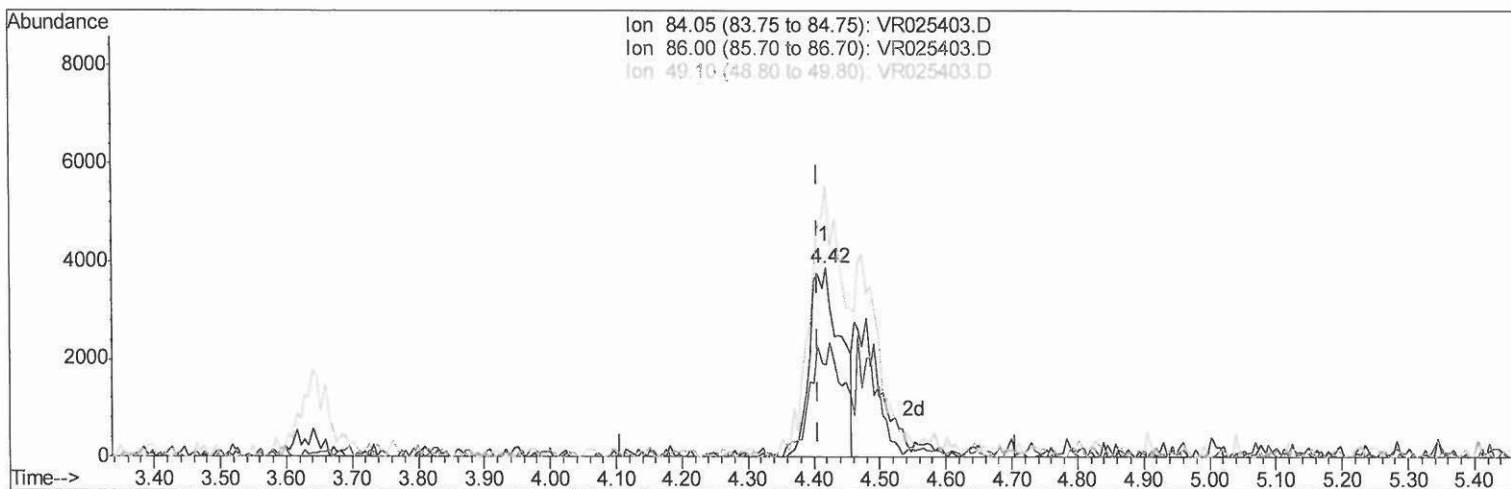

TIC: VR025403.D

(16) Methylene chloride (T)

4.419min (+0.012) 0.85ug/L

response 12745

Ion	Exp%	Act%
84.05	100	100
86.00	62.40	48.67
49.10	124.60	142.86
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR062118\
 Data File : VR025403.D
 Acq On : 21 Jun 2018 18:15
 Operator : SY/MD
 Sample : J3615-06
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEXW3

Manual Integrations
 APPROVED

MMDadoda
 6/26/2018 12:01:58 PM

Quant Time: Jun 22 02:54:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 22 02:50:30 2018
 Response via : Initial Calibration

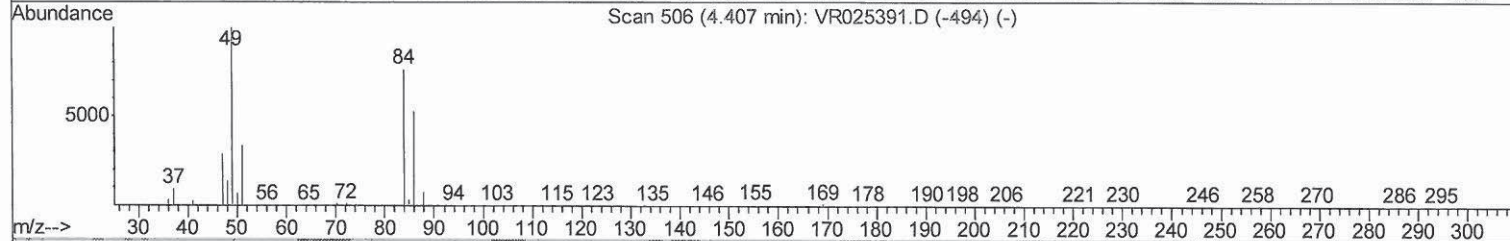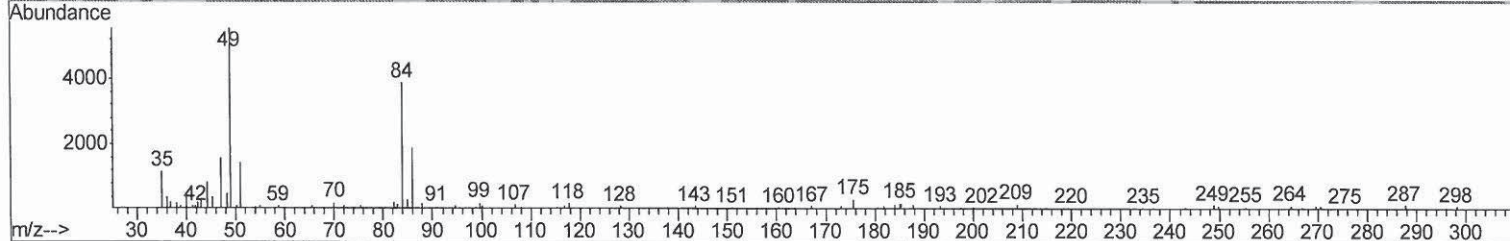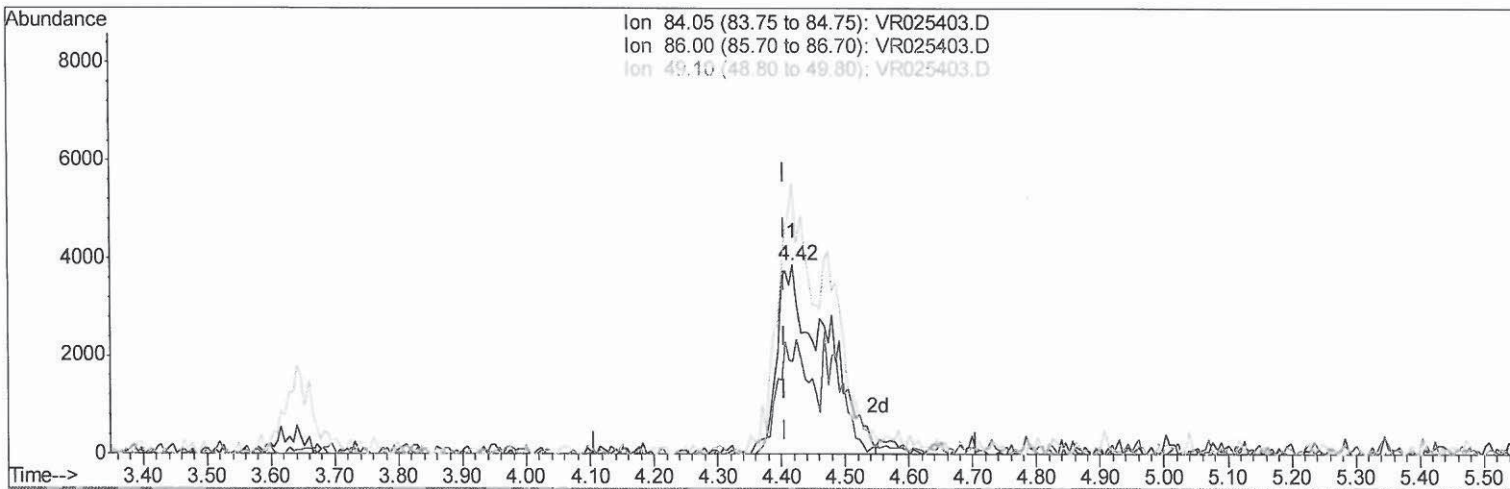

TIC: VR025403.D

(16) Methylene chloride (T)

4.419min (+0.012) 1.37ug/L m

response 20505

Ion	Exp%	Act%
84.05	100	100
86.00	62.40	48.67
49.10	124.60	142.86
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR062118\
 Data File : VR025403.D
 Acq On : 21 Jun 2018 18:15
 Operator : SY/MD
 Sample : J3615-06
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEXW3

Manual Integrations
 APPROVED

MMDadoda
 6/26/2018 12:01:58 PM

Quant Time: Jun 22 03:59:52 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 22 02:50:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	469097	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	412062	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	141910	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	67910	4.25	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.00%
7) Chloroethane-d5	2.64	69	56077	4.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.40%
11) 1,1-Dichloroethene-d2	3.64	63	137532	3.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.00%
20) 2-Butanone-d5	6.60	46	285089	66.57	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	133.14%#
24) Chloroform-d	7.21	84	317574	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
26) 1,2-Dichloroethane-d4	7.90	65	134935	5.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.20%
32) Benzene-d6	7.86	84	639894	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
36) 1,2-Dichloropropane-d6	8.90	67	202163	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	9.97	98	542637	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
43) trans-1,3-Dichloropropene-	10.24	79	40714	3.85	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.00%
46) 2-Hexanone-d5	10.59	63	243478	66.41	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	132.82%#
57) 1,1,2,2-Tetrachloroethane-	12.36	84	104346	6.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	135.20%#
64) 1,2-Dichlorobenzene-d4	13.51	152	139350	5.79	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.80%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	3.72	43	7228	3.737	ug/L	85
16) Methylene chloride	4.42	84	20505m	1.367	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed