

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR062118\
 Data File : VR025398.D
 Acq On : 21 Jun 2018 14:38
 Operator : SY/MD
 Sample : J3514-20RE
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 C0KH7RE

Quant Time: Jun 22 03:51:41 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 22 02:50:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.47	114	508564	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	430175	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	141383	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	66932	3.86	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.20%
7) Chloroethane-d5	2.64	69	54577	4.29	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.80%
11) 1,1-Dichloroethene-d2	3.64	63	144181	3.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.80%
20) 2-Butanone-d5	6.60	46	304229	65.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	131.04%#
24) Chloroform-d	7.20	84	349779	5.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.20%
26) 1,2-Dichloroethane-d4	7.89	65	143332	5.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.80%
32) Benzene-d6	7.86	84	708203	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
36) 1,2-Dichloropropane-d6	8.90	67	223634	5.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.00%
41) Toluene-d8	9.97	98	605483	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.80%
43) trans-1,3-Dichloropropene-	10.24	79	48811	4.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.60%
46) 2-Hexanone-d5	10.59	63	257468	67.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	134.54%#
57) 1,1,2,2-Tetrachloroethane-	12.36	84	102879	6.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	127.60%#
64) 1,2-Dichlorobenzene-d4	13.51	152	148705	6.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	124.00%#


Target Compounds					Ovalue
13) Acetone	3.71	43	13789	6.58 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR062118\
Data File : VR025398.D
Acq On : 21 Jun 2018 14:38
Operator : SY/MD
Sample : J3514-20RE
Misc : 25mL/MSVOA R/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0KH7RE

Quant Time: Jun 22 03:51:41 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 22 02:50:30 2018
Response via : Initial Calibration

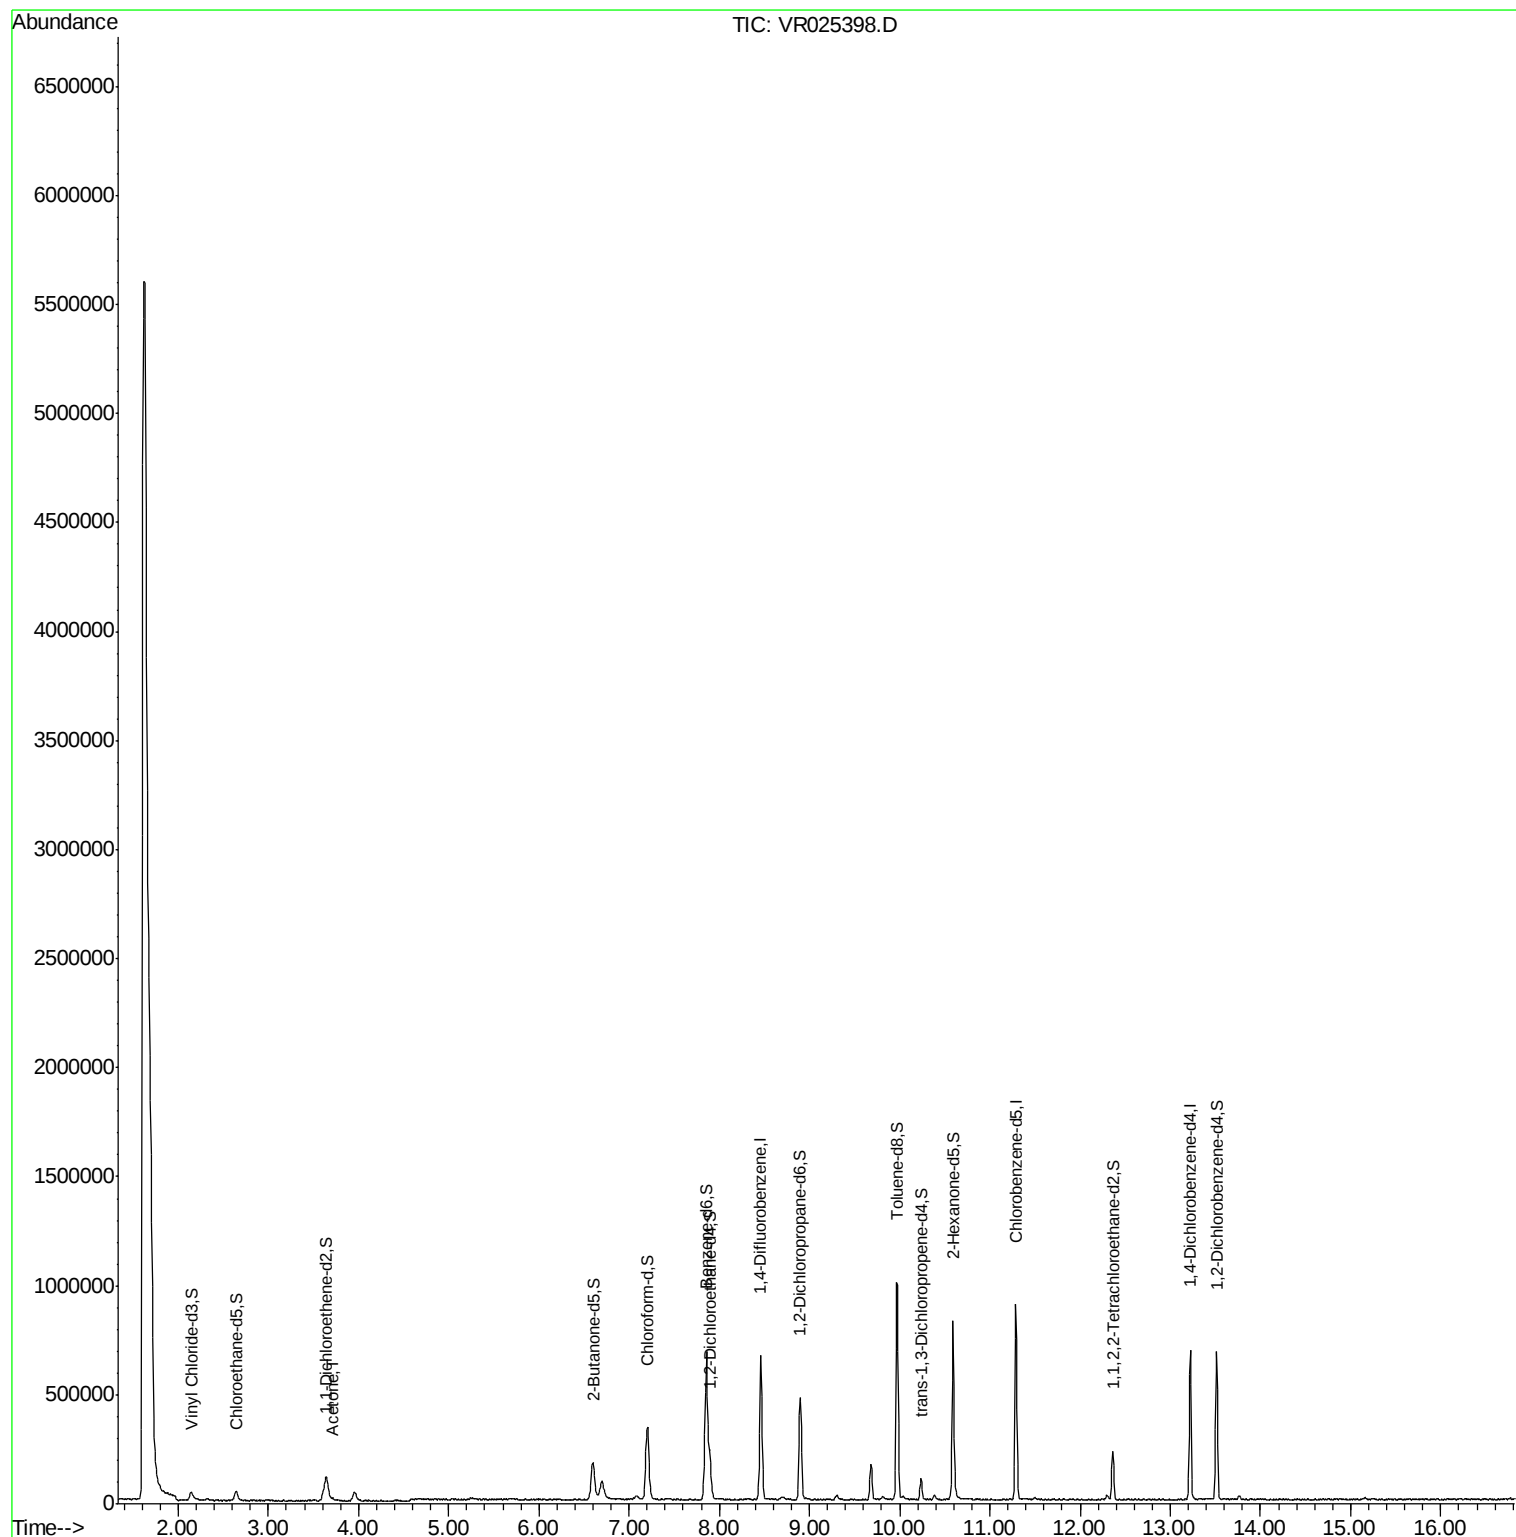

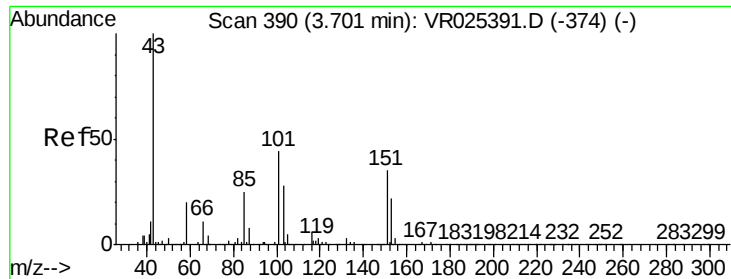

#13

Acetone

Concen: 6.58 ug/L

RT: 3.71 min Scan# 392

Delta R.T. 0.01 min

Lab File: VR025398.D

Acq: 21 Jun 2018 14:38

Instrument :
MSVOA_R
ClientSampleId :
C0KH7RE

Tot Ion: 43 Resp: 13789

Ion Ratio Lower Upper

43 100

58 22.8 0.0 41.6

