

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR062118\
 Data File : VR025405.D
 Acq On : 21 Jun 2018 19:21
 Operator : SY/MD
 Sample : J3615-03 1000X
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_R
 ClientSampleId :
 BEXT9

Quant Time: Jun 22 04:03:20 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 22 02:50:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	504676	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	435464	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	142338	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	60557	3.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	70.40%
7) Chloroethane-d5	2.64	69	48545	3.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.80%
11) 1,1-Dichloroethene-d2	3.65	63	133585	3.02	ug/L	0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.40%
20) 2-Butanone-d5	6.60	46	305883	66.39	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.78%#
24) Chloroform-d	7.20	84	324748	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	7.89	65	141314	5.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.00%
32) Benzene-d6	7.86	84	662786	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
36) 1,2-Dichloropropane-d6	8.90	67	213755	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.00%
41) Toluene-d8	9.97	98	558643	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.60%
43) trans-1,3-Dichloropropene-	10.24	79	38724	3.47	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.40%
46) 2-Hexanone-d5	10.59	63	266430	68.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	137.52%#
57) 1,1,2,2-Tetrachloroethane-	12.36	84	106413	6.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	130.40%#
64) 1,2-Dichlorobenzene-d4	13.51	152	141092	5.84	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.80%


Target Compounds					Ovalue
33) Benzene	7.91	78	193002	1.13 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA R\DATA\VR062118\
Data File : VR025405.D
Acq On : 21 Jun 2018 19:21
Operator : SY/MD
Sample : J3615-03 1000X
Misc : 25mL/MSVOA R/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BEXT9

Quant Time: Jun 22 04:03:20 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR061518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 22 02:50:30 2018
Response via : Initial Calibration

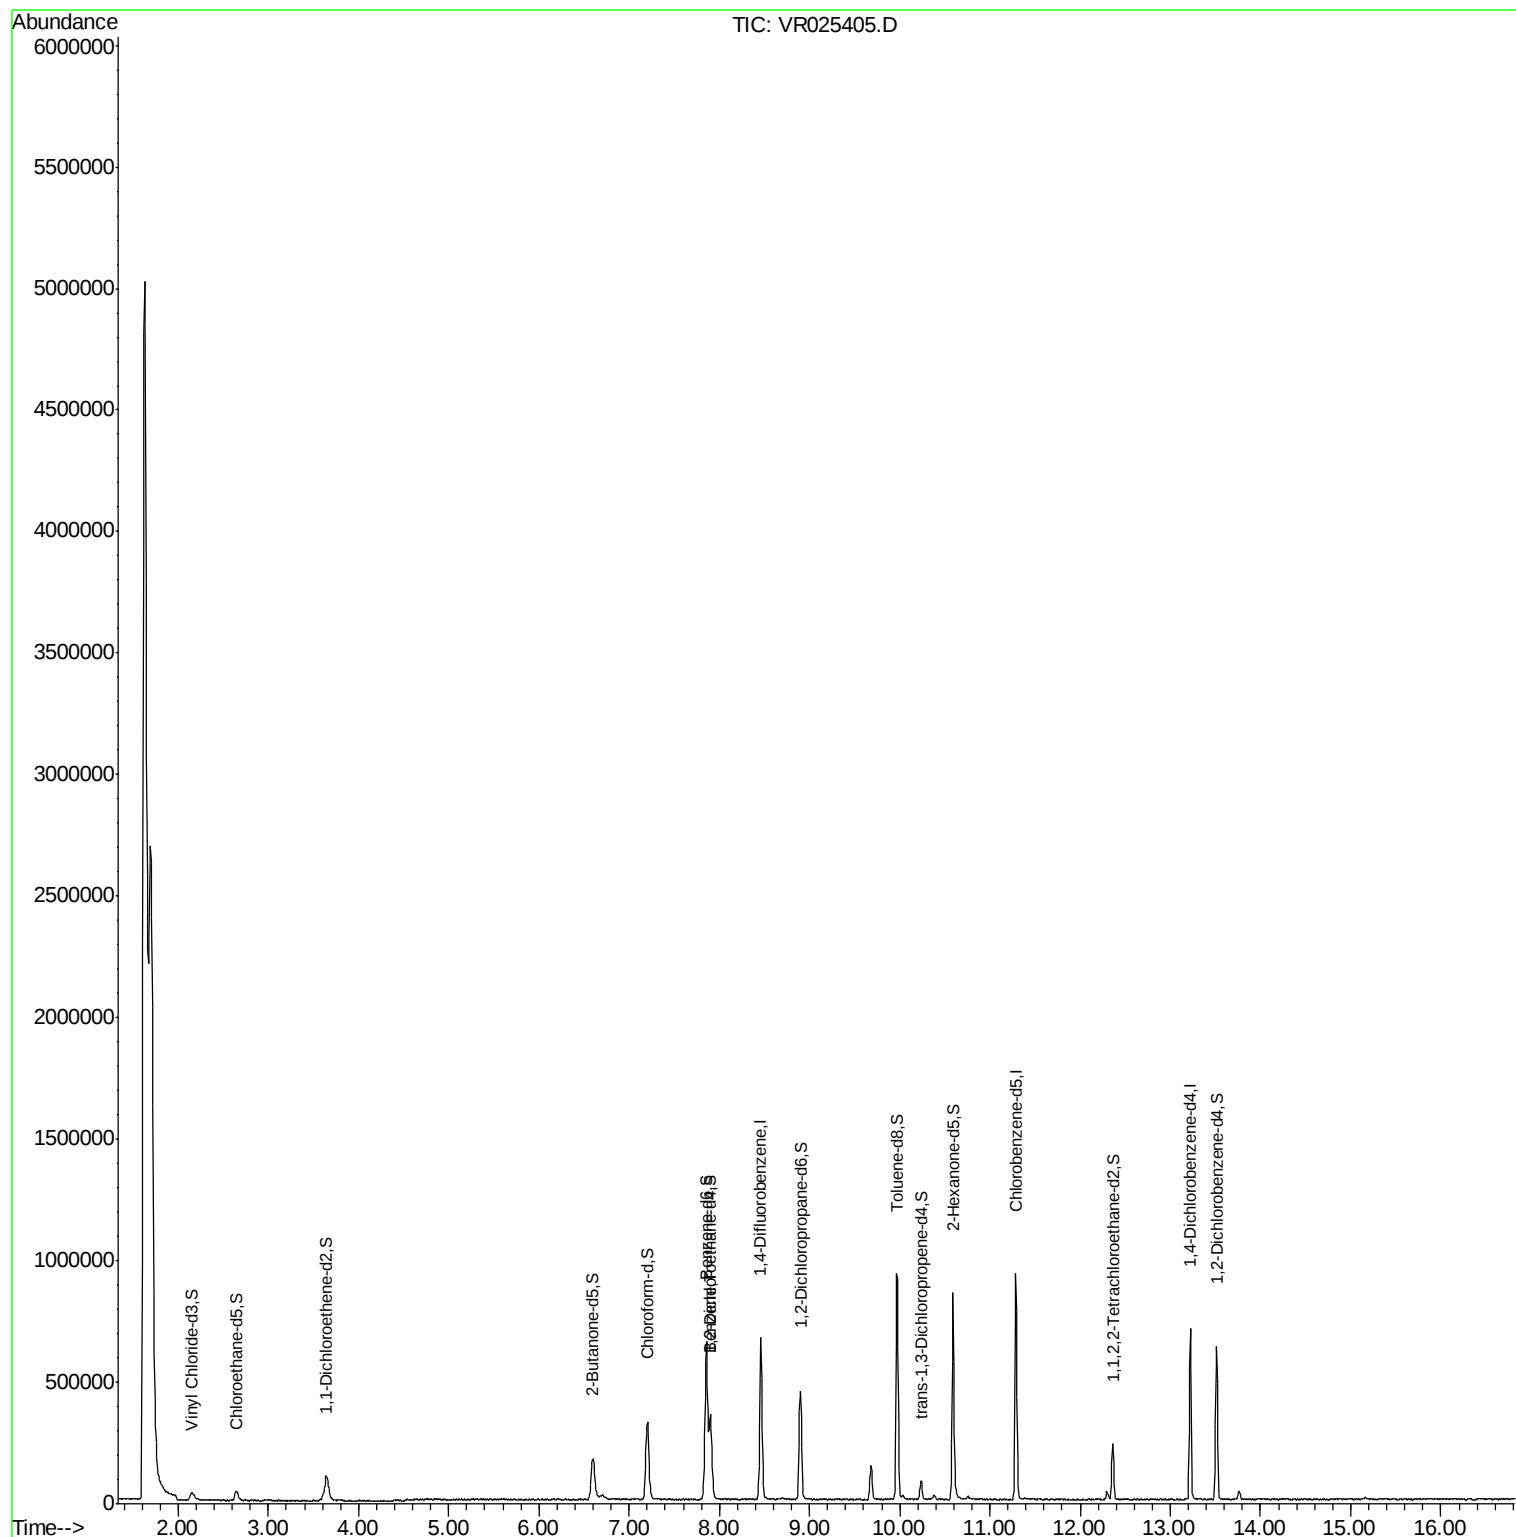

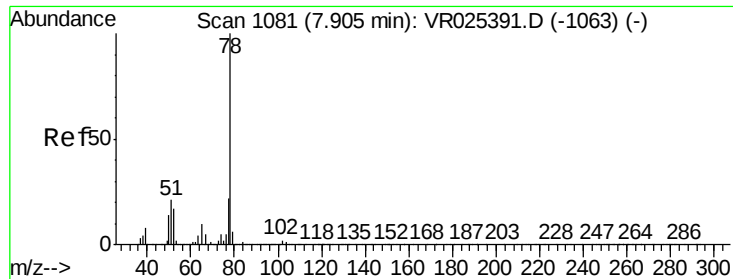

#33

Benzene

Concen: 1.13 ug/L

RT: 7.91 min Scan# 1081

Delta R.T. 0.00 min

Lab File: VR025405.D

Acq: 21 Jun 2018 19:21

Instrument :

MSVOA_R

ClientSampleId :

BEXT9

Tgt Ion: 78 Resp: 193002

