

Data File : VR025452.D
Acq On : 12 Jul 2018 15:22
Operator : SY/MD
Sample : J3960-08
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0AH6

Quant Time: Jul 13 00:50:36 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR070518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 13 00:37:37 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	1012485	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	770460	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	282651	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	101779	3.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.00%
7) Chloroethane-d5	2.63	69	82540	3.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.40%
11) 1,1-Dichloroethene-d2	3.63	63	216514	2.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	51.20%#
20) 2-Butanone-d5	6.59	46	309859	35.74	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	71.48%
24) Chloroform-d	7.20	84	470551	3.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	68.20%#
26) 1,2-Dichloroethane-d4	7.89	65	178860	3.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.60%#
32) Benzene-d6	7.85	84	1032025	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.00%
36) 1,2-Dichloropropane-d6	8.90	67	269182	3.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	72.00%
41) Toluene-d8	9.97	98	886186	3.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.40%
43) trans-1,3-Dichloropropene-	10.24	79	74795	3.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.40%
46) 2-Hexanone-d5	10.59	63	235785	36.81	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.62%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	111557	3.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	66.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	189702	4.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	81.40%


Target Compounds					Qvalue
13) Acetone	3.70	43	15352	3.930 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VR025452.D
Acq On : 12 Jul 2018 15:22
Operator : SY/MD
Sample : J3960-08
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
C0AH6

Quant Time: Jul 13 00:50:36 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR070518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 13 00:37:37 2018
Response via : Initial Calibration

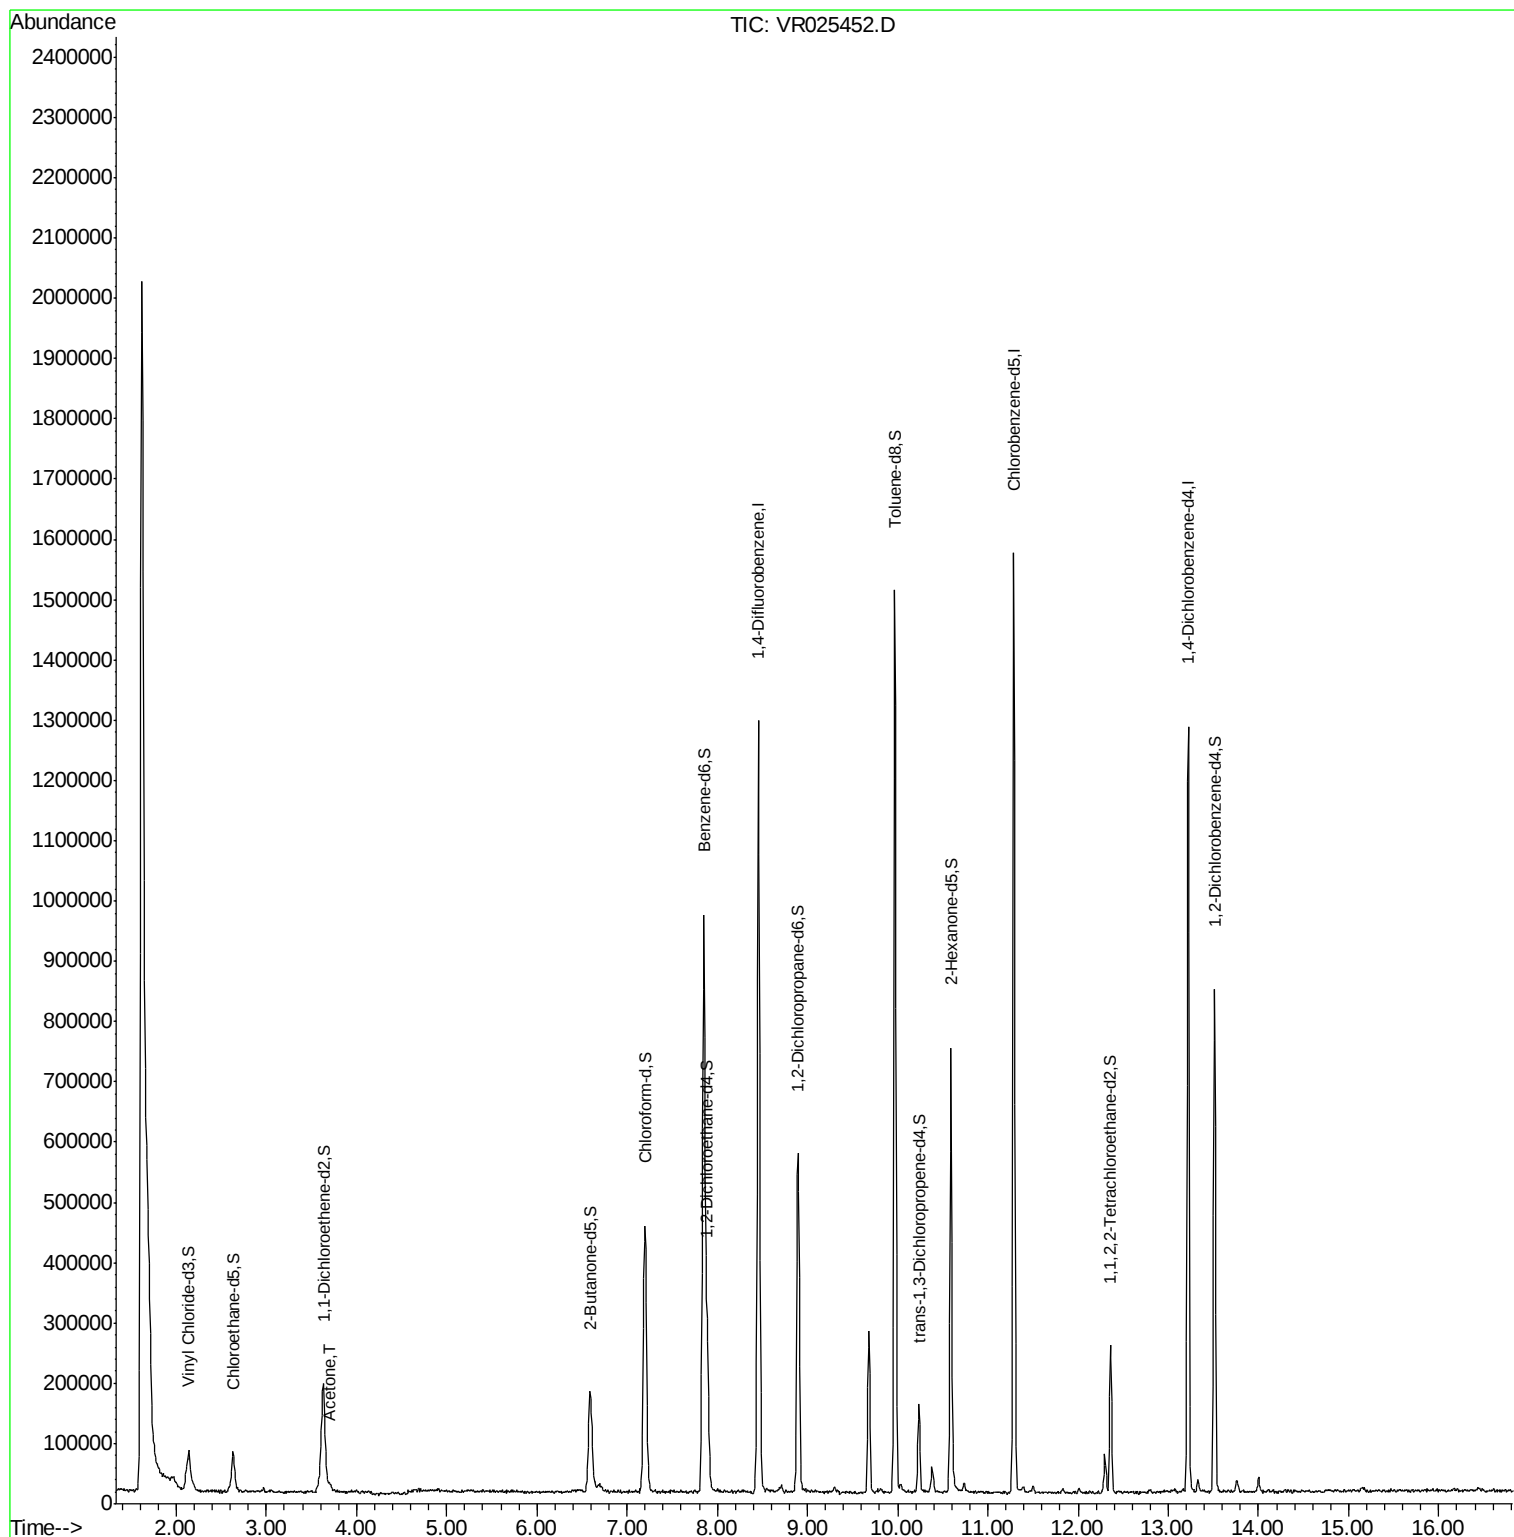

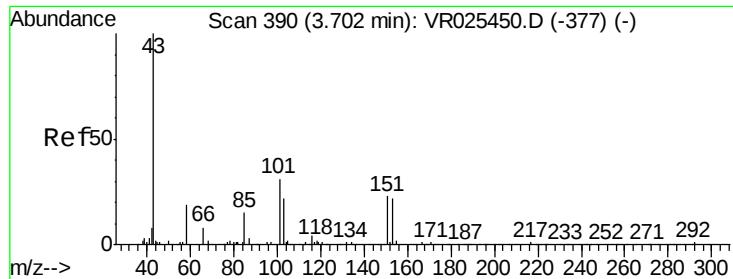

#13

Acetone

Concen: 3.930 ug/L

RT: 3.70 min Scan# 390

Delta R.T. -0.00 min

Lab File: VR025452.D

Acq: 12 Jul 2018 15:22

Instrument :

MSVOA_R

ClientSampleId :


C0AH6

Tgt Ion: 43 Resp: 15352

Ion Ratio Lower Upper

43 100

58 21.5 0.0 41.6

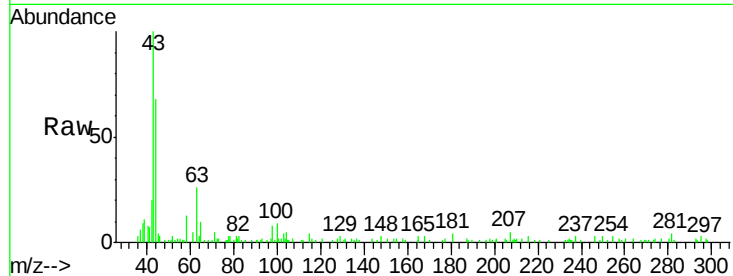

Abundance Ion 43.05 (42.75 to 43.75): VR0

Ion 58.05 (57.75 to 58.75): VR0

