

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR073018\

Quantitation Report (QT Reviewed)

Data File : VR025538.D

Acq On : 30 Jul 2018 12:29

Operator : SY/MD

Sample : VSTD00182

Misc : 25mL/MSVOA_R/WATER

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 30 15:11:14 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Jul 30 15:00:06 2018

Response via : Initial Calibration

Instrument :

MSVOA_R

Client Sampled :


VSTD00182

Manual Integrations

APPROVED

MMDadoda

7/31/2018 6:22:46 PM

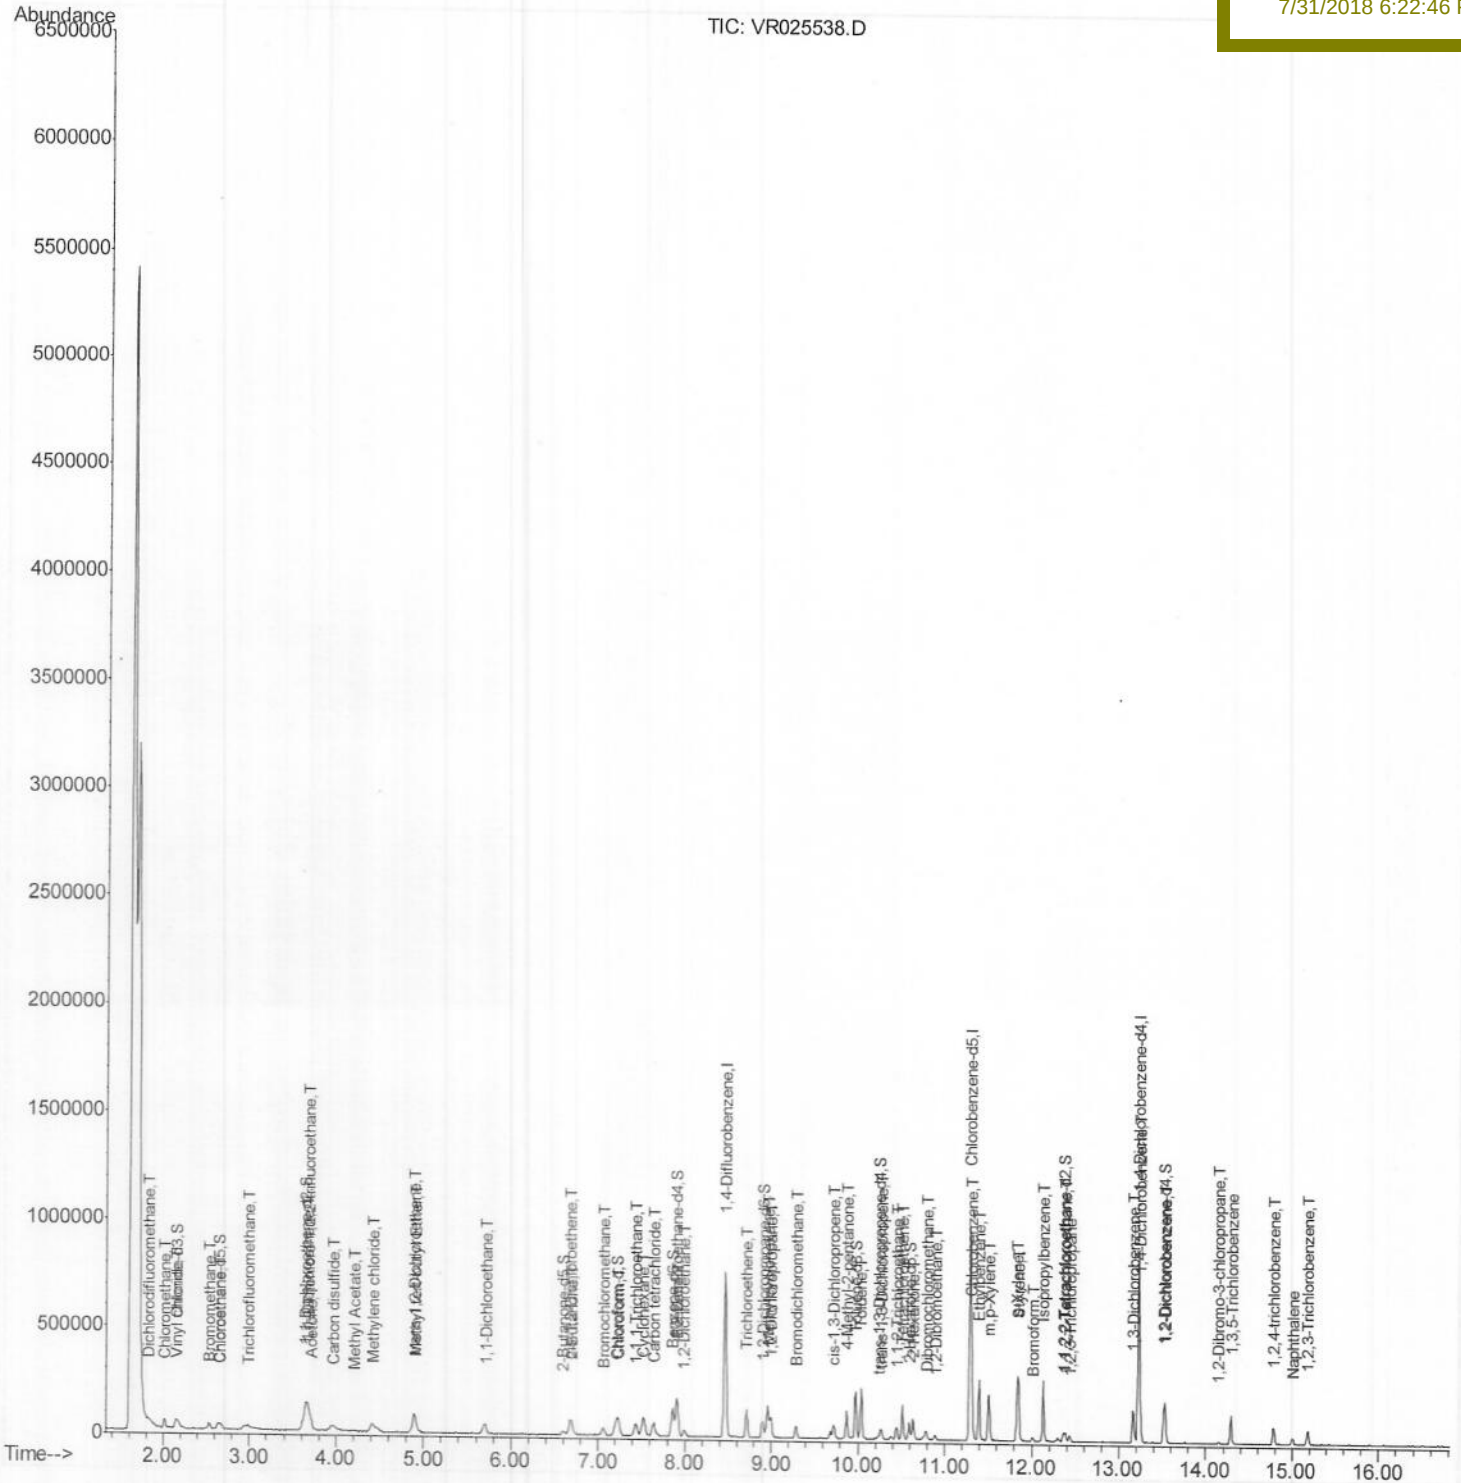

SOMRTR073018WMA.M Mon Jul 30 15:12:27 2018




Data File : VR025538.D
Acq On : 30 Jul 2018 12:29
Operator : SY/MD
Sample : VSTD00182
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 30 15:01:18 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 15:00:06 2018
Response via : Initial Calibration

Instrument :
MSVOA_R
Client Sampled :
VSTD00182

Manual Integrations
APPROVED

MMDadoda
7/31/2018 6:22:46 PM

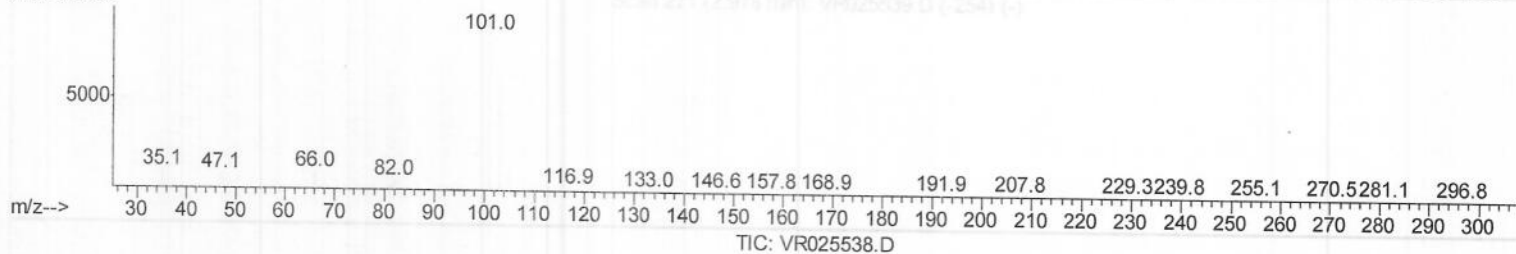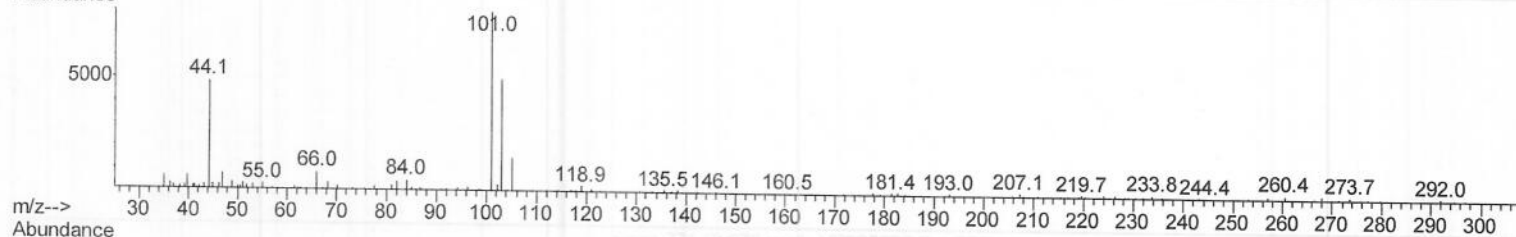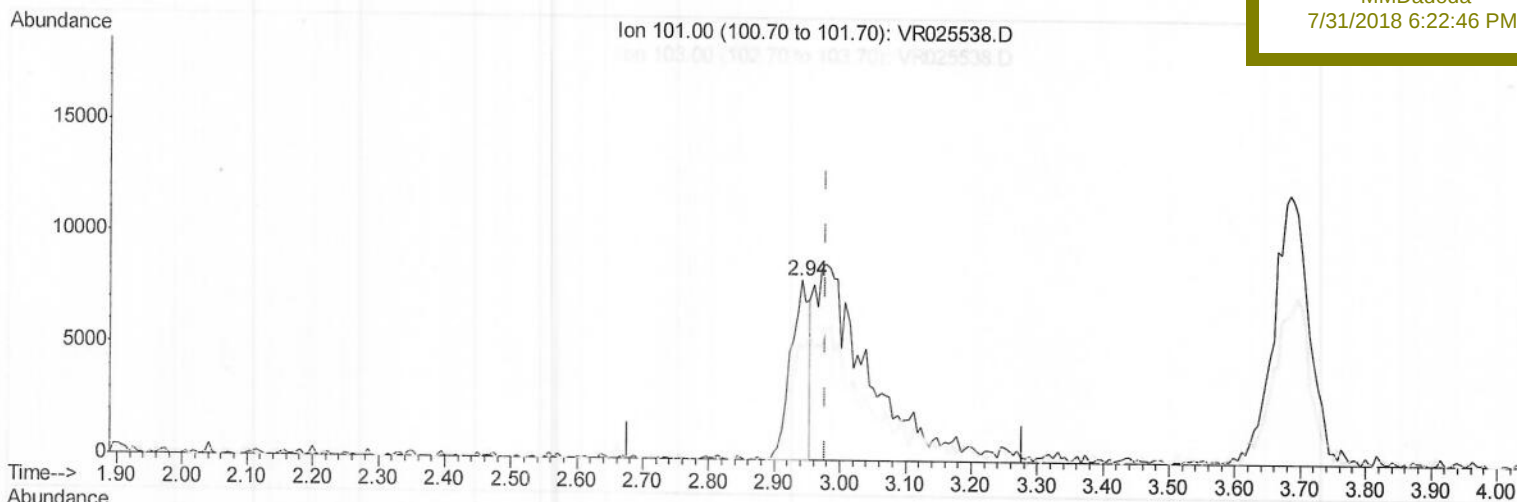

(9) Trichlorofluoromethane (T)

2.941min (-0.036) 0.50ug/L

response 16038

Ion	Exp%	Act%
101.00	100	100
103.00	24.70	81.36#
0.00	0.00	0.00
0.00	0.00	0.00




Data File : VR025538.D
Acq On : 30 Jul 2018 12:29
Operator : SY/MD
Sample : VSTD00182
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 30 15:01:18 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 15:00:06 2018
Response via : Initial Calibration

Instrument :
MSVOA_R
Client Sampled :
VSTD00182

Manual Integrations
APPROVED

MMDadoda
7/31/2018 6:22:46 PM

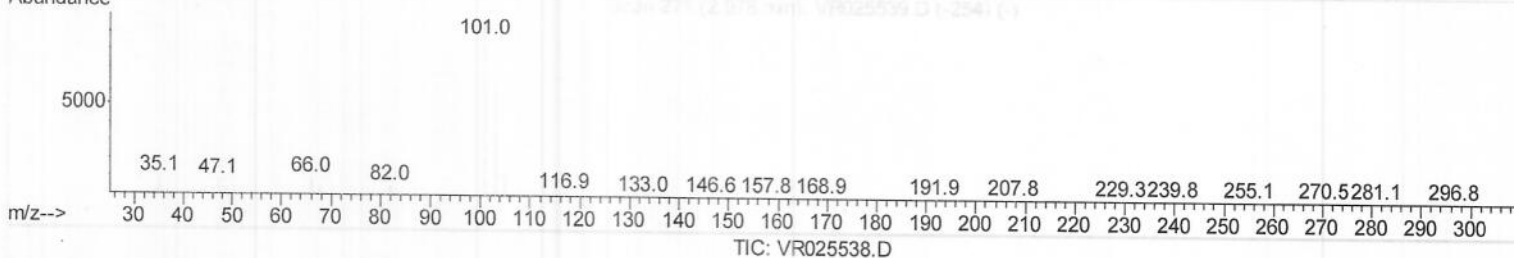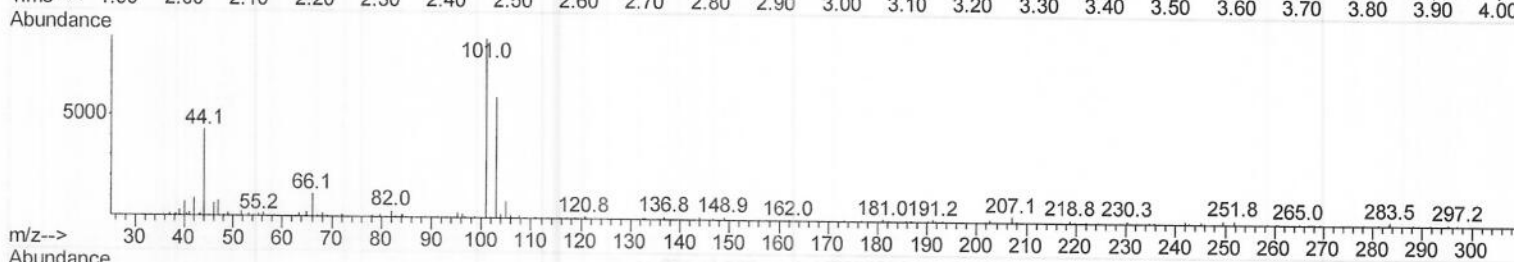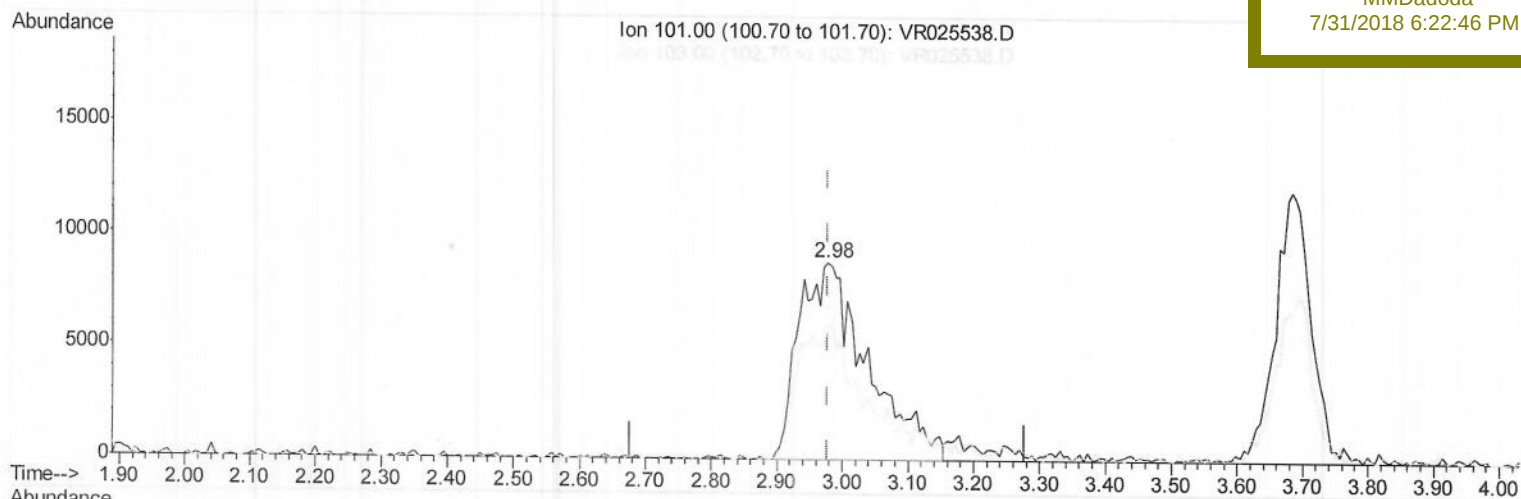

(9) Trichlorofluoromethane (T)

2.978min (+0.000) 2.00ug/L m) MDO8/07/18

response 63693

Ion	Exp%	Act%
101.00	100	100
103.00	24.70	20.49
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR073018\
Quantitation Report (Qedit)


Data File : VR025538.D
Acq On : 30 Jul 2018 12:29
Operator : SY/MD
Sample : VSTD00182
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 30 15:01:18 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 15:00:06 2018
Response via : Initial Calibration

Instrument :
MSVOA_R
ClientSampleId :
VSTD00182

Manual Integrations
APPROVED

MMDadoda
7/31/2018 6:22:46 PM

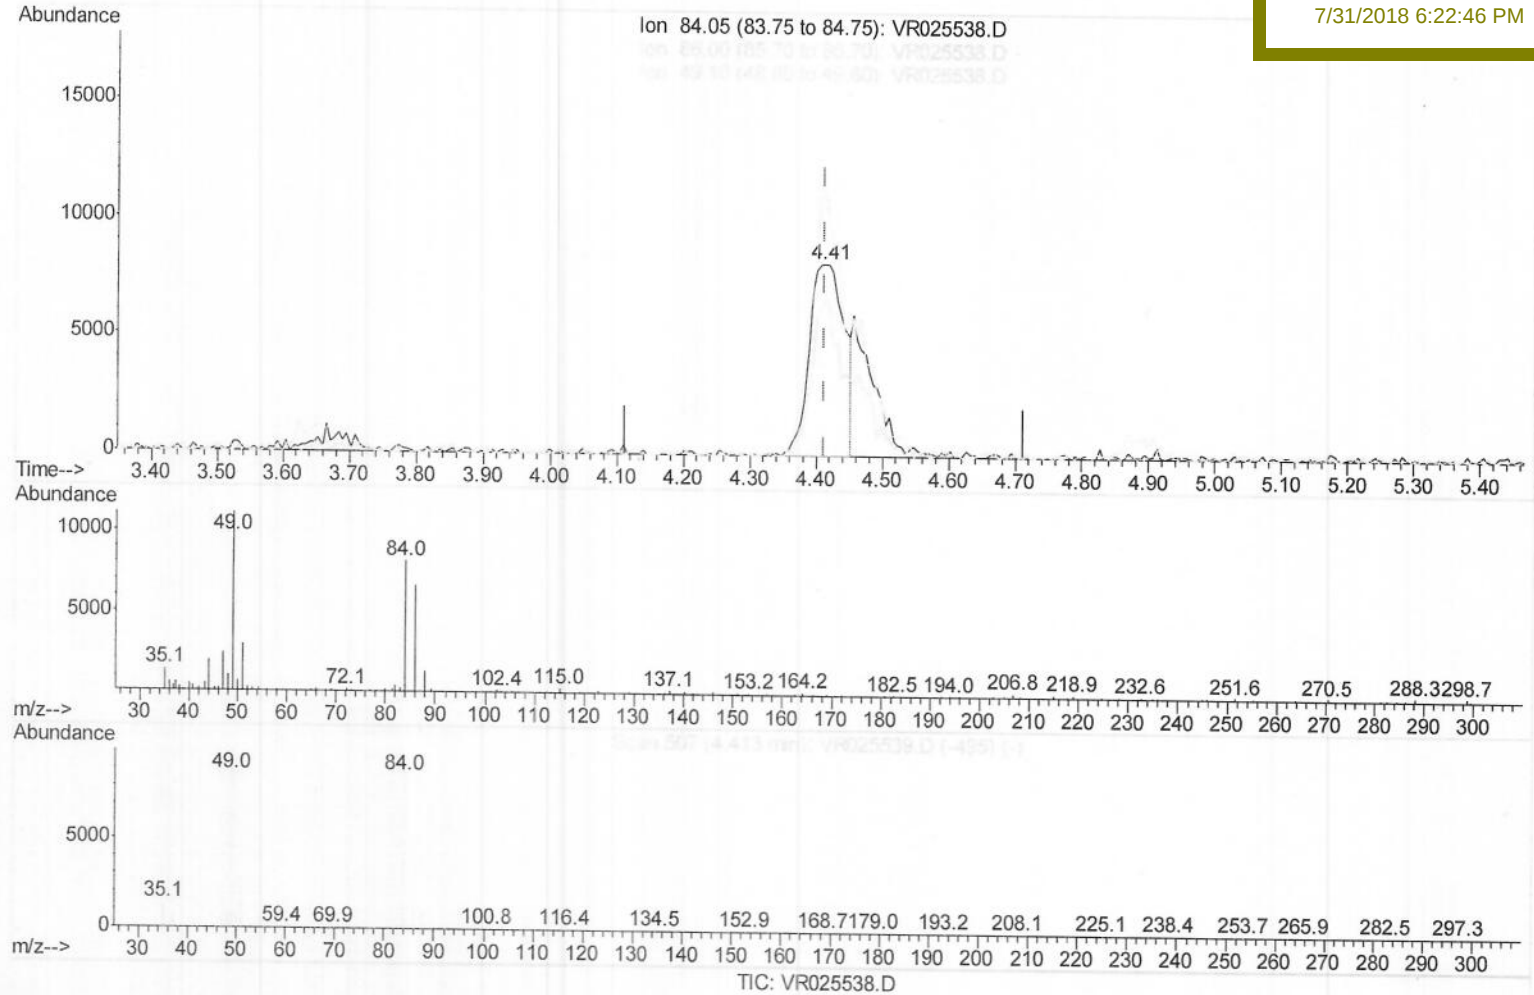

(16) Methylene chloride (T)

4.413min (+0.000) 1.55ug/L

response 29380

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	81.68#
49.10	108.80	136.46
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR073018\
Quantitation Report (Qedit)


Data File : VR025538.D
Acq On : 30 Jul 2018 12:29
Operator : SY/MD
Sample : VSTD00182
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 30 15:01:18 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 15:00:06 2018
Response via : Initial Calibration

Instrument :
MSVOA_R
Client Sample Id :
VSTD00182

Manual Integrations
APPROVED

MMDadoda
7/31/2018 6:22:46 PM

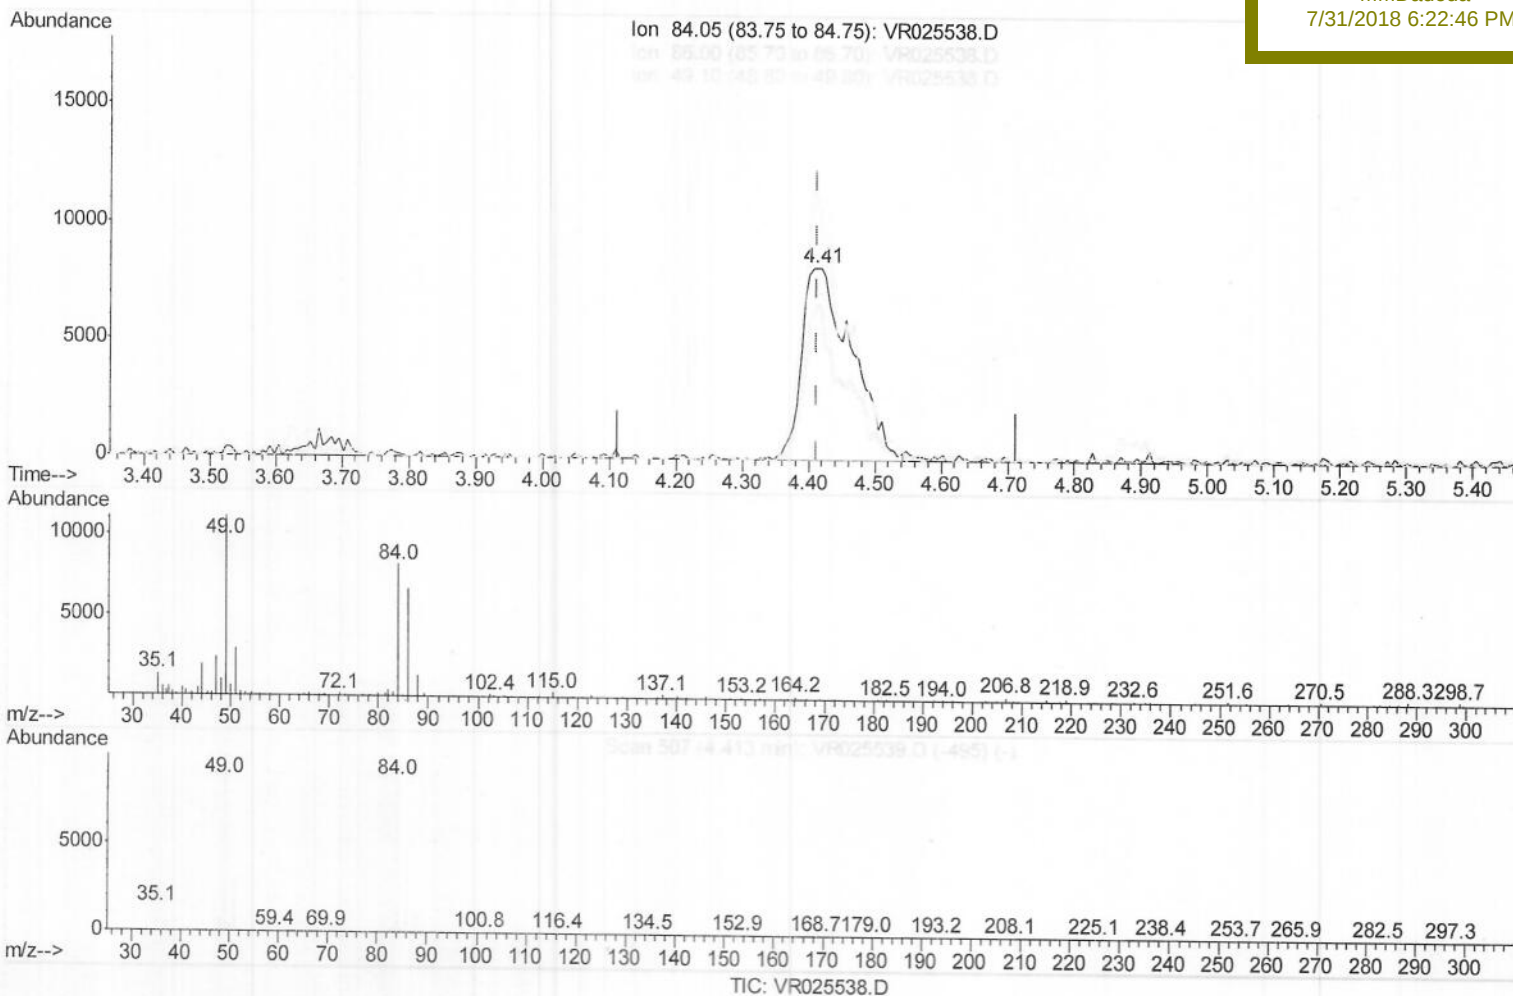

(16) Methylene chloride (T)

4.413min (+0.000) 2.26ug/L m) M P 08/07/18

response 42699

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	81.68#
49.10	108.80	136.46
0.00	0.00	0.00

Data File : VR025538.D
Acq On : 30 Jul 2018 12:29
Operator : SY/MD
Sample : VSTD00182
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampled :
VSTD00182

Quant Time: Jul 30 15:11:14 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 15:00:06 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
7/31/2018 6:22:46 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.47	114	646358	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	521646	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	209960	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	41836	2.35	ug/L	0.00
7) Chloroethane-d5	2.64	69	33017	2.17	ug/L	0.00
11) 1,1-Dichloroethene-d2	3.64	63	93063	1.72	ug/L	0.00
20) 2-Butanone-d5	6.60	46	26832	4.85	ug/L	0.00
24) Chloroform-d	7.21	84	65835	0.75	ug/L	0.00
26) 1,2-Dichloroethane-d4	7.90	65	20922	0.62	ug/L	0.00
32) Benzene-d6	7.86	84	140475	0.80	ug/L	0.00
36) 1,2-Dichloropropane-d6	8.90	67	37444	0.74	ug/L	0.00
41) Toluene-d8	9.97	98	133060	0.87	ug/L	0.00
43) trans-1,3-Dichloropropene-	10.24	79	8644	0.64	ug/L	0.00
46) 2-Hexanone-d5	10.59	63	25263	5.83	ug/L	0.00
57) 1,1,2,2-Tetrachloroethane-	12.36	84	16403	0.72	ug/L	0.00
64) 1,2-Dichlorobenzene-d4	13.51	152	32986	0.95	ug/L	0.00

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.83	85	38000	1.041	ug/L	98
3) Chloromethane	2.02	50	50256	2.322	ug/L	95
5) Vinyl chloride	2.16	62	51142	2.629	ug/L	87
6) Bromomethane	2.53	94	25411	2.220	ug/L	85
8) Chloroethane	2.67	64	29322	2.421	ug/L	86
9) Trichlorofluoromethane	2.98	101	63693m	2.004	ug/L	
10) 1,1,2-Trichloro-1,2,2-trif	3.68	101	44745	2.313	ug/L	97
12) 1,1-Dichloroethene	3.66	96	47316	2.449	ug/L	88
13) Acetone	3.71	43	23312	9.349	ug/L	97
14) Carbon disulfide	3.97	76	101695	2.313	ug/L #	95
15) Methyl Acetate	4.21	43	7631	1.368	ug/L #	77
16) Methylene chloride	4.41	84	42699m	2.256	ug/L	
17) Methyl tert-butyl Ether	4.91	73	42316	0.672	ug/L #	84
18) trans-1,2-Dichloroethene	4.89	96	42733	0.889	ug/L	95
19) 1,1-Dichloroethane	5.70	63	64859	0.787	ug/L #	92
21) 2-Butanone	6.69	43	30511	5.253	ug/L	99
22) cis-1,2-Dichloroethene	6.68	96	37159	0.842	ug/L #	98
23) Bromochloromethane	7.06	128	13474	0.949	ug/L #	86
25) Chloroform	7.24	83	64294	0.812	ug/L	91
27) 1,2-Dichloroethane	8.00	62	25367	0.714	ug/L	96
29) 1,1,1-Trichloroethane	7.43	97	48644	0.917	ug/L	99
30) Cyclohexane	7.52	56	47585	0.836	ug/L	100
31) Carbon tetrachloride	7.64	117	47556	1.013	ug/L	100
33) Benzene	7.91	78	163055	0.907	ug/L	100
34) Trichloroethene	8.71	95	39748	0.868	ug/L	95
35) Methylcyclohexane	8.96	83	54916	0.897	ug/L	96
37) 1,2-Dichloropropane	9.00	63	35061	0.839	ug/L #	96
38) Bromodichloromethane	9.29	83	33136	0.778	ug/L #	92
39) cis-1,3-Dichloropropene	9.72	75	32477	0.691	ug/L	86
40) 4-Methyl-2-pentanone	9.86	43	83359	6.882	ug/L	98

M08/07/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR073018\

Quantitation Report (QT Reviewed)

Data File : VR025538.D

Acq On : 30 Jul 2018 12:29

Operator : SY/MD

Sample : VSTD00182

Misc : 25mL/MSVOA_R/WATER

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 30 15:11:14 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Jul 30 15:00:06 2018

Response via : Initial Calibration

Instrument :

MSVOA_R

ClientSampled :

VSTD00182

Manual Integrations

APPROVED

MMDadoda

7/31/2018 6:22:46 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) Toluene	10.03	91	165471	0.946	ug/L	98
44) trans-1,3-Dichloropropene	10.27	75	21971	0.637	ug/L	93
45) 1,1,2-Trichloroethane	10.45	97	17159	0.838	ug/L	90
47) Tetrachloroethene	10.52	164	34132	1.142	ug/L	93
48) 2-Hexanone	10.64	43	58066	6.969	ug/L	95
49) Dibromochloromethane	10.79	129	19572	0.917	ug/L	96
50) 1,2-Dibromoethane	10.89	107	13421	0.809	ug/L #	73
51) Chlorobenzene	11.31	112	106187	0.997	ug/L	97
52) Ethylbenzene	11.39	91	179580	0.958	ug/L	96
53) m,p-Xylene	11.51	106	66804	0.950	ug/L	93
54) o-Xylene	11.83	106	57824	0.954	ug/L	97
55) Styrene	11.85	104	96648	0.969	ug/L	97
56) Isopropylbenzene	12.13	105	157654	0.982	ug/L	100
58) 1,1,2,2-Tetrachloroethane	12.38	83	16499	0.818	ug/L	98
59) 1,2,3-Trichloropropane	12.43	75	11150	0.768	ug/L	93
61) Bromoform	12.01	173	8184	0.957	ug/L #	93
62) 1,3-Dichlorobenzene	13.16	146	58348	0.948	ug/L	88
63) 1,4-Dichlorobenzene	13.24	146	70605	1.034	ug/L	99
65) 1,2-Dichlorobenzene	13.53	146	54265	1.015	ug/L	97
66) 1,2-Dibromo-3-chloropropan	14.15	75	2066	0.874	ug/L #	66
67) 1,3,5-Trichlorobenzene	14.29	180	40655	1.012	ug/L	97
68) 1,2,4-trichlorobenzene	14.79	180	23962	0.868	ug/L	98
69) Naphthalene	15.00	128	21587	0.610	ug/L	97
70) 1,2,3-Trichlorobenzene	15.18	180	20178	0.947	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed