

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR073018\
Data File : VR025544.D
Acq On : 30 Jul 2018 17:49
Operator : SY/MD
Sample : J4202-02
Misc : 25mL/MSVOA R/WATER
ALS Vial : 9 Sample Multiplier: 1


Quant Time: Jul 31 08:38:06 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jul 30 16:58:41 2018
Response via : Initial Calibration

Instrument :
MSVOA_R
ClientSampleId :
BE720

Manual Integrations
APPROVED

MMDadoda
7/31/2018 6:22:49 PM

7/31/2018 6:22:49 PM

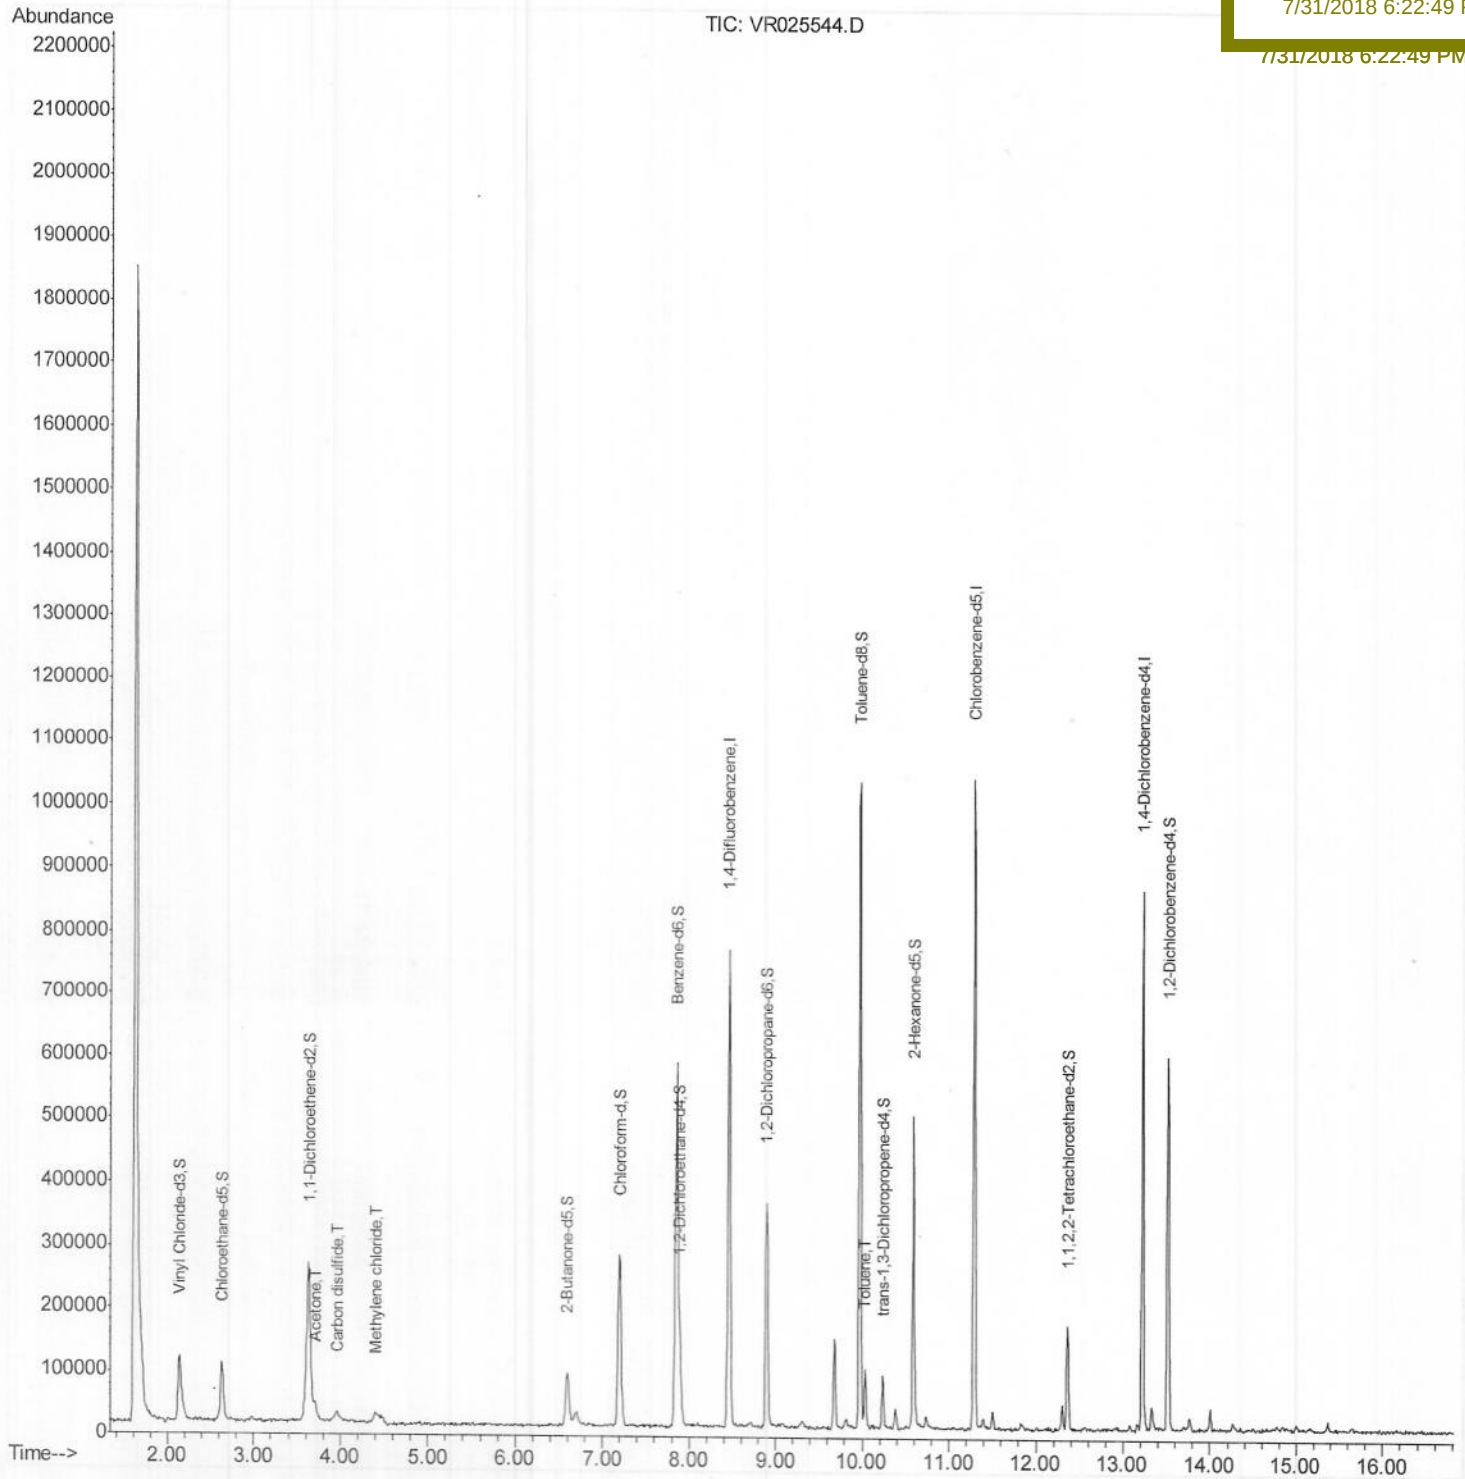

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR073018\

Data File : VR025544.D

Acq On : 30 Jul 2018 17:49

Operator : SY/MD

Sample : J4202-02

Misc : 25mL/MSVOA R/WATER

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Jul 31 08:27:24 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Jul 30 16:58:41 2018

Response via : Initial Calibration

Instrument :

MSVOA_R

Client Sampled :




BE720

Manual Integrations
APPROVED

MMDadoda

7/31/2018 6:22:49 PM

7/31/2018 6:22:49 PM

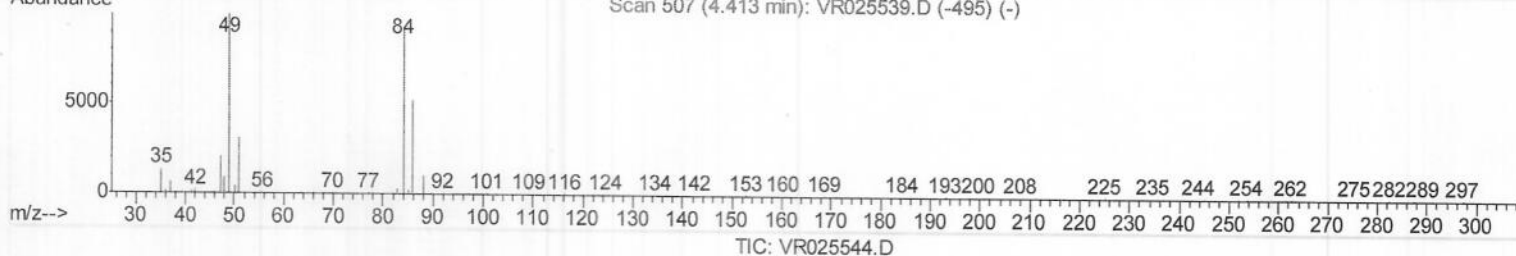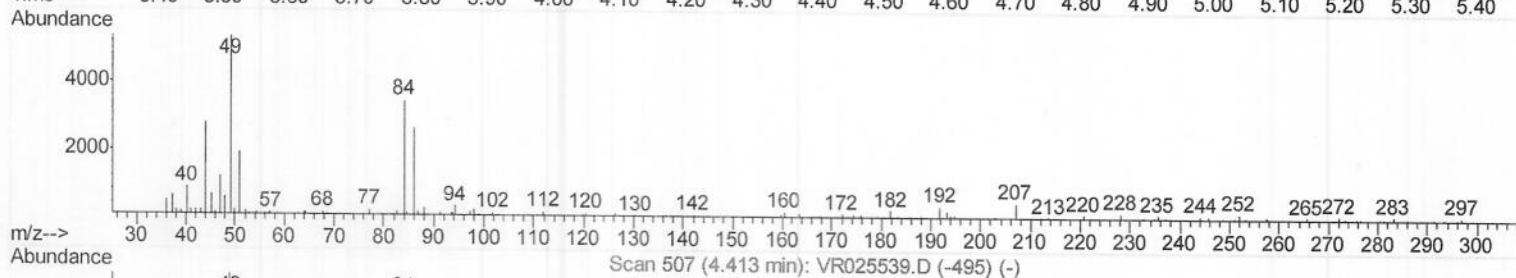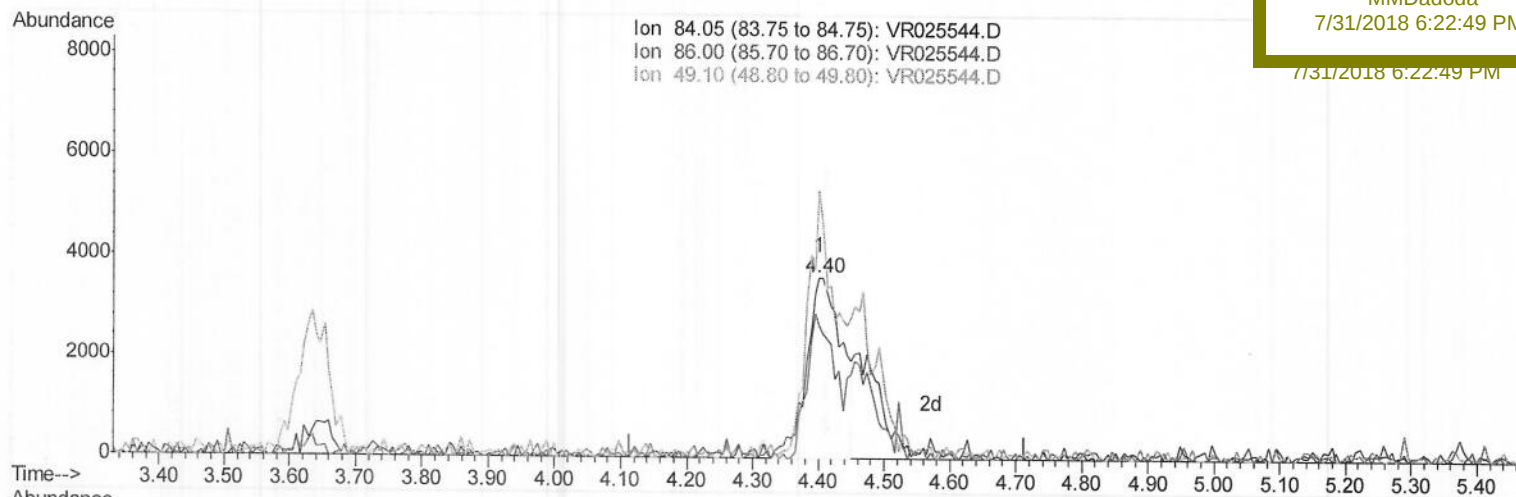

(16) Methylene chloride (T)

4.401min (-0.012) 0.35ug/L

response 13352

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	73.89
49.10	108.80	148.53#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR073018\

Data File : VR025544.D

Acq On : 30 Jul 2018 17:49

Operator : SY/MD

Sample : J4202-02

Misc : 25mL/MSVOA R/WATER

ALS Vial : 9 Sample Multiplier: 1

Quant Time: Jul 31 08:27:24 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Jul 30 16:58:41 2018

Response via : Initial Calibration

Instrument :

MSVOA_R

ClientSampleId :

BE720




Manual Integrations

APPROVED

MMDadoda

7/31/2018 6:22:49 PM

7/31/2018 6:22:49 PM

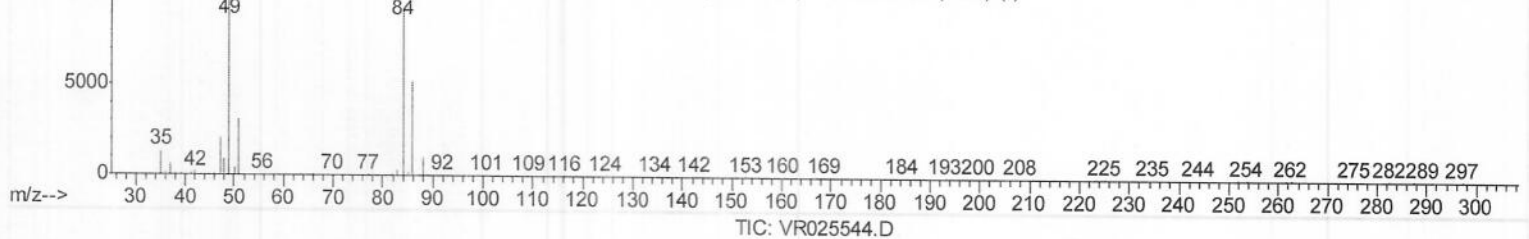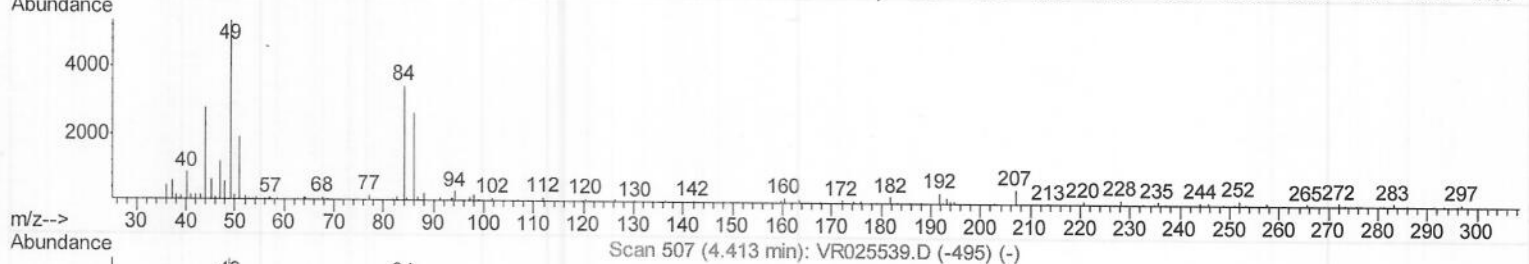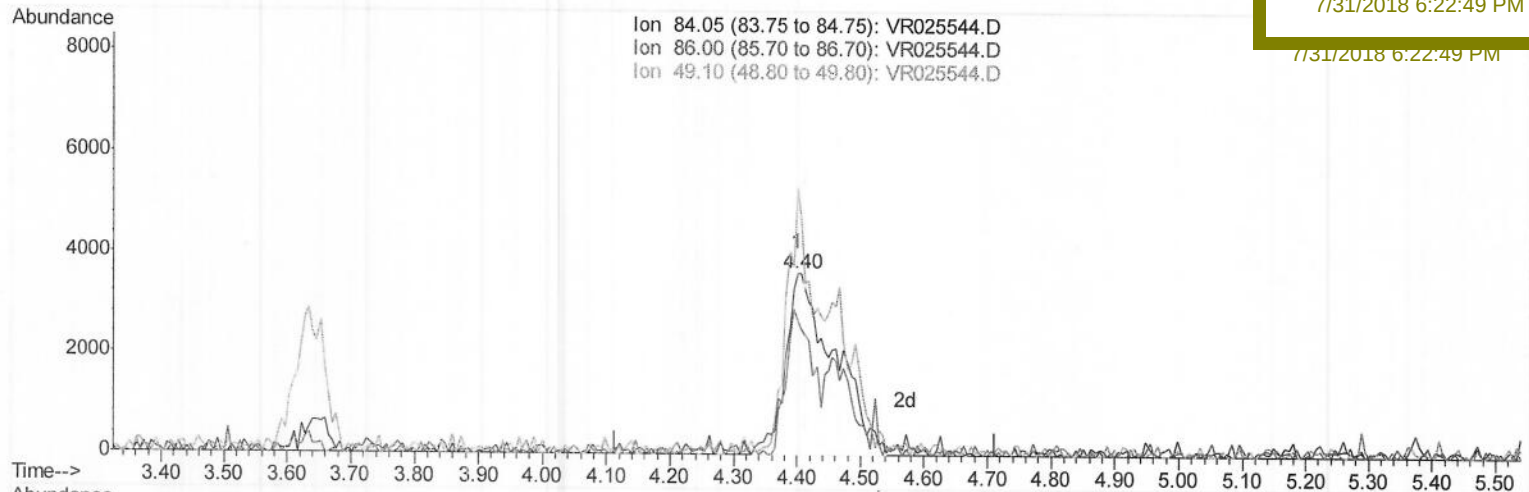

TIC: VR025544.D

(16) Methylene chloride (T)

4.401min (-0.012) 0.50ug/L m 2 MD 08/07/18

response 19292

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	76.48#
49.10	108.80	153.74#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA R\DATA\VR073018\
 Data File : VR025544.D
 Acq On : 30 Jul 2018 17:49
 Operator : SY/MD
 Sample : J4202-02
 Misc : 25mL/MSVOA R/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_R
 Client Sampled :
 BE720

Quant Time: Jul 31 08:38:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jul 30 16:58:41 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 7/31/2018 6:22:49 PM

7/31/2018 6:22:49 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	638981	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	543042	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	204090	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	182651	4.61	ug/L	-0.01
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.20%
7) Chloroethane-d5	2.64	69	133257	4.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.40%
11) 1,1-Dichloroethene-d2	3.63	63	307331	3.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.20%
20) 2-Butanone-d5	6.60	46	150999	46.14	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.28%
24) Chloroform-d	7.20	84	280315	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.20%
26) 1,2-Dichloroethane-d4	7.89	65	103342	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
32) Benzene-d6	7.86	84	653569	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.80%
36) 1,2-Dichloropropane-d6	8.90	67	172523	4.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.20%
41) Toluene-d8	9.97	98	638018	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
43) trans-1,3-Dichloropropene-	10.24	79	39744	4.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.20%
46) 2-Hexanone-d5	10.59	63	151521	48.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.98%
57) 1,1,2,2-Tetrachloroethane-	12.36	84	75862	4.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.80%
64) 1,2-Dichlorobenzene-d4	13.51	152	152367	4.89	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.80%

Target Compounds

					Ovalue
13) Acetone	3.71	43	45803	16.651 ug/L	95
14) Carbon disulfide	3.96	76	31477	0.298 ug/L	96
16) Methylene chloride	4.40	84	19292m	0.501 ug/L	
42) Toluene	10.03	91	64802	0.363 ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD08/07/18