
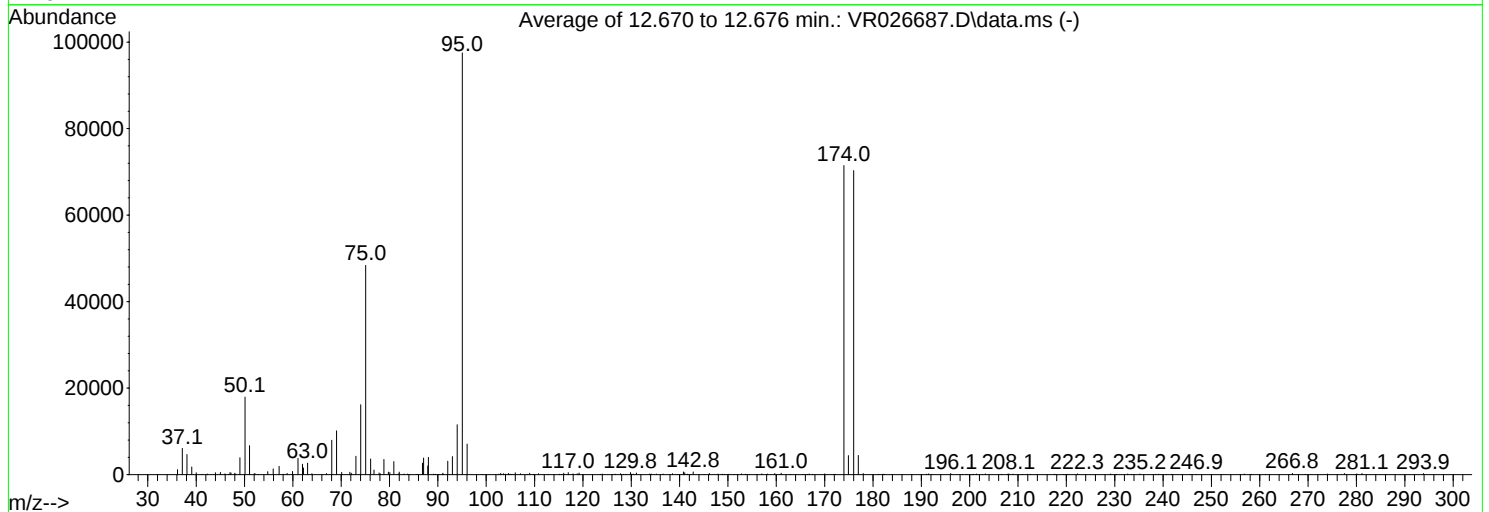


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080425\
Data File : VR026687.D
Acq On : 4 Aug 2025 10:04
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R080425W.M
Title : SW846 8260
Last Update : Tue Aug 05 02:27:49 2025

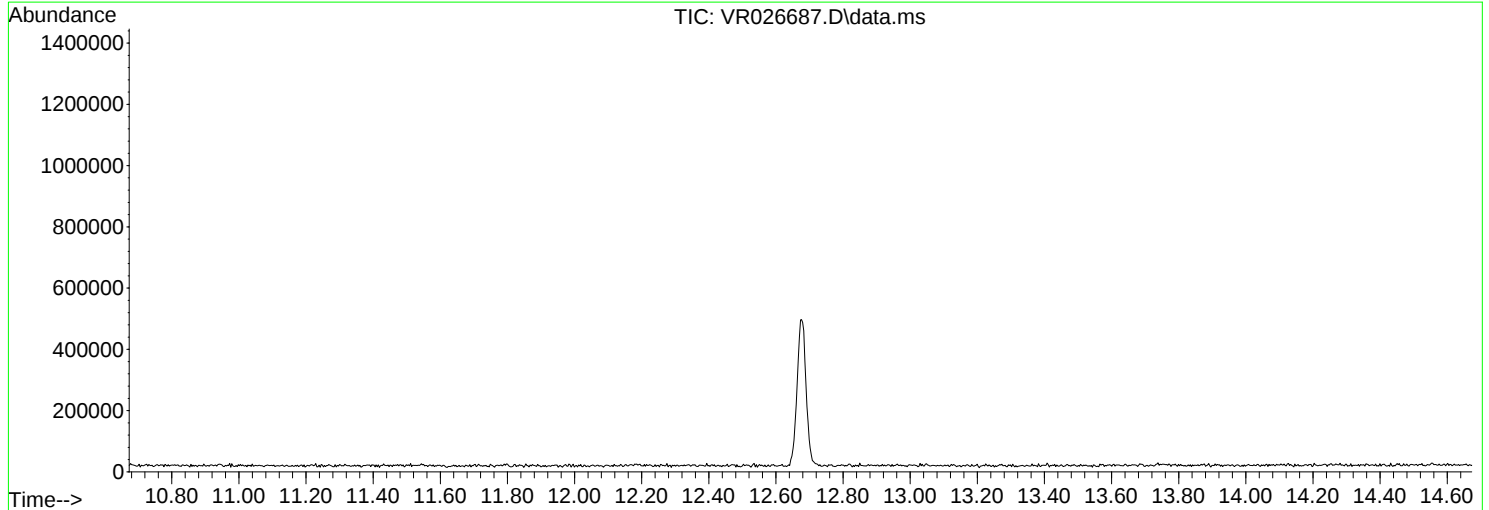

AutoFind: Scans 3767, 3768, 3769; Background Corrected with Scan 3754

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	17939	PASS
75	95	30	60	49.6	48405	PASS
95	95	100	100	100.0	97517	PASS
96	95	5	9	7.2	7053	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.3	71480	PASS
175	174	5	9	6.2	4417	PASS
176	174	95	101	98.3	70280	PASS
177	176	5	9	6.3	4437	PASS