


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080525\
Data File : VR026702.D
Acq On : 5 Aug 2025 8:52
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R080425W.M
Title : SW846 8260
Last Update : Tue Aug 05 02:27:49 2025

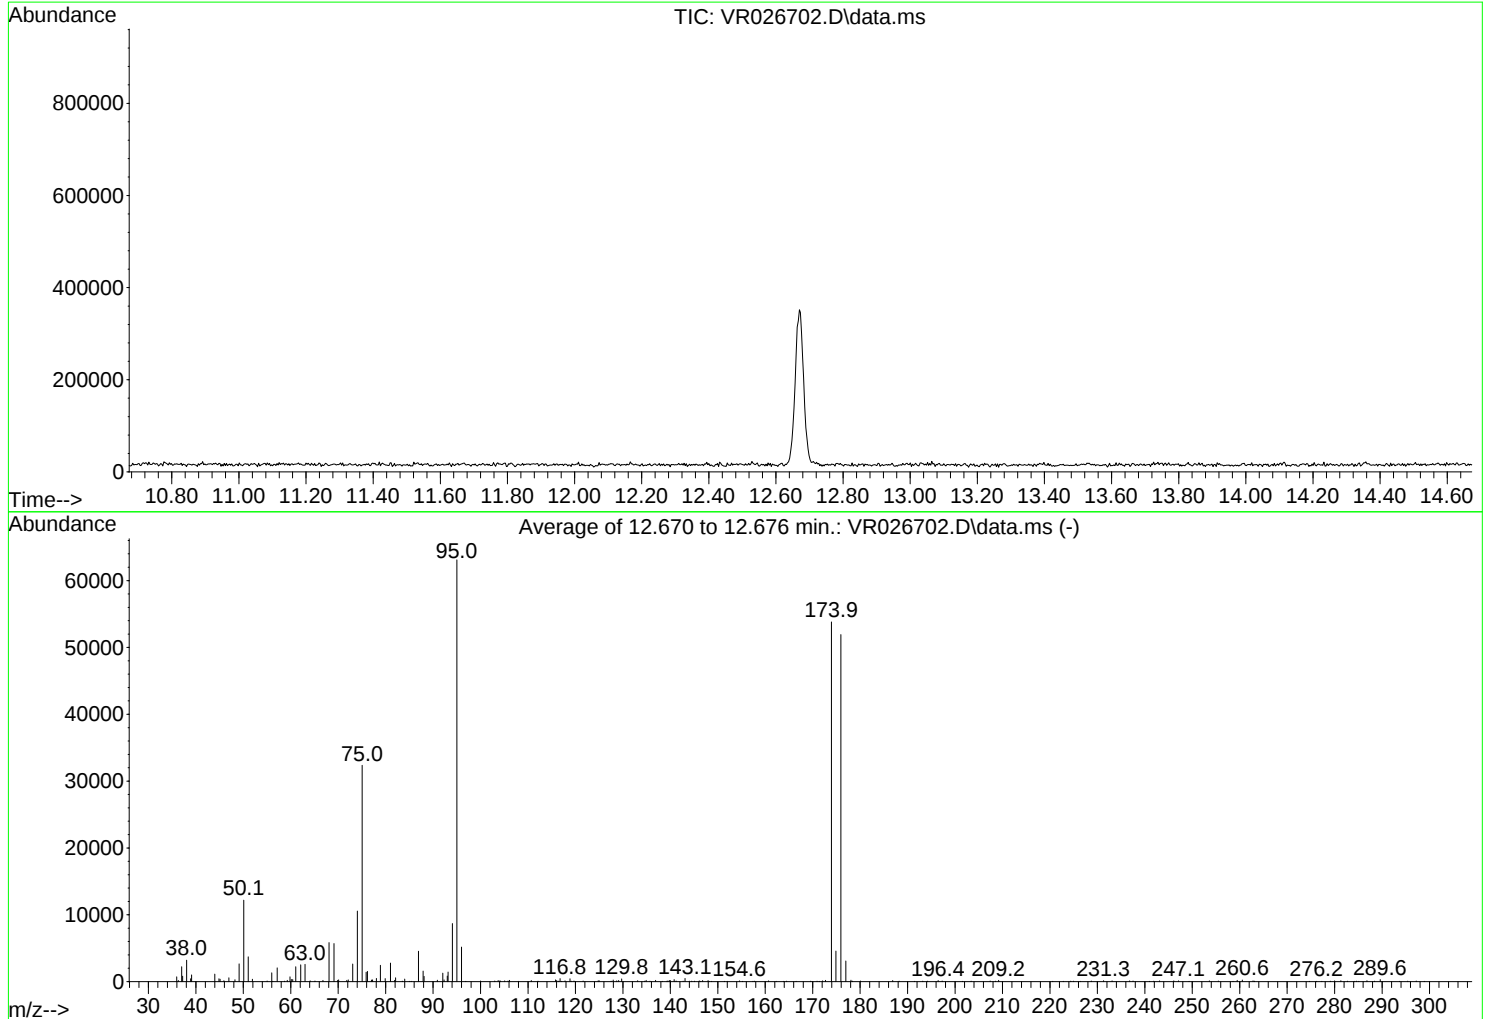

AutoFind: Scans 3767, 3768, 3769; Background Corrected with Scan 3753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	12179	PASS
75	95	30	60	51.3	32357	PASS
95	95	100	100	100.0	63107	PASS
96	95	5	9	8.2	5168	PASS
173	174	0.00	2	0.4	198	PASS
174	95	50	100	85.3	53816	PASS
175	174	5	9	8.5	4565	PASS
176	174	95	101	96.5	51920	PASS
177	176	5	9	6.0	3096	PASS