
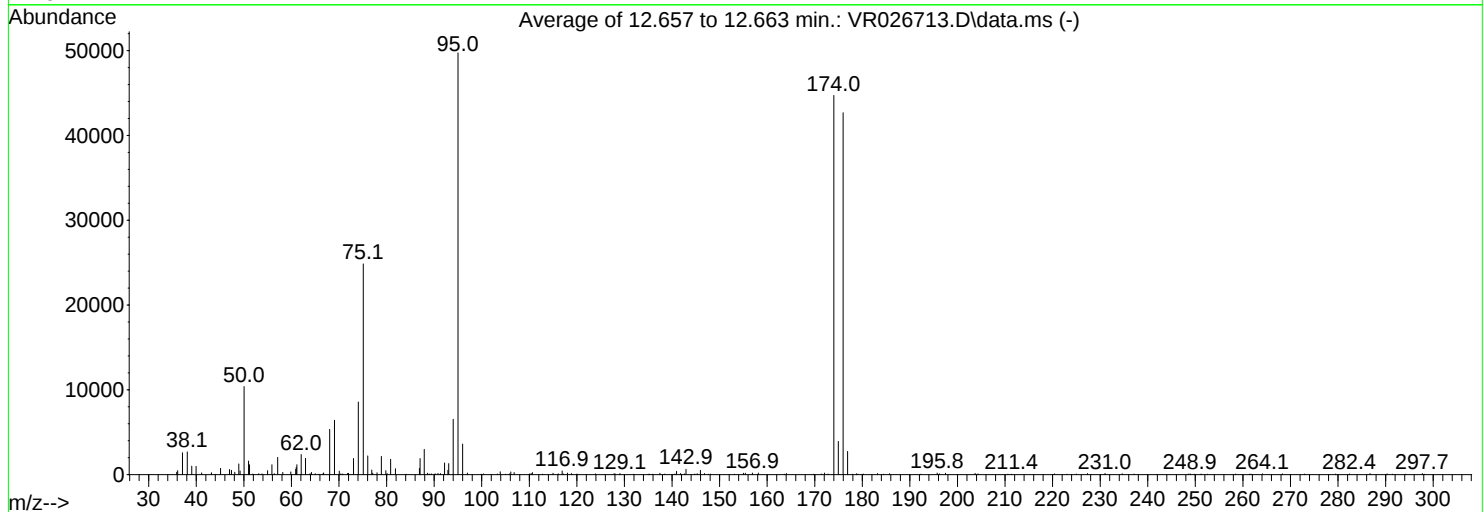


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080625\
Data File : VR026713.D
Acq On : 6 Aug 2025 12:30
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R080425W.M
Title : SW846 8260
Last Update : Tue Aug 05 02:27:49 2025

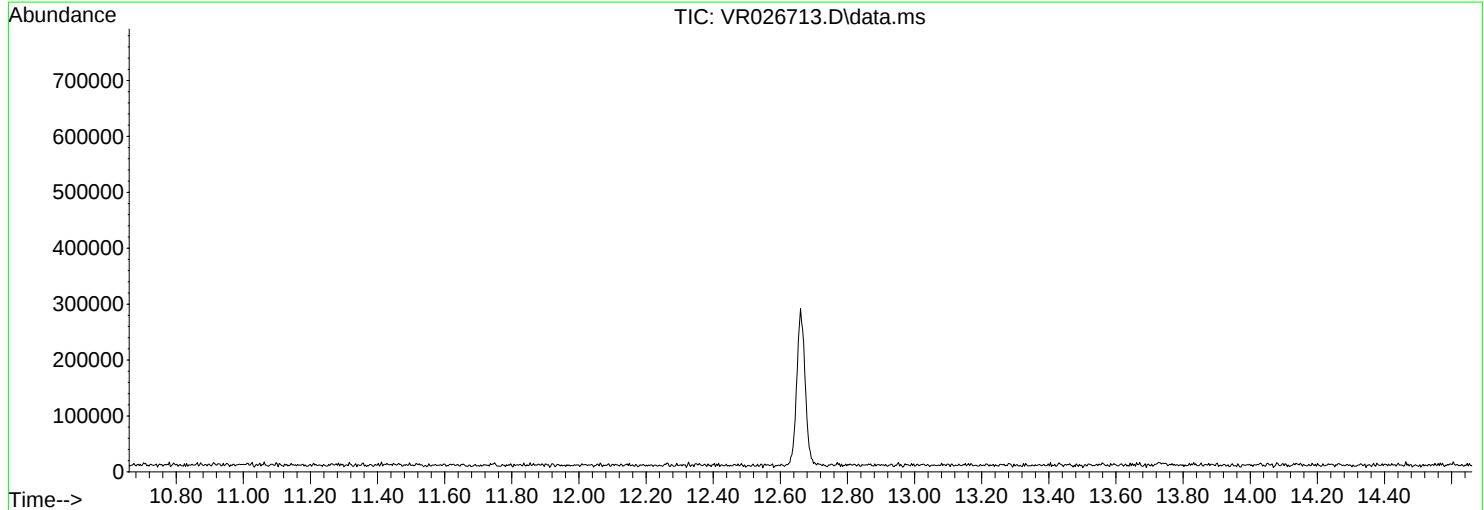

AutoFind: Scans 3763, 3764, 3765; Background Corrected with Scan 3749

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	10404	PASS
75	95	30	60	50.0	24850	PASS
95	95	100	100	100.0	49741	PASS
96	95	5	9	7.3	3613	PASS
173	174	0.00	2	0.2	80	PASS
174	95	50	100	89.9	44712	PASS
175	174	5	9	8.8	3918	PASS
176	174	95	101	95.5	42688	PASS
177	176	5	9	6.4	2728	PASS