

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
 Data File : VR025568.D
 Acq On : 7 Aug 2018 9:37
 Operator : SY/MD
 Sample : VSTDCCC005
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_R
 LabSampleId :
 VSTD00592

Manual Integrations
 APPROVED

MMDadoda
 8/10/2018 11:11:47 AM

Quant Time: Aug 08 01:51:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 23:40:46 2018
 Response via : Initial Calibration

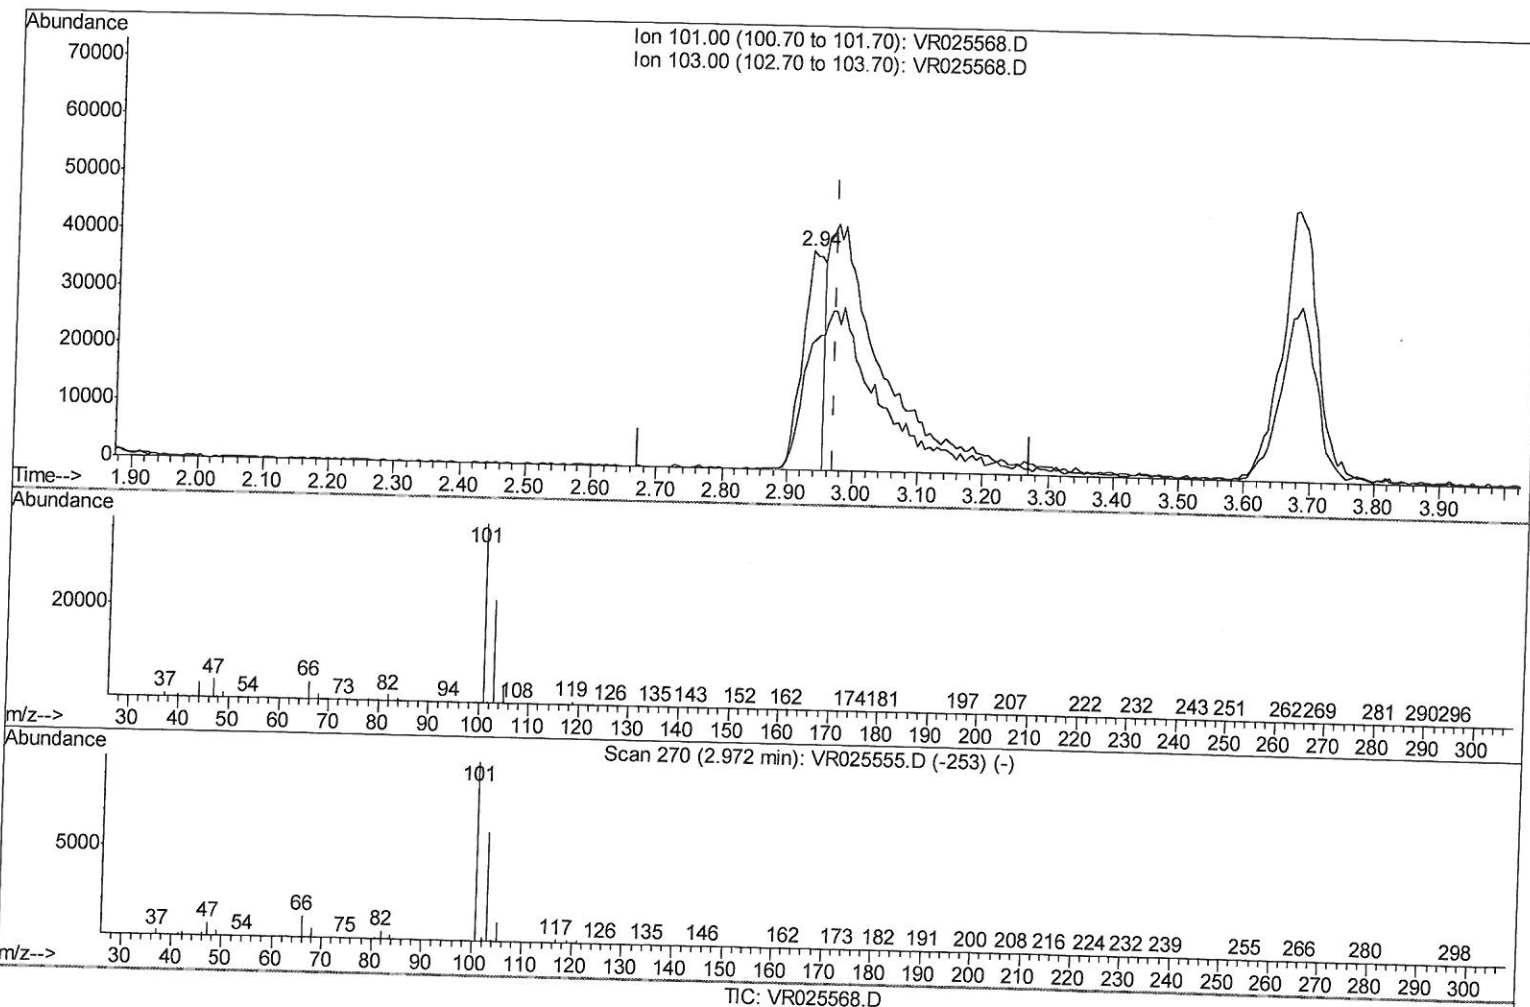

(9) Trichlorofluoromethane (T)

2.935min (-0.037) 1.58ug/L

response 87854

Ion	Exp%	Act%
101.00	100	100
103.00	24.70	225.87#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
Data File : VR025568.D
Acq On : 7 Aug 2018 9:37
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
LabSampled :
VSTD00592

Manual Integrations
APPROVED

MMDadoda
8/10/2018 11:11:47 AM




Quant Time: Aug 08 01:51:04 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Mon Aug 06 23:40:46 2018

Response via : Initial Calibration

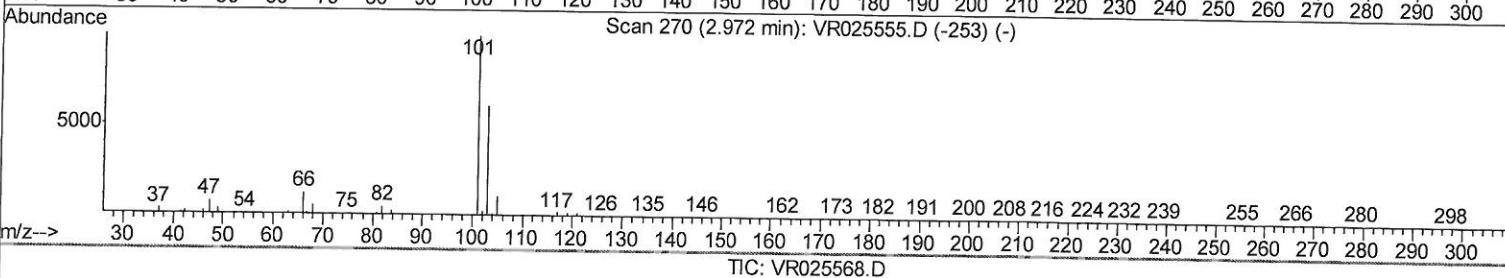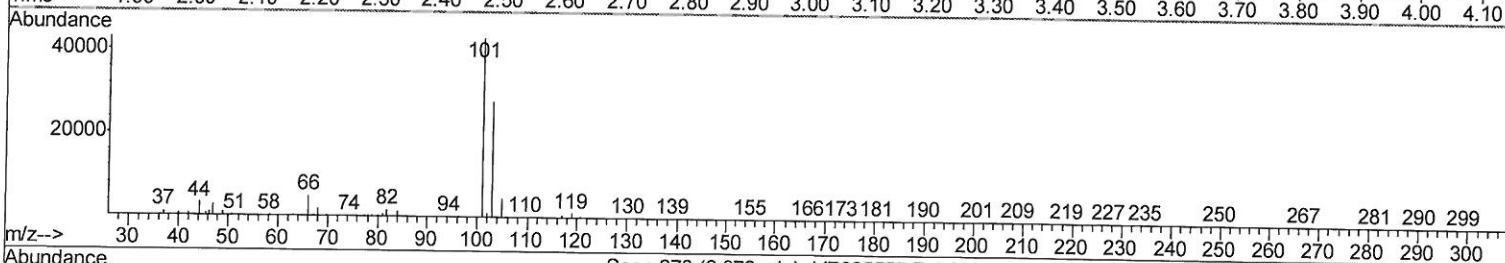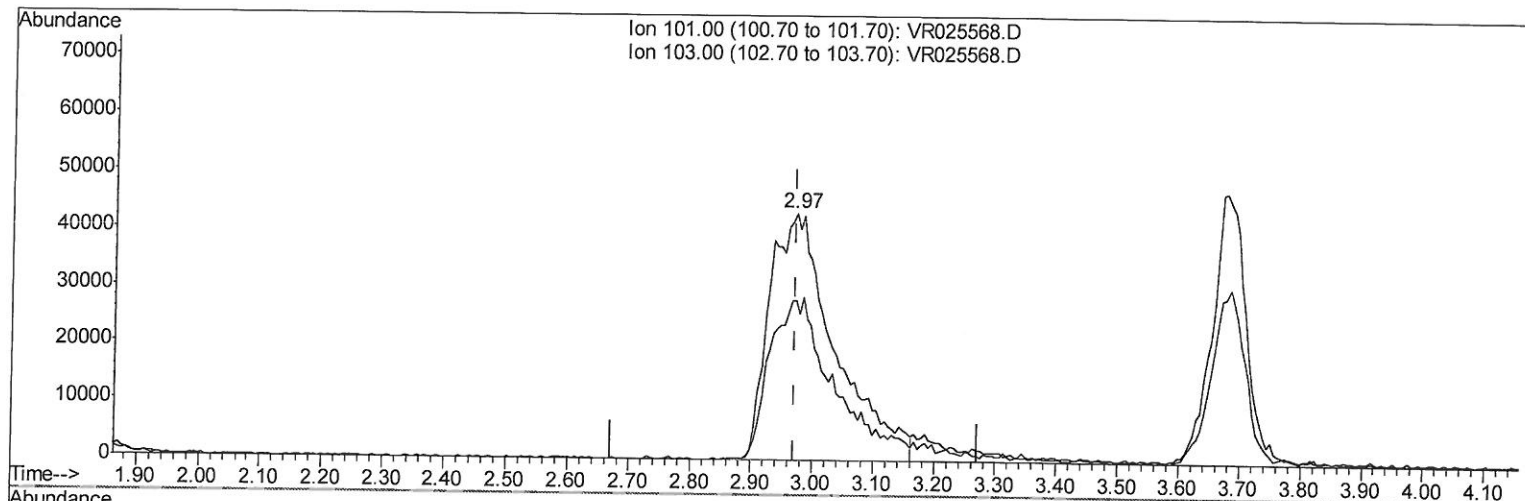

TIC: VR025568.D

(9) Trichlorofluoromethane (T)

2.972min (-0.000) 5.72ug/L m

response 318874

Ion	Exp%	Act%
101.00	100	100
103.00	24.70	62.23#
0.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
Data File : VR025568.D
Acq On : 7 Aug 2018 9:37
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
LabSampleId :
VSTD00592

Manual Integrations
APPROVED

MMDadoda
8/10/2018 11:11:47 AM

Quant Time: Aug 08 01:51:04 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 23:40:46 2018
Response via : Initial Calibration

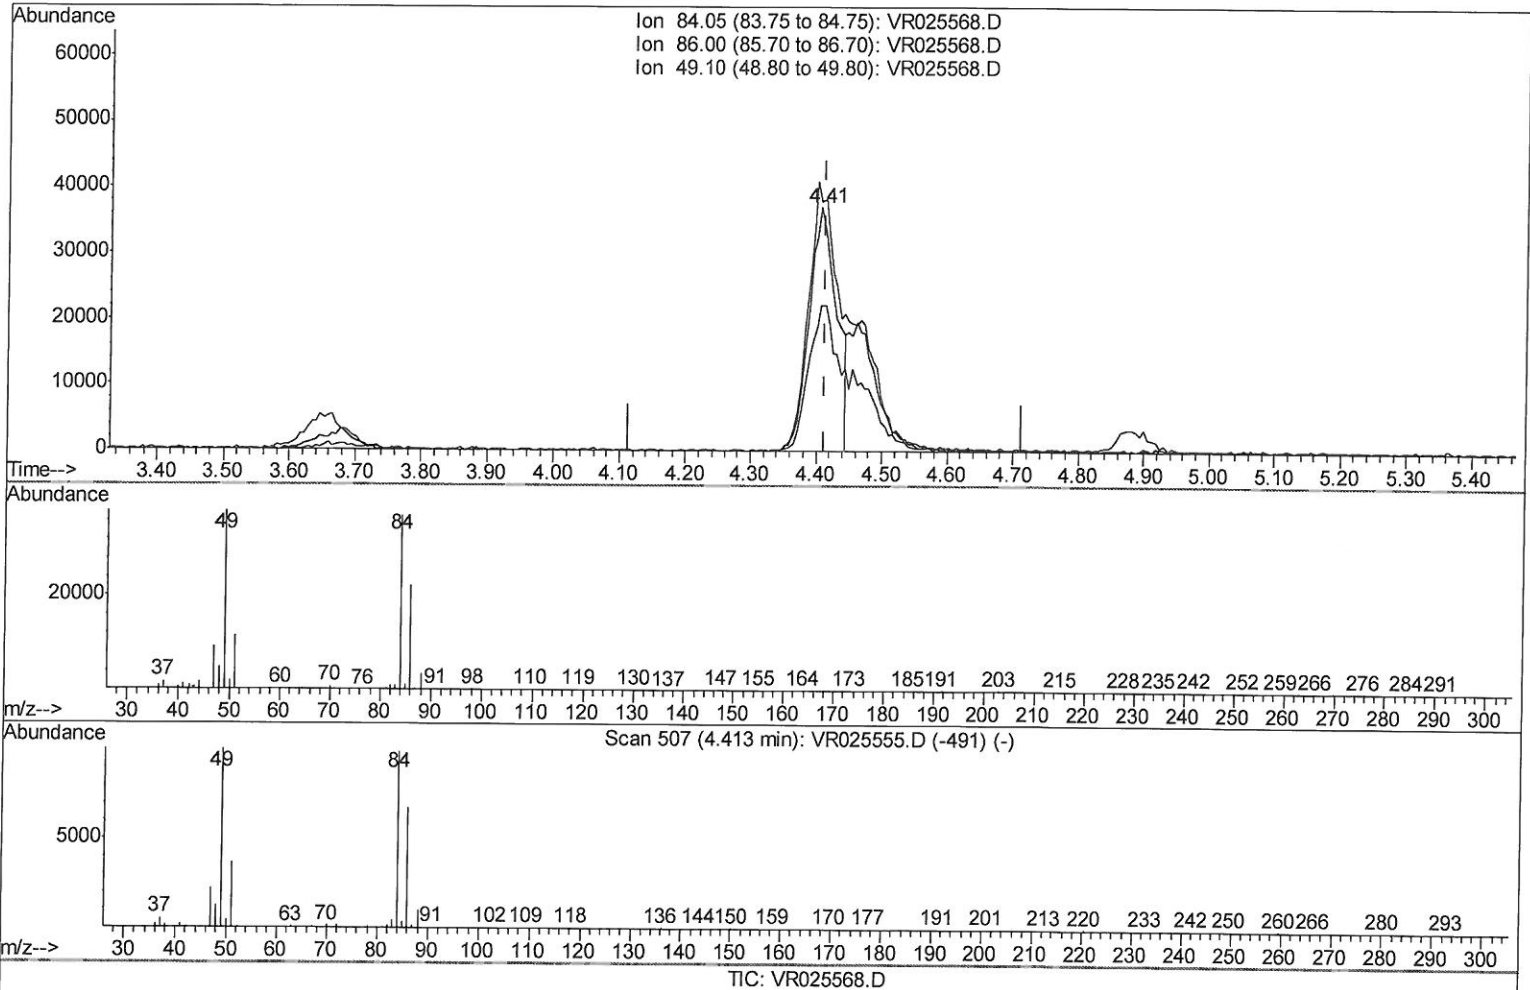

(16) Methylene chloride (T)

4.407min (-0.006) 3.33ug/L

response 108644

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	59.80
49.10	108.80	102.72
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
Data File : VR025568.D
Acq On : 7 Aug 2018 9:37
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
LabSampleId :
VSTD00592

Manual Integrations
APPROVED

MMDadoda
8/10/2018 11:11:47 AM

Quant Time: Aug 08 01:51:04 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 23:40:46 2018
Response via : Initial Calibration

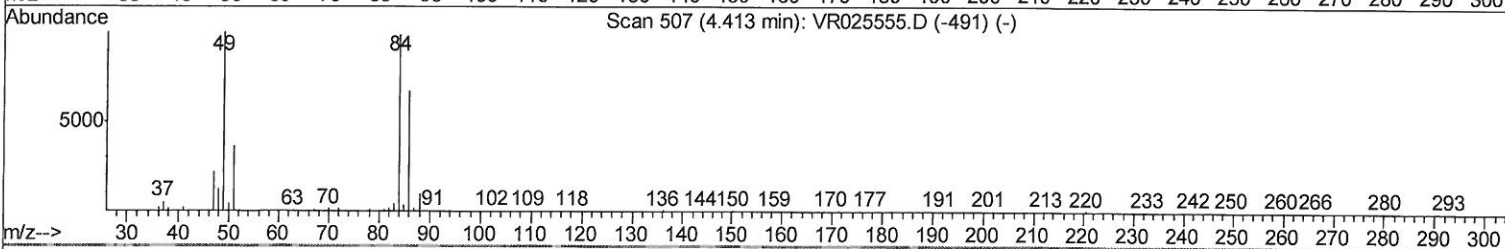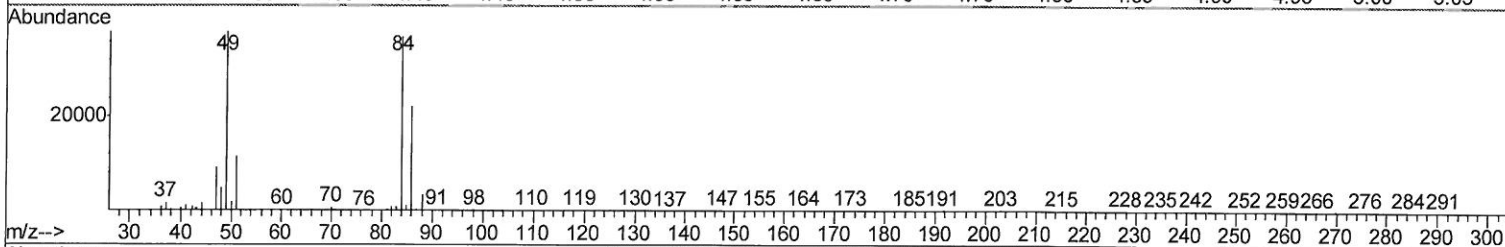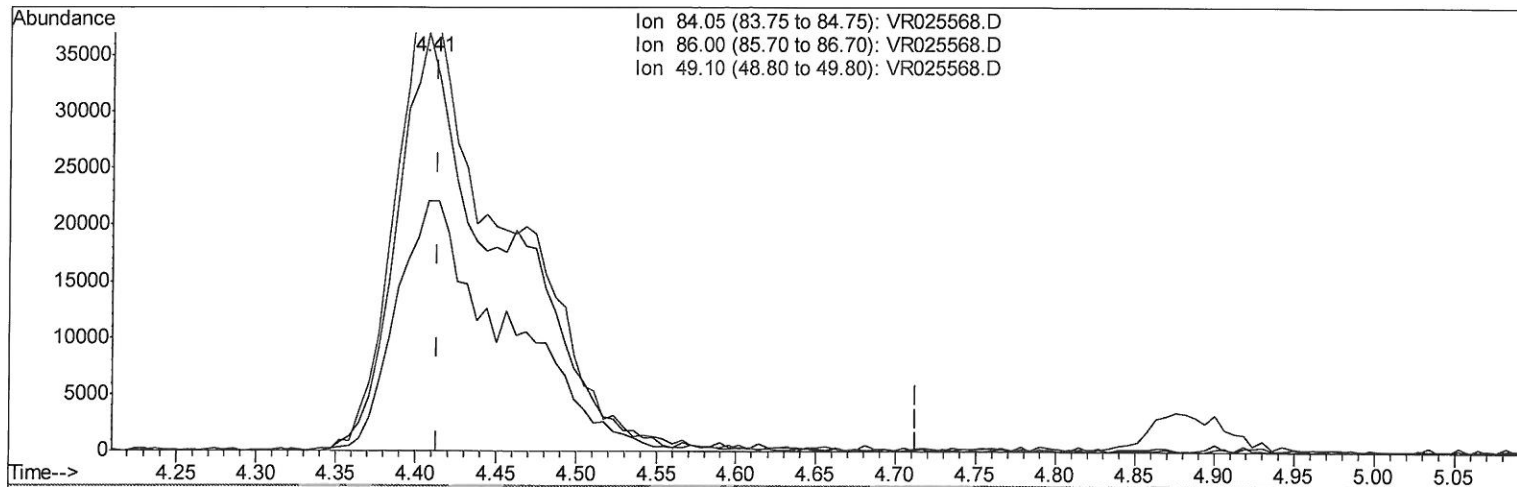

(16) Methylene chloride (T)

4.407min (-0.006) 5.10ug/L m

response 166066

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	59.80
49.10	108.80	102.72
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
 Data File : VR025568.D
 Acq On : 7 Aug 2018 9:37
 Operator : SY/MD
 Sample : VSTDCCC005
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_R
 LabSampleId :
 VSTD00592

Manual Integrations
 APPROVED

MMDadoda
 8/10/2018 11:11:47 AM

Quant Time: Aug 08 01:58:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 23:40:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	540302	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	482997	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	225077	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.14	65	176854	5.28	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	105.60%		
7) Chloroethane-d5	2.64	69	116891	4.43	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	88.60%		
11) 1,1-Dichloroethene-d2	3.64	63	407936	5.28	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	105.60%		
20) 2-Butanone-d5	6.60	46	125843	45.48	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	90.96%		
24) Chloroform-d	7.21	84	287135	5.16	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	103.20%		
26) 1,2-Dichloroethane-d4	7.90	65	100352	5.32	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	106.40%		
32) Benzene-d6	7.86	84	659805	5.09	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	101.80%		
36) 1,2-Dichloropropane-d6	8.90	67	168140	4.94	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	98.80%		
41) Toluene-d8	9.97	98	667867	5.24	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	104.80%		
43) trans-1,3-Dichloropropene-	10.24	79	41559	4.78	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	95.60%		
46) 2-Hexanone-d5	10.59	63	161942	58.26	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	116.52%		
57) 1,1,2,2-Tetrachloroethane-	12.36	84	82095	5.34	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	106.80%		
64) 1,2-Dichlorobenzene-d4	13.51	152	170616	4.96	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	99.20%		

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	1.83	85	155240	5.019 ug/L	97
3) Chloromethane	2.01	50	210372	5.149 ug/L	97
5) Vinyl chloride	2.15	62	196563	4.815 ug/L	90
6) Bromomethane	2.53	94	82885	3.692 ug/L	84
8) Chloroethane	2.67	64	93100	4.106 ug/L	98
9) Trichlorofluoromethane	2.97	101	318874m	5.718 ug/L	
10) 1,1,2-Trichloro-1,2,2-trif	3.68	101	178006	4.940 ug/L	95
12) 1,1-Dichloroethene	3.66	96	199041	5.157 ug/L	90
13) Acetone	3.71	43	110577	47.541 ug/L	99
14) Carbon disulfide	3.96	76	394633	4.414 ug/L	99
15) Methyl Acetate	4.21	43	33292	4.533 ug/L	95
16) Methylene chloride	4.41	84	166066m	5.095 ug/L	
17) Methyl tert-butyl Ether	4.91	73	187183	4.832 ug/L	98
18) trans-1,2-Dichloroethene	4.88	96	191202	5.173 ug/L	91
19) 1,1-Dichloroethane	5.69	63	267939	4.954 ug/L	97
21) 2-Butanone	6.70	43	166497	51.524 ug/L	97
22) cis-1,2-Dichloroethene	6.68	96	177353	5.254 ug/L #	99

8/13/18

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
 Data File : VR025568.D
 Acq On : 7 Aug 2018 9:37
 Operator : SY/MD
 Sample : VSTDCCC005
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_R
 LabSampleId :
 VSTD00592

Manual Integrations
 APPROVED

MMDadoda
 8/10/2018 11:11:47 AM

Quant Time: Aug 08 01:58:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Aug 06 23:40:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
23) Bromochloromethane	7.05	128	61759	5.515	ug/L	91
25) Chloroform	7.23	83	270748	5.057	ug/L	96
27) 1,2-Dichloroethane	8.00	62	112247	5.261	ug/L #	88
29) 1,1,1-Trichloroethane	7.43	97	195000	4.558	ug/L	99
30) Cyclohexane	7.52	56	255340	5.182	ug/L	98
31) Carbon tetrachloride	7.64	117	207878	4.708	ug/L	100
33) Benzene	7.91	78	747741	5.012	ug/L	100
34) Trichloroethene	8.71	95	176484	4.756	ug/L	94
35) Methylcyclohexane	8.96	83	298217	5.344	ug/L	98
37) 1,2-Dichloropropane	8.99	63	151534	4.824	ug/L	98
38) Bromodichloromethane	9.28	83	156459	4.876	ug/L	97
39) cis-1,3-Dichloropropene	9.72	75	175836	5.070	ug/L	96
40) 4-Methyl-2-pentanone	9.86	43	496264	56.069	ug/L	99
42) Toluene	10.03	91	842783	5.304	ug/L	100
44) trans-1,3-Dichloropropene	10.27	75	123895	5.117	ug/L	99
45) 1,1,2-Trichloroethane	10.44	97	79856	5.105	ug/L	97
47) Tetrachloroethene	10.52	164	165429	5.210	ug/L	95
48) 2-Hexanone	10.64	43	342852	57.439	ug/L	99
49) Dibromochloromethane	10.78	129	97434	5.280	ug/L	93
50) 1,2-Dibromoethane	10.89	107	68636	5.259	ug/L #	100
51) Chlorobenzene	11.31	112	506683	5.273	ug/L	97
52) Ethylbenzene	11.39	91	919826	5.324	ug/L	98
53) m,p-Xylene	11.51	106	368411	5.511	ug/L	96
54) o-Xylene	11.83	106	333757	5.438	ug/L	96
55) Styrene	11.85	104	557209	5.699	ug/L	100
56) Isopropylbenzene	12.13	105	889229	5.508	ug/L	99
58) 1,1,2,2-Tetrachloroethane	12.38	83	83304	5.620	ug/L	93
59) 1,2,3-Trichloropropane	12.44	75	52829	5.335	ug/L	97
61) Bromoform	12.01	173	41417	4.620	ug/L	99
62) 1,3-Dichlorobenzene	13.16	146	322830	4.960	ug/L	99
63) 1,4-Dichlorobenzene	13.24	146	361091	5.111	ug/L	95
65) 1,2-Dichlorobenzene	13.53	146	287652	5.144	ug/L	99
66) 1,2-Dibromo-3-chloropropan	14.15	75	7815	4.517	ug/L #	67
67) 1,3,5-Trichlorobenzene	14.29	180	218669	4.943	ug/L	98
68) 1,2,4-trichlorobenzene	14.79	180	142612	5.017	ug/L	98
69) Naphthalene	15.00	128	143882	4.430	ug/L	99
70) 1,2,3-Trichlorobenzene	15.18	180	121866	5.574	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
Data File : VR025568.D
Acq On : 7 Aug 2018 9:37
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_R
LabSampleId :
VSTD00592

Manual Integrations
APPROVED

MMDadoda
8/10/2018 11:11:47 AM

Quant Time: Aug 08 01:58:12 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Aug 06 23:40:46 2018
Response via : Initial Calibration

