
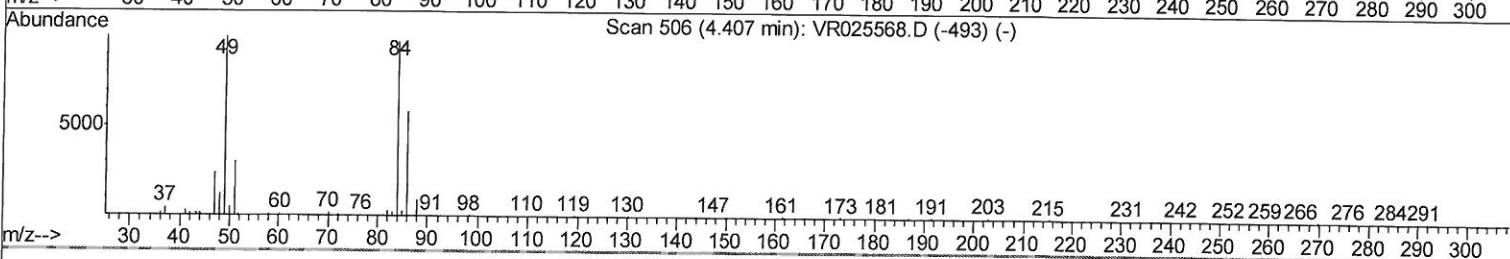
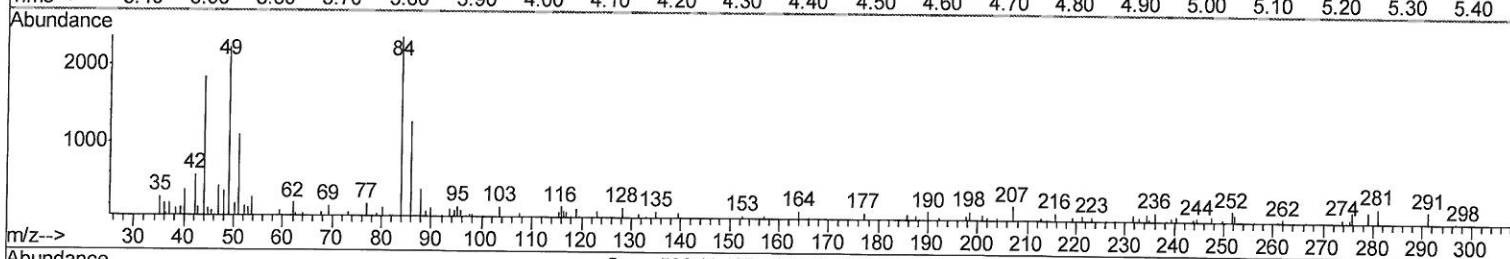


Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
 Data File : VR025570.D
 Acq On : 7 Aug 2018 11:34
 Operator : SY/MD
 Sample : J4243-08
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 08 02:30:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 08 02:00:36 2018
 Response via : Initial Calibration

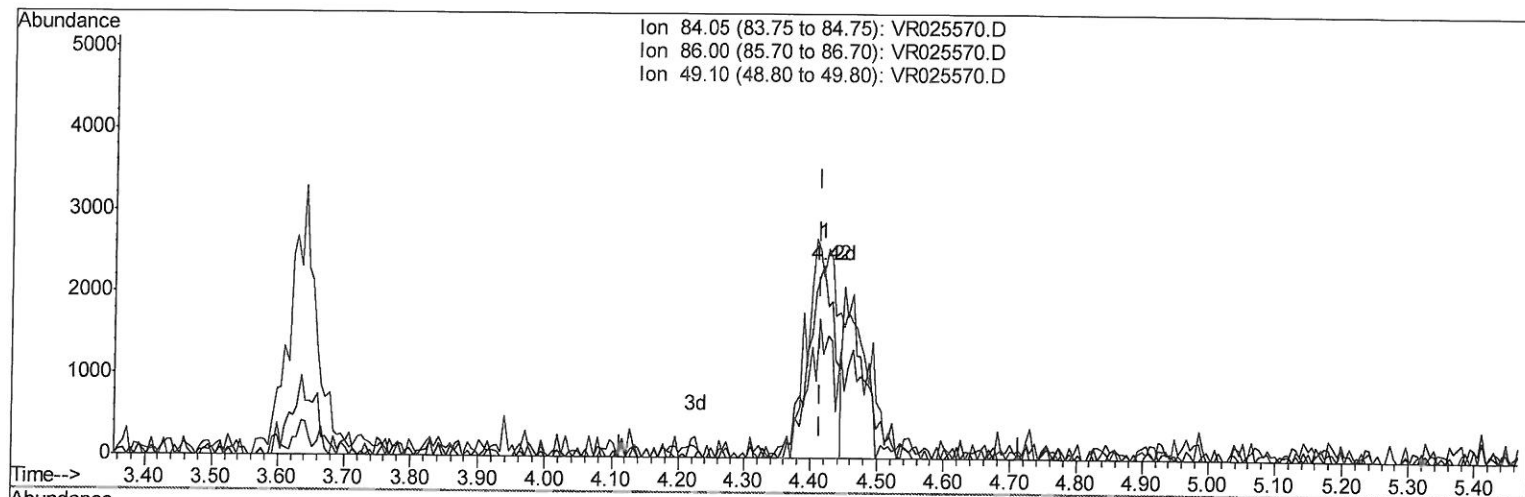

TIC: VR025570.D

(16) Methylene chloride (T)

4.419min (+0.006) 0.20ug/L




response 6521

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	54.12
49.10	108.80	94.10
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
 Data File : VR025570.D
 Acq On : 7 Aug 2018 11:34
 Operator : SY/MD
 Sample : J4243-08
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 08 02:30:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 08 02:00:36 2018
 Response via : Initial Calibration

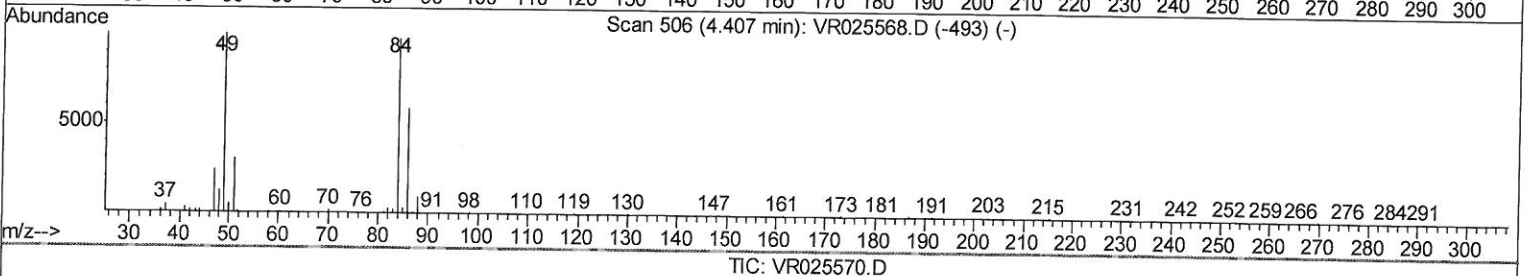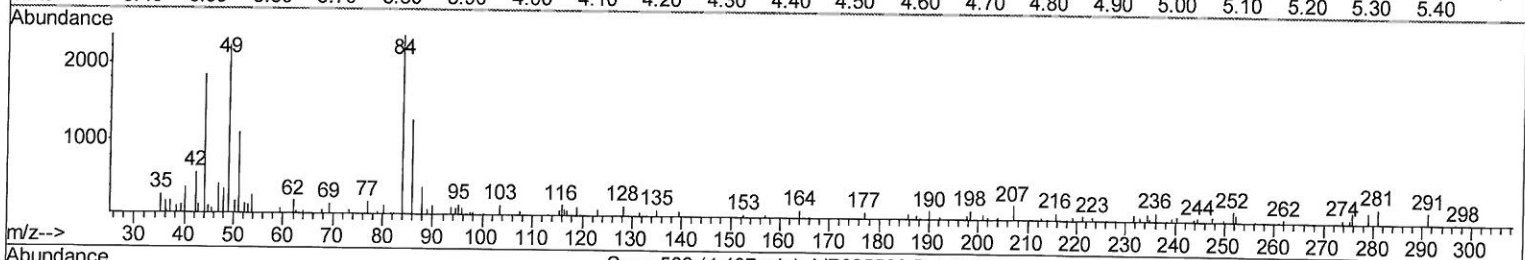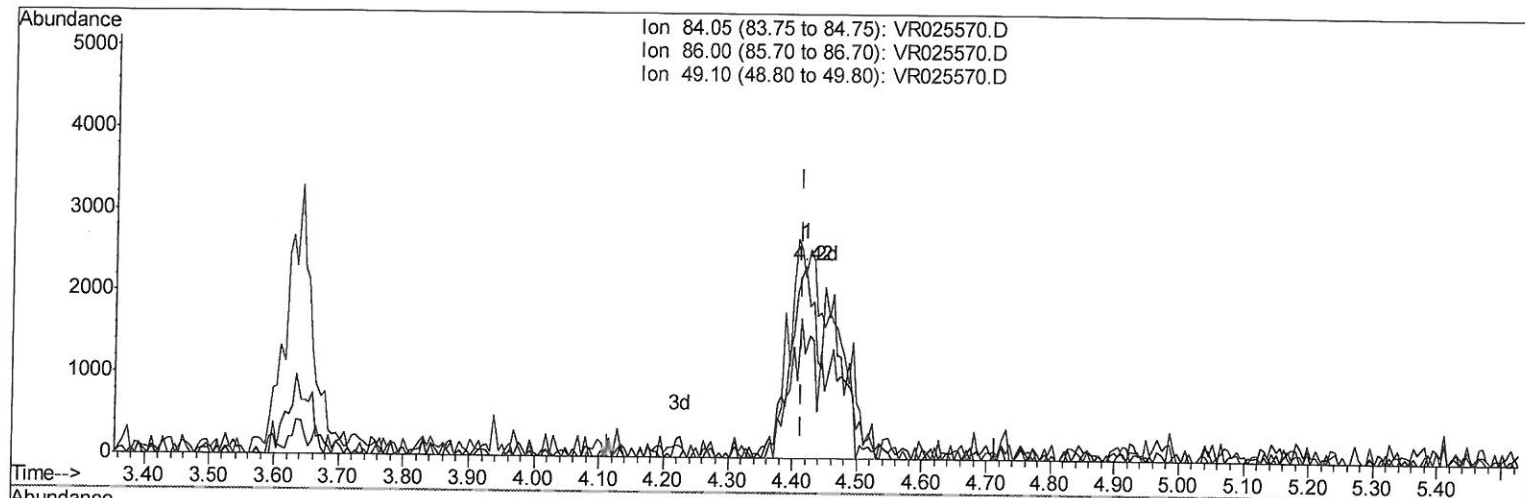

(16) Methylene chloride (T)

4.419min (+0.006) 0.35ug/L m

Handwritten signature: 08/13/18 sy

response 11154

Ion	Exp%	Act%
84.05	100	100
86.00	57.70	54.12
49.10	108.80	94.10
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
 Data File : VR025570.D
 Acq On : 7 Aug 2018 11:34
 Operator : SY/MD
 Sample : J4243-08
 Misc : 25mL/MSVOA_R/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 08 02:34:25 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 08 02:00:36 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.46	114	533583	5.00	ug/L	0.00
28) Chlorobenzene-d5	11.29	117	460863	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.22	152	166614	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.15	65	182533	5.52	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	110.40%		
7) Chloroethane-d5	2.64	69	134578	5.16	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	103.20%		
11) 1,1-Dichloroethene-d2	3.63	63	309006	4.05	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	81.00%		
20) 2-Butanone-d5	6.60	46	133536	48.87	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	97.74%		
24) Chloroform-d	7.21	84	267413	4.87	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.40%		
26) 1,2-Dichloroethane-d4	7.90	65	95501	5.12	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	102.40%		
32) Benzene-d6	7.86	84	612223	4.95	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	99.00%		
36) 1,2-Dichloropropane-d6	8.90	67	160312	4.94	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	98.80%		
41) Toluene-d8	9.97	98	590647	4.85	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.00%		
43) trans-1,3-Dichloropropene-	10.24	79	38483	4.64	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	92.80%		
46) 2-Hexanone-d5	10.59	63	141775	53.46	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	106.92%		
57) 1,1,2,2-Tetrachloroethane-	12.36	84	70135	4.78	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	95.60%		
64) 1,2-Dichlorobenzene-d4	13.51	152	149190	5.86	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	117.20%		

Target Compounds

16) Methylene chloride	4.42	84	11154m)	0.347	ug/L	Qvalue
------------------------	------	----	---------	-------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

08/13/18 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_R\DATA\VR080718\
Data File : VR025570.D
Acq On : 7 Aug 2018 11:34
Operator : SY/MD
Sample : J4243-08
Misc : 25mL/MSVOA_R/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 08 02:34:25 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_R\METHODS\SOMRTR073018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 08 02:00:36 2018
Response via : Initial Calibration

