
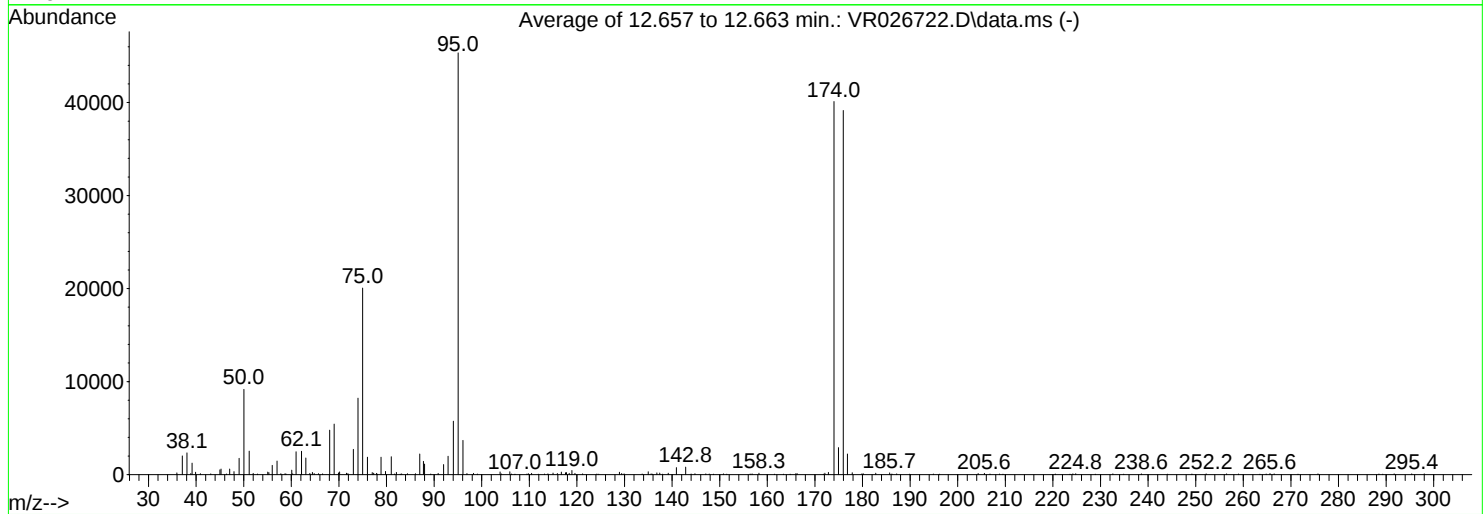


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR080725\
Data File : VR026722.D
Acq On : 7 Aug 2025 9:33
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R080425W.M
Title : SW846 8260
Last Update : Tue Aug 05 02:27:49 2025

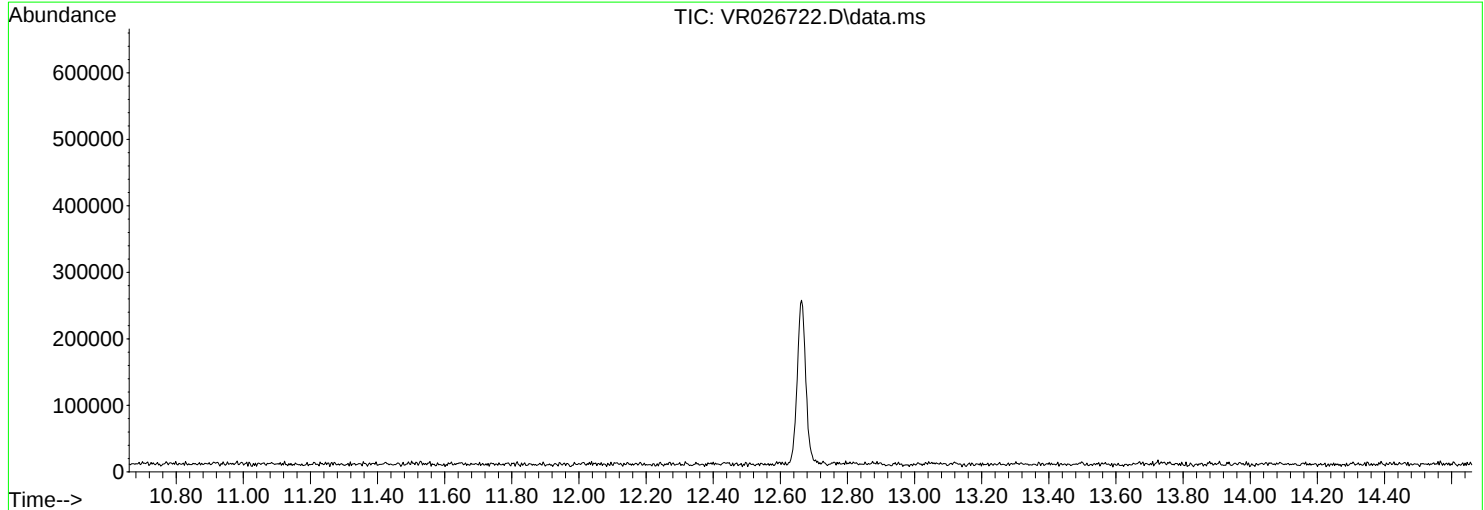

AutoFind: Scans 3763, 3764, 3765; Background Corrected with Scan 3750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	9172	PASS
75	95	30	60	44.2	20053	PASS
95	95	100	100	100.0	45341	PASS
96	95	5	9	8.1	3683	PASS
173	174	0.00	2	0.6	244	PASS
174	95	50	100	88.5	40109	PASS
175	174	5	9	7.3	2908	PASS
176	174	95	101	97.6	39139	PASS
177	176	5	9	5.7	2213	PASS