
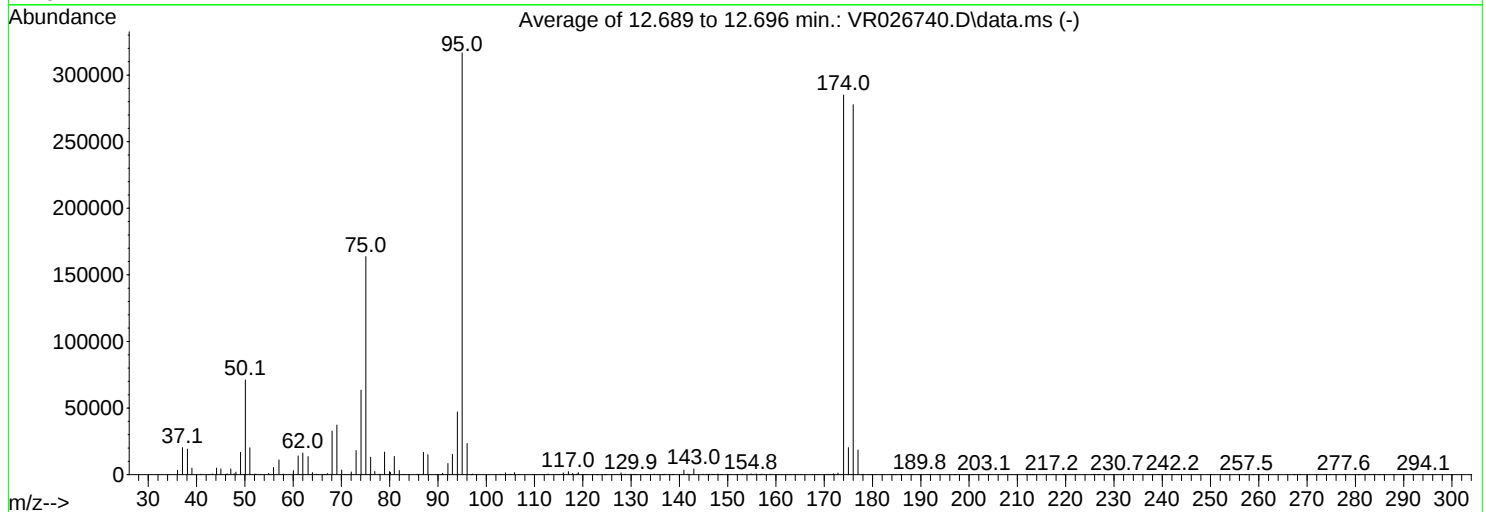


Data Path : Z:\voasrv\HPCHEM1\MSVOA_R\Data\VR082025\
Data File : VR026740.D
Acq On : 20 Aug 2025 13:44
Operator : SY/MD
Sample : BFB
Misc : 5mL/MSVOA_R/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_R
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_R\methods\82R082025W.M
Title : SW846 8260
Last Update : Thu Aug 21 08:59:04 2025

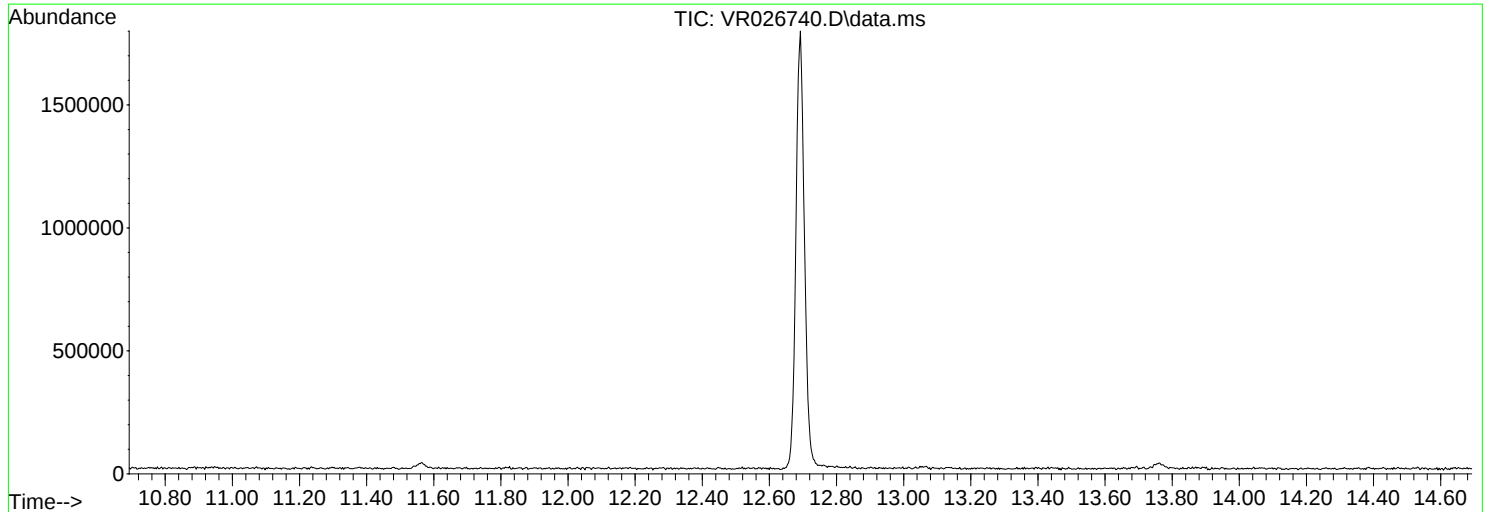

AutoFind: Scans 3773, 3774, 3775; Background Corrected with Scan 3757

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	71131	PASS
75	95	30	60	51.7	163691	PASS
95	95	100	100	100.0	316672	PASS
96	95	5	9	7.4	23451	PASS
173	174	0.00	2	0.4	1233	PASS
174	95	50	100	90.0	285099	PASS
175	174	5	9	7.1	20307	PASS
176	174	95	101	97.4	277717	PASS
177	176	5	9	6.7	18555	PASS